

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029726.D
 Acq On : 19 Dec 2022 16:59
 Operator : SY/MD
 Sample : N6093-06 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP1

Quant Time: Dec 20 00:54:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 20 00:50:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	474998	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	441358	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	229507	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	130249	44.779	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.560%
7) Chloroethane-d5	1.564	69	108449	48.896	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.800%
11) 1,1-Dichloroethene-d2	2.105	63	171563	37.816	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.640%
21) 2-Butanone-d5	3.873	46	166922	94.074	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.070%
24) Chloroform-d	4.339	84	240961	44.022	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.040%
26) 1,2-Dichloroethane-d4	5.024	65	141654	45.312	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.620%
32) Benzene-d6	5.043	84	512772	43.969	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.940%
36) 1,2-Dichloropropane-d6	6.063	67	163332	45.851	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.700%
41) Toluene-d8	7.307	98	458745	41.748	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.500%
43) trans-1,3-Dichloroprop...	7.612	79	66312	36.865	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.720%
47) 2-Hexanone-d5	8.082	63	139269	91.554	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.550%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	227015	44.596	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	11.612	152	189509	43.377	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.760%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	1781	0.717	ug/L	Qvalue # 18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029726.D
Acq On : 19 Dec 2022 16:59
Operator : SY/MD
Sample : N6093-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP1

Quant Time: Dec 20 00:54:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 20 00:50:16 2022
Response via : Initial Calibration

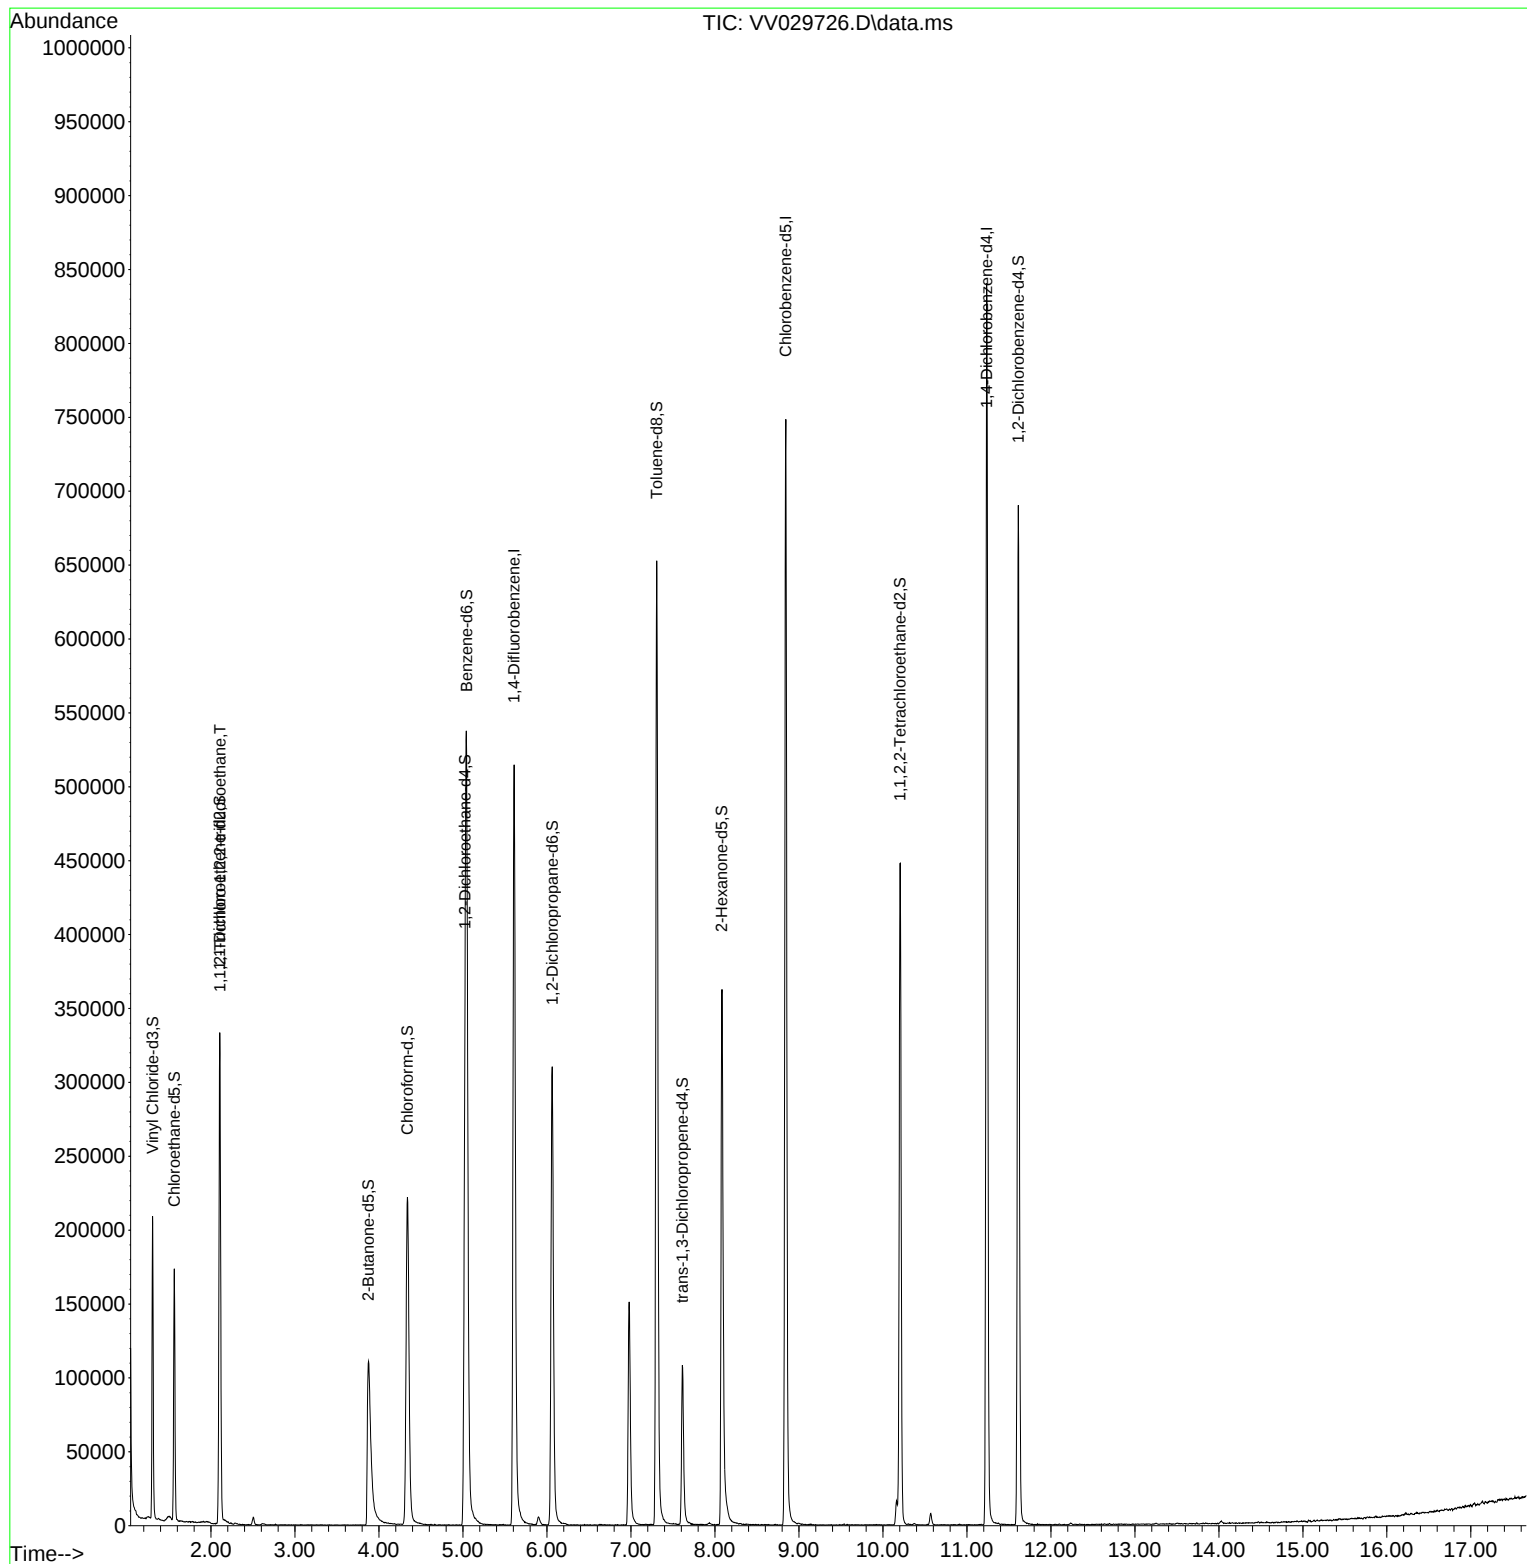

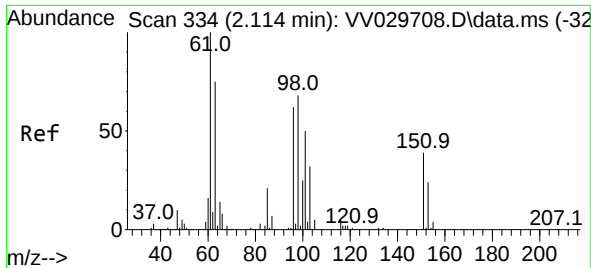

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.717 ug/L
 RT: 2.108 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV029726.D
 Acq: 19 Dec 2022 16:59

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP1

Tgt Ion:101 Resp: 1781
 Ion Ratio Lower Upper
 101 100
 85 0.0 33.6 50.4#
 151 0.0 63.5 95.3#

