

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029727.D
 Acq On : 19 Dec 2022 17:23
 Operator : SY/MD
 Sample : N6093-07 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Quant Time: Dec 20 00:54:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 20 00:50:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	466395	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	438519	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	228953	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	126102	44.153	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.300%
7) Chloroethane-d5	1.564	69	110750	50.854	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	101.700%
11) 1,1-Dichloroethene-d2	2.105	63	172678	38.764	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.520%
21) 2-Butanone-d5	3.876	46	178982	102.731	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.730%
24) Chloroform-d	4.339	84	244849	45.558	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.120%
26) 1,2-Dichloroethane-d4	5.024	65	145612	47.438	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.880%
32) Benzene-d6	5.043	84	521446	45.002	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.000%
36) 1,2-Dichloropropane-d6	6.063	67	166426	47.022	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.040%
41) Toluene-d8	7.307	98	459535	42.091	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.180%
43) trans-1,3-Dichloroprop...	7.612	79	68223	38.172	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.340%
47) 2-Hexanone-d5	8.085	63	142577	94.336	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.340%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	234147	46.295	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	11.612	152	195375	44.827	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.660%
Target Compounds						
15) Methyl Acetate	2.169	43	1897	0.734	ug/L	Qvalue # 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029727.D
Acq On : 19 Dec 2022 17:23
Operator : SY/MD
Sample : N6093-07 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Time: Dec 20 00:54:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 20 00:50:16 2022
Response via : Initial Calibration

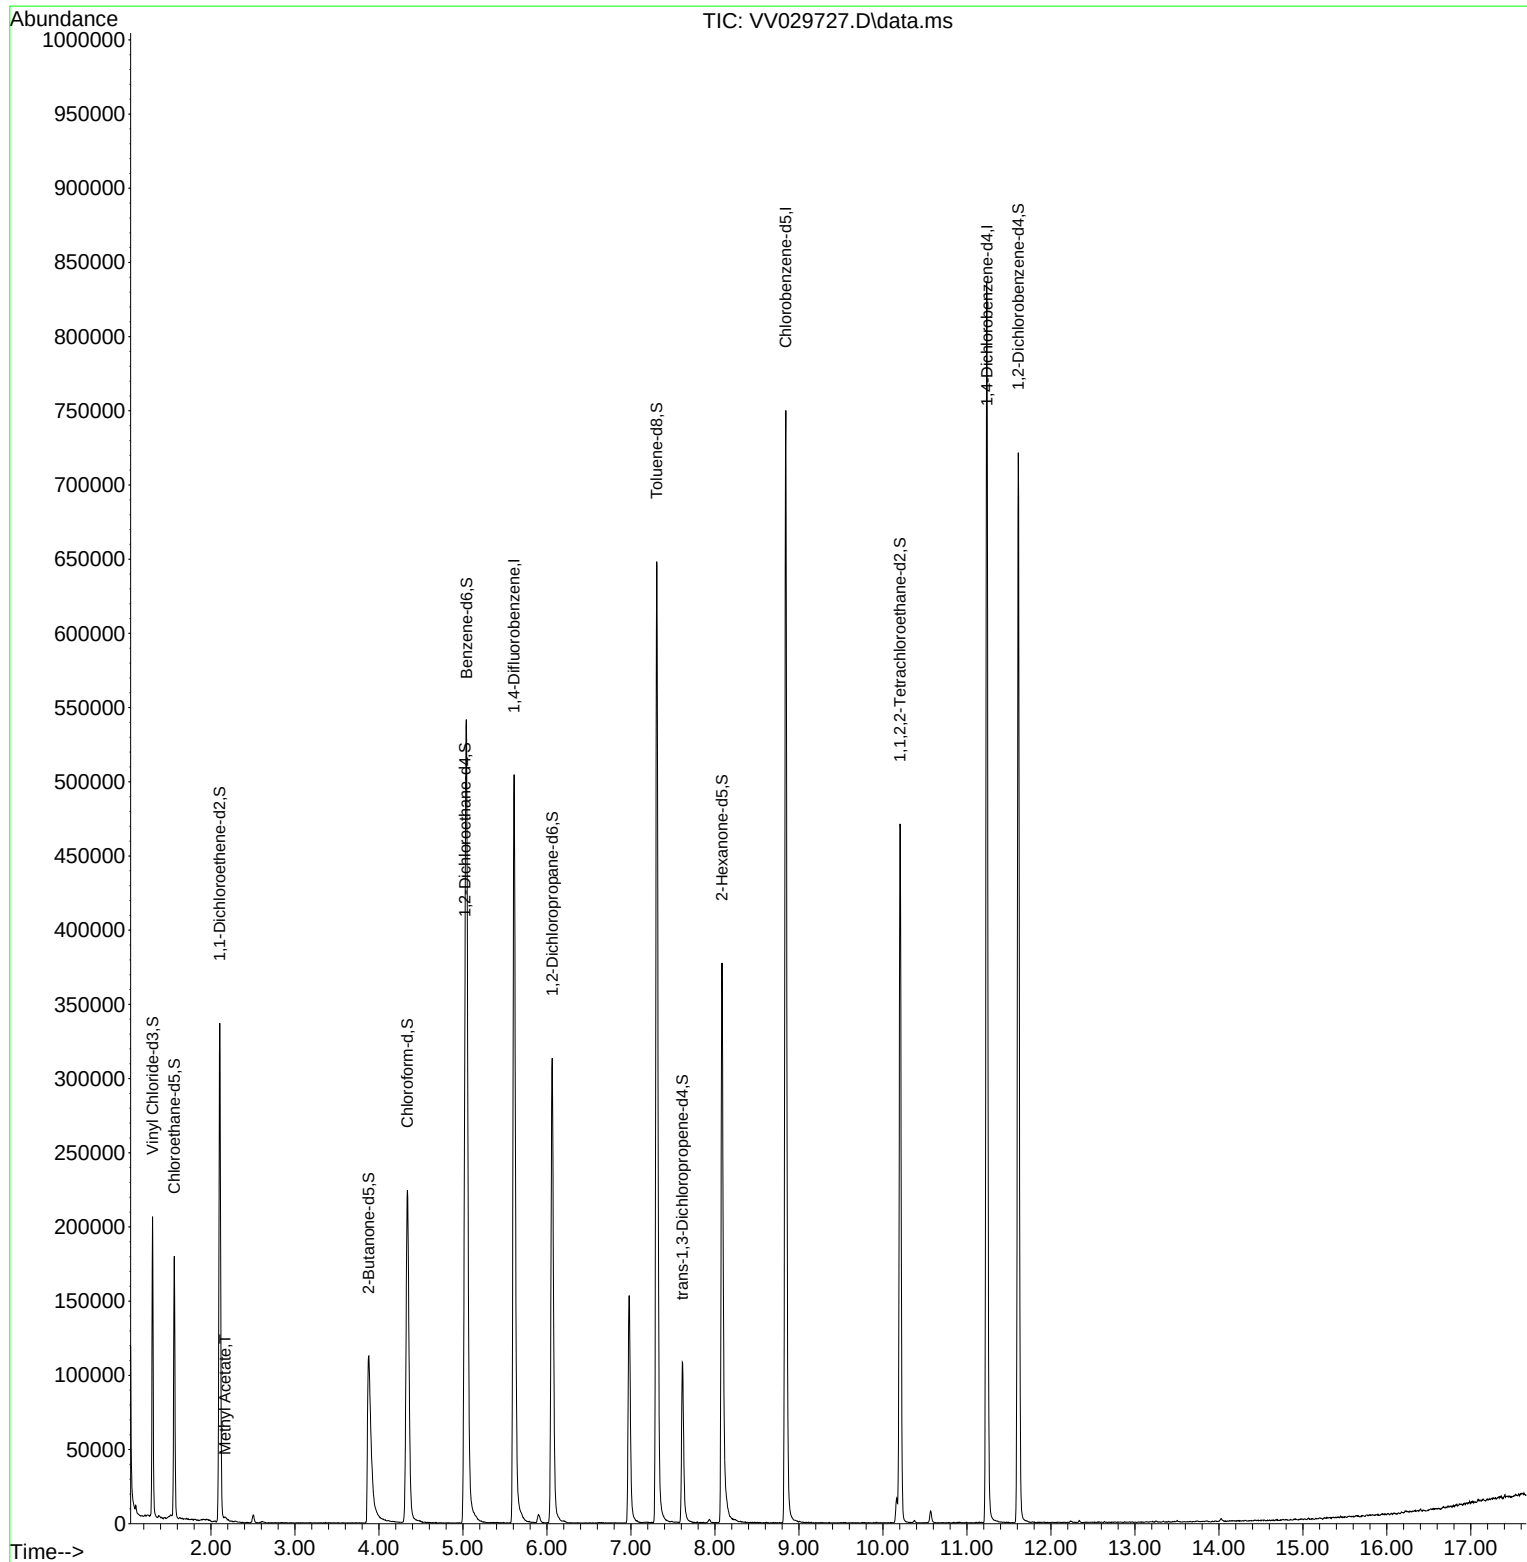

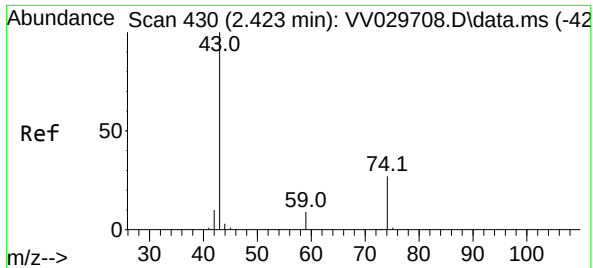

#15
Methyl Acetate
Concen: 0.734 ug/L
RT: 2.169 min Scan# 31
Delta R.T. -0.254 min
Lab File: VV029727.D
Acq: 19 Dec 2022 17:23

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Tgt Ion: 43 Resp: 1897
Ion Ratio Lower Upper
43 100
74 0.0 23.5 35.3#

