

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029733.D
 Acq On : 19 Dec 2022 19:44
 Operator : SY/MD
 Sample : N6093-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Quant Time: Dec 20 00:55:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 20 00:50:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	465329	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	434491	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	223609	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	125094	43.901	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.800%
7) Chloroethane-d5	1.561	69	108425	49.901	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.105	63	169990	38.248	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.500%
21) 2-Butanone-d5	3.873	46	184272	106.010	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.010%
24) Chloroform-d	4.339	84	242077	45.145	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.300%
26) 1,2-Dichloroethane-d4	5.024	65	145609	47.545	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.100%
32) Benzene-d6	5.043	84	518175	45.134	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.260%
36) 1,2-Dichloropropane-d6	6.063	67	164573	46.929	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.860%
41) Toluene-d8	7.307	98	454643	42.029	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.060%
43) trans-1,3-Dichloroprop...	7.612	79	67563	38.154	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.300%
47) 2-Hexanone-d5	8.085	63	147571	98.545	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.550%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	233331	46.561	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.120%
66) 1,2-Dichlorobenzene-d4	11.612	152	189100	44.425	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.840%
Target Compounds						
37) 1,2-Dichloropropane	6.063	63	16132	5.457	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029733.D
Acq On : 19 Dec 2022 19:44
Operator : SY/MD
Sample : N6093-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Time: Dec 20 00:55:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 20 00:50:16 2022
Response via : Initial Calibration

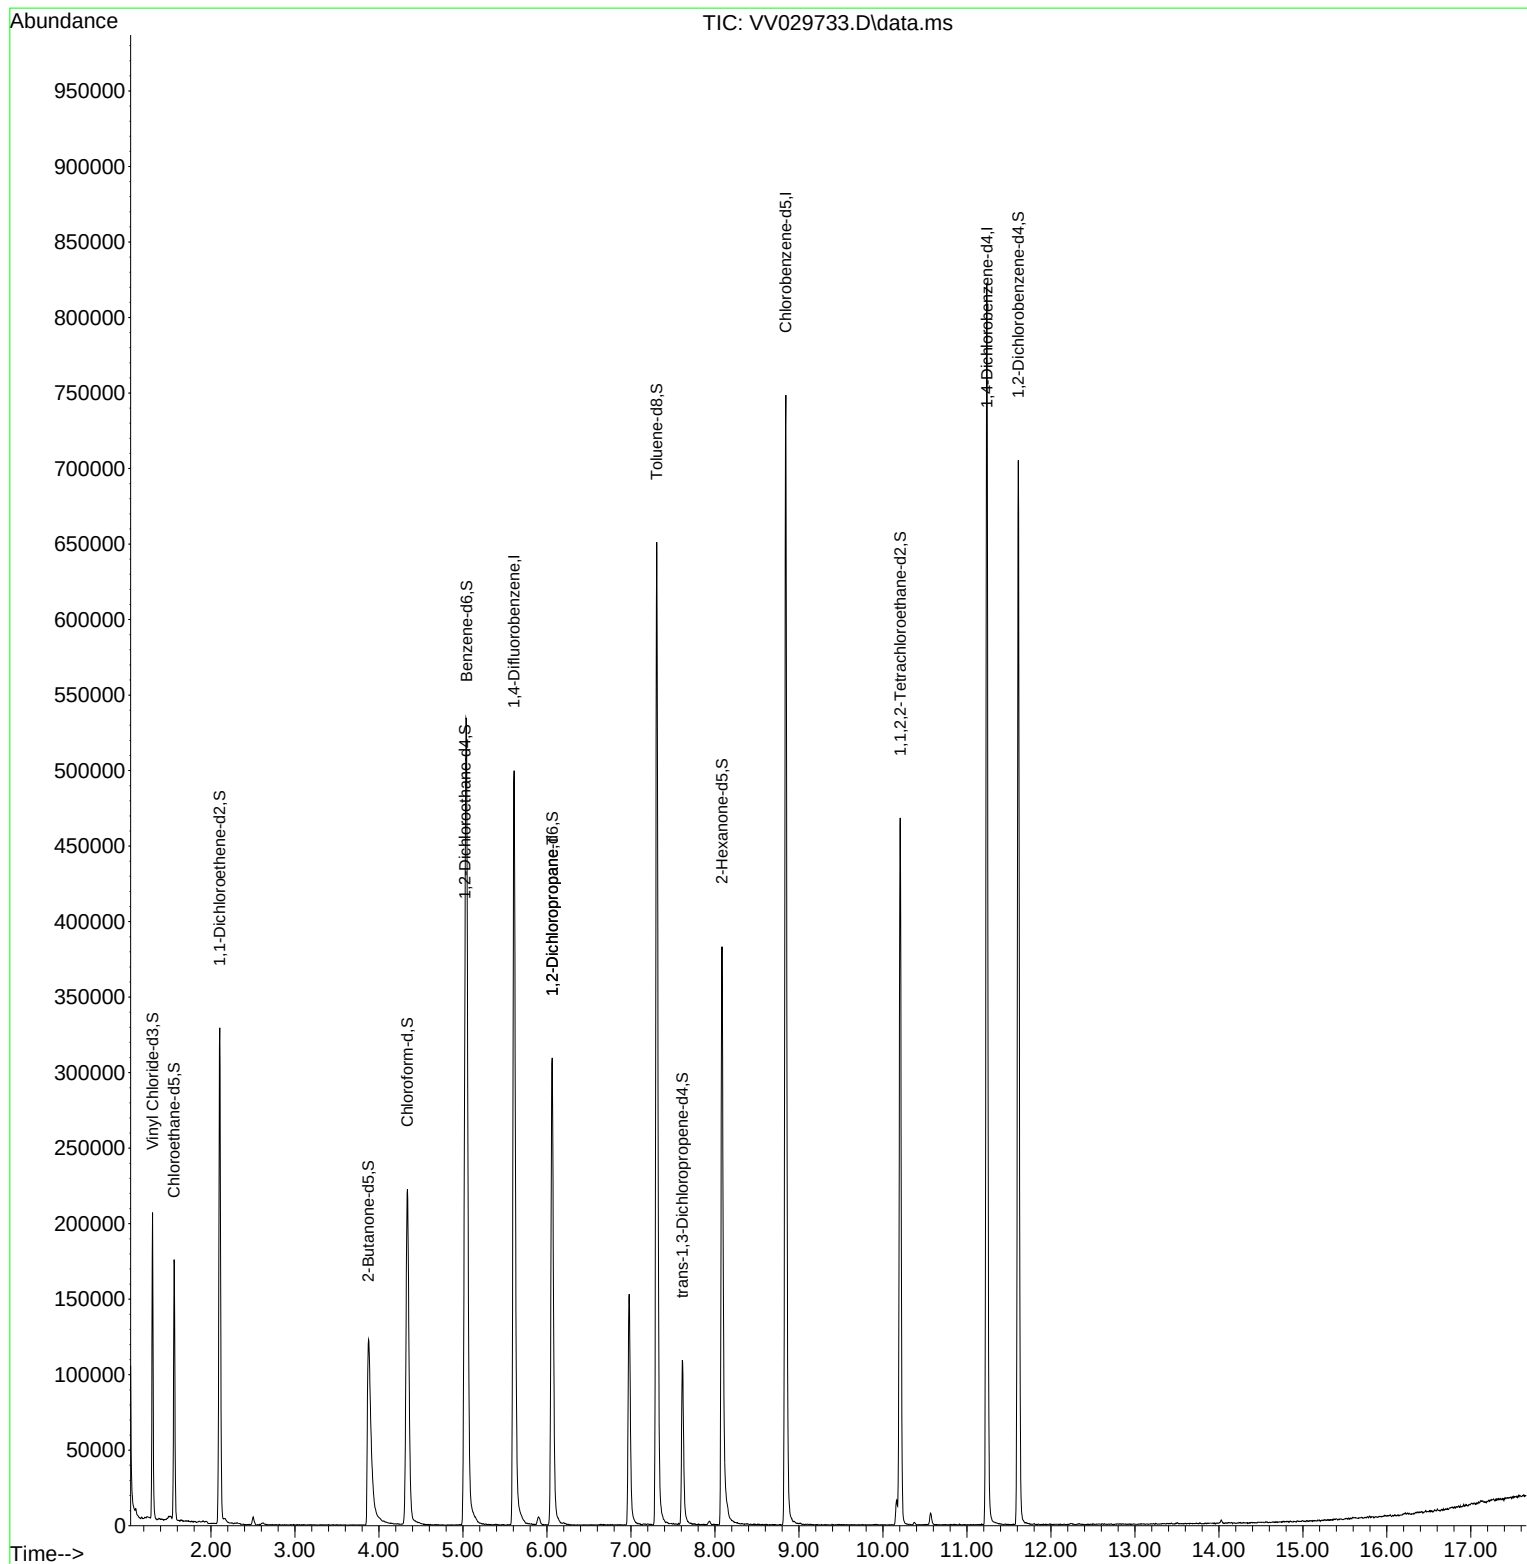

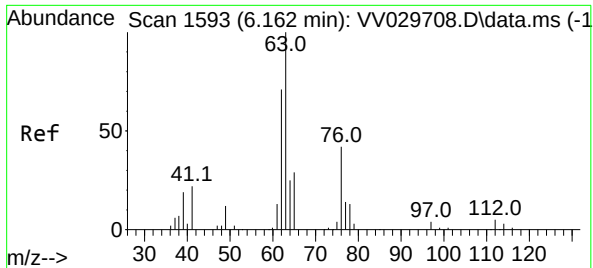

#37
 1,2-Dichloropropane
 Concen: 5.457 ug/L
 RT: 6.063 min Scan# 11
 Delta R.T. -0.100 min
 Lab File: VV029733.D
 Acq: 19 Dec 2022 19:44

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Tgt Ion: 63 Resp: 16132
 Ion Ratio Lower Upper
 63 100
 112 0.2 3.9 5.9#

