

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
 Data File : VV029725.D
 Acq On : 19 Dec 2022 16:36
 Operator : SY/MD
 Sample : N6093-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	203548	205502	14.24%	1.770%
2	1.565	156	163	176	rVB	175654	193409	13.40%	1.666%
3	2.105	320	331	346	rBV	336005	485357	33.63%	4.181%
4	2.507	447	456	465	rVB	5103	7949	0.55%	0.068%
5	2.561	471	473	476	rVB2	304	124	0.01%	0.001%
6	2.719	520	522	524	rBB	240	89	0.01%	0.001%
7	2.764	530	536	539	rBV4	552	556	0.04%	0.005%
8	2.915	580	583	585	rBV	161	107	0.01%	0.001%
9	3.015	612	614	615	rBB	125	26	0.00%	0.000%
10	3.188	663	668	671	rBV2	216	167	0.01%	0.001%
11	3.310	704	706	709	rBV2	216	93	0.01%	0.001%
12	3.407	732	736	737	rBV2	304	179	0.01%	0.002%
13	3.468	752	755	759	rBV2	178	151	0.01%	0.001%
14	3.571	785	787	792	rVB	281	169	0.01%	0.001%
15	3.600	792	796	797	rBV	106	77	0.01%	0.001%
16	3.735	834	838	842	rBV2	249	261	0.02%	0.002%
17	3.796	854	857	858	rBV2	87	58	0.00%	0.000%
18	3.876	871	882	924	rBV2	112913	346810	24.03%	2.988%
19	4.339	1010	1026	1051	rBV	224319	555432	38.48%	4.785%
20	4.632	1113	1117	1118	rBV	193	133	0.01%	0.001%
21	4.667	1124	1128	1129	rBV3	300	151	0.01%	0.001%
22	4.677	1129	1131	1135	rVB3	546	327	0.02%	0.003%
23	4.741	1145	1151	1153	rVB3	266	228	0.02%	0.002%
24	4.764	1156	1158	1161	rVB2	312	152	0.01%	0.001%
25	4.783	1161	1164	1165	rBV	200	81	0.01%	0.001%
26	4.896	1192	1199	1200	rBV	155	186	0.01%	0.002%
27	4.937	1210	1212	1217	rVB	139	92	0.01%	0.001%
28	4.970	1219	1222	1224	rBV2	192	111	0.01%	0.001%
29	5.040	1224	1244	1288	rBV2	546830	1443301	100.00%	12.434%
30	5.439	1365	1368	1370	rBV2	212	154	0.01%	0.001%
31	5.455	1370	1373	1374	rBV	184	103	0.01%	0.001%
32	5.539	1398	1399	1400	rBV	251	72	0.00%	0.001%
33	5.609	1408	1421	1467	rBV	492939	1018521	70.57%	8.775%
34	6.063	1548	1562	1600	rBV	312881	649130	44.98%	5.592%
35	6.317	1640	1641	1642	rVB	189	36	0.00%	0.000%
36	6.330	1642	1645	1647	rBV2	147	118	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029725.D
 Acq On : 19 Dec 2022 16:36
 Operator : SY/MD
 Sample : N6093-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.433	1675	1677	1678	rBV	91	42	0.00%	0.000%
38	6.445	1679	1681	1682	rVV	259	101	0.01%	0.001%
39	6.468	1686	1688	1693	rVB2	104	81	0.01%	0.001%
40	6.490	1693	1695	1698	rBV2	98	53	0.00%	0.000%
41	6.513	1699	1702	1705	rVV	219	136	0.01%	0.001%
42	6.532	1705	1708	1710	rVB	189	114	0.01%	0.001%
43	6.574	1719	1721	1723	rVB2	164	45	0.00%	0.000%
44	6.587	1723	1725	1726	rBV	46	19	0.00%	0.000%
45	6.600	1726	1729	1732	rVB2	118	67	0.00%	0.001%
46	6.632	1732	1739	1741	rBV3	317	362	0.03%	0.003%
47	6.645	1741	1743	1748	rVB3	294	214	0.01%	0.002%
48	6.699	1758	1760	1761	rBV3	140	58	0.00%	0.000%
49	6.712	1761	1764	1766	rBV	265	182	0.01%	0.002%
50	6.748	1772	1775	1778	rVB2	127	89	0.01%	0.001%
51	6.764	1778	1780	1781	rBV	83	39	0.00%	0.000%
52	6.799	1789	1791	1795	rVB3	235	172	0.01%	0.001%
53	6.828	1795	1800	1806	rBV	127	134	0.01%	0.001%
54	6.873	1810	1814	1817	rVB	385	222	0.02%	0.002%
55	6.896	1817	1821	1823	rBV	211	154	0.01%	0.001%
56	6.928	1829	1831	1832	rBV	131	36	0.00%	0.000%
57	6.979	1834	1847	1873	rBV	157103	288959	20.02%	2.489%
58	7.130	1892	1894	1898	rBV3	397	239	0.02%	0.002%
59	7.236	1922	1927	1929	rBV2	519	500	0.03%	0.004%
60	7.262	1933	1935	1936	rBV	253	117	0.01%	0.001%
61	7.310	1937	1950	1980	rBV	666812	1179850	81.75%	10.165%
62	7.616	2034	2045	2067	rBV	109190	195974	13.58%	1.688%
63	7.822	2108	2109	2111	rBV	373	198	0.01%	0.002%
64	7.899	2129	2133	2134	rBV2	252	163	0.01%	0.001%
65	8.085	2180	2191	2226	rBV	368861	692781	48.00%	5.968%
66	8.381	2280	2283	2286	rBV2	399	350	0.02%	0.003%
67	8.600	2349	2351	2353	rBV	132	53	0.00%	0.000%
68	8.622	2353	2358	2359	rBV	246	207	0.01%	0.002%
69	8.661	2368	2370	2372	rBV	305	131	0.01%	0.001%
70	8.699	2379	2382	2389	rVB2	414	214	0.01%	0.002%
71	8.731	2389	2392	2396	rVB2	312	237	0.02%	0.002%
72	8.757	2396	2400	2404	rBV3	343	293	0.02%	0.003%
73	8.844	2415	2427	2454	rBV	732555	1203140	83.36%	10.365%
74	9.072	2496	2498	2501	rBV2	268	106	0.01%	0.001%
75	9.227	2542	2546	2548	rBV2	207	170	0.01%	0.001%
76	9.310	2570	2572	2573	rBV	178	71	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
 Data File : VV029725.D
 Acq On : 19 Dec 2022 16:36
 Operator : SY/MD
 Sample : N6093-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.487	2622	2627	2628	rBV2	215	182	0.01%	0.002%
78	9.603	2661	2663	2664	rBV2	263	97	0.01%	0.001%
79	9.651	2675	2678	2681	rVB2	295	169	0.01%	0.001%
80	9.722	2699	2700	2703	rVB2	138	49	0.00%	0.000%
81	9.744	2705	2707	2708	rVV	164	47	0.00%	0.000%
82	9.860	2742	2743	2744	rBV	131	39	0.00%	0.000%
83	9.963	2772	2775	2778	rBV	310	189	0.01%	0.002%
84	10.005	2786	2788	2790	rVB	182	54	0.00%	0.000%
85	10.162	2828	2837	2841	rBV2	16658	23695	1.64%	0.204%
86	10.207	2841	2851	2867	rVB	460128	729847	50.57%	6.288%
87	10.365	2895	2900	2903	rBV3	919	947	0.07%	0.008%
88	10.535	2946	2953	2955	rBV3	715	937	0.06%	0.008%
89	10.567	2955	2963	2977	rVB2	7945	13222	0.92%	0.114%
90	11.066	3116	3118	3119	rBV	223	74	0.01%	0.001%
91	11.175	3147	3152	3154	rBV2	826	719	0.05%	0.006%
92	11.239	3159	3172	3193	rBV	812938	1261925	87.43%	10.872%
93	11.468	3240	3243	3247	rBV2	650	413	0.03%	0.004%
94	11.612	3275	3288	3311	rBV	702201	1098080	76.08%	9.460%
95	11.876	3369	3370	3371	rVB	218	42	0.00%	0.000%
96	11.889	3371	3374	3376	rBV2	231	123	0.01%	0.001%
97	12.153	3453	3456	3459	rVB	387	214	0.01%	0.002%
98	12.169	3459	3461	3465	rBV	222	211	0.01%	0.002%
99	12.365	3520	3522	3526	rBV	414	359	0.02%	0.003%
100	12.825	3662	3665	3667	rBV	406	306	0.02%	0.003%


Sum of corrected areas: 11607425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029725.D
Acq On : 19 Dec 2022 16:36
Operator : SY/MD
Sample : N6093-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

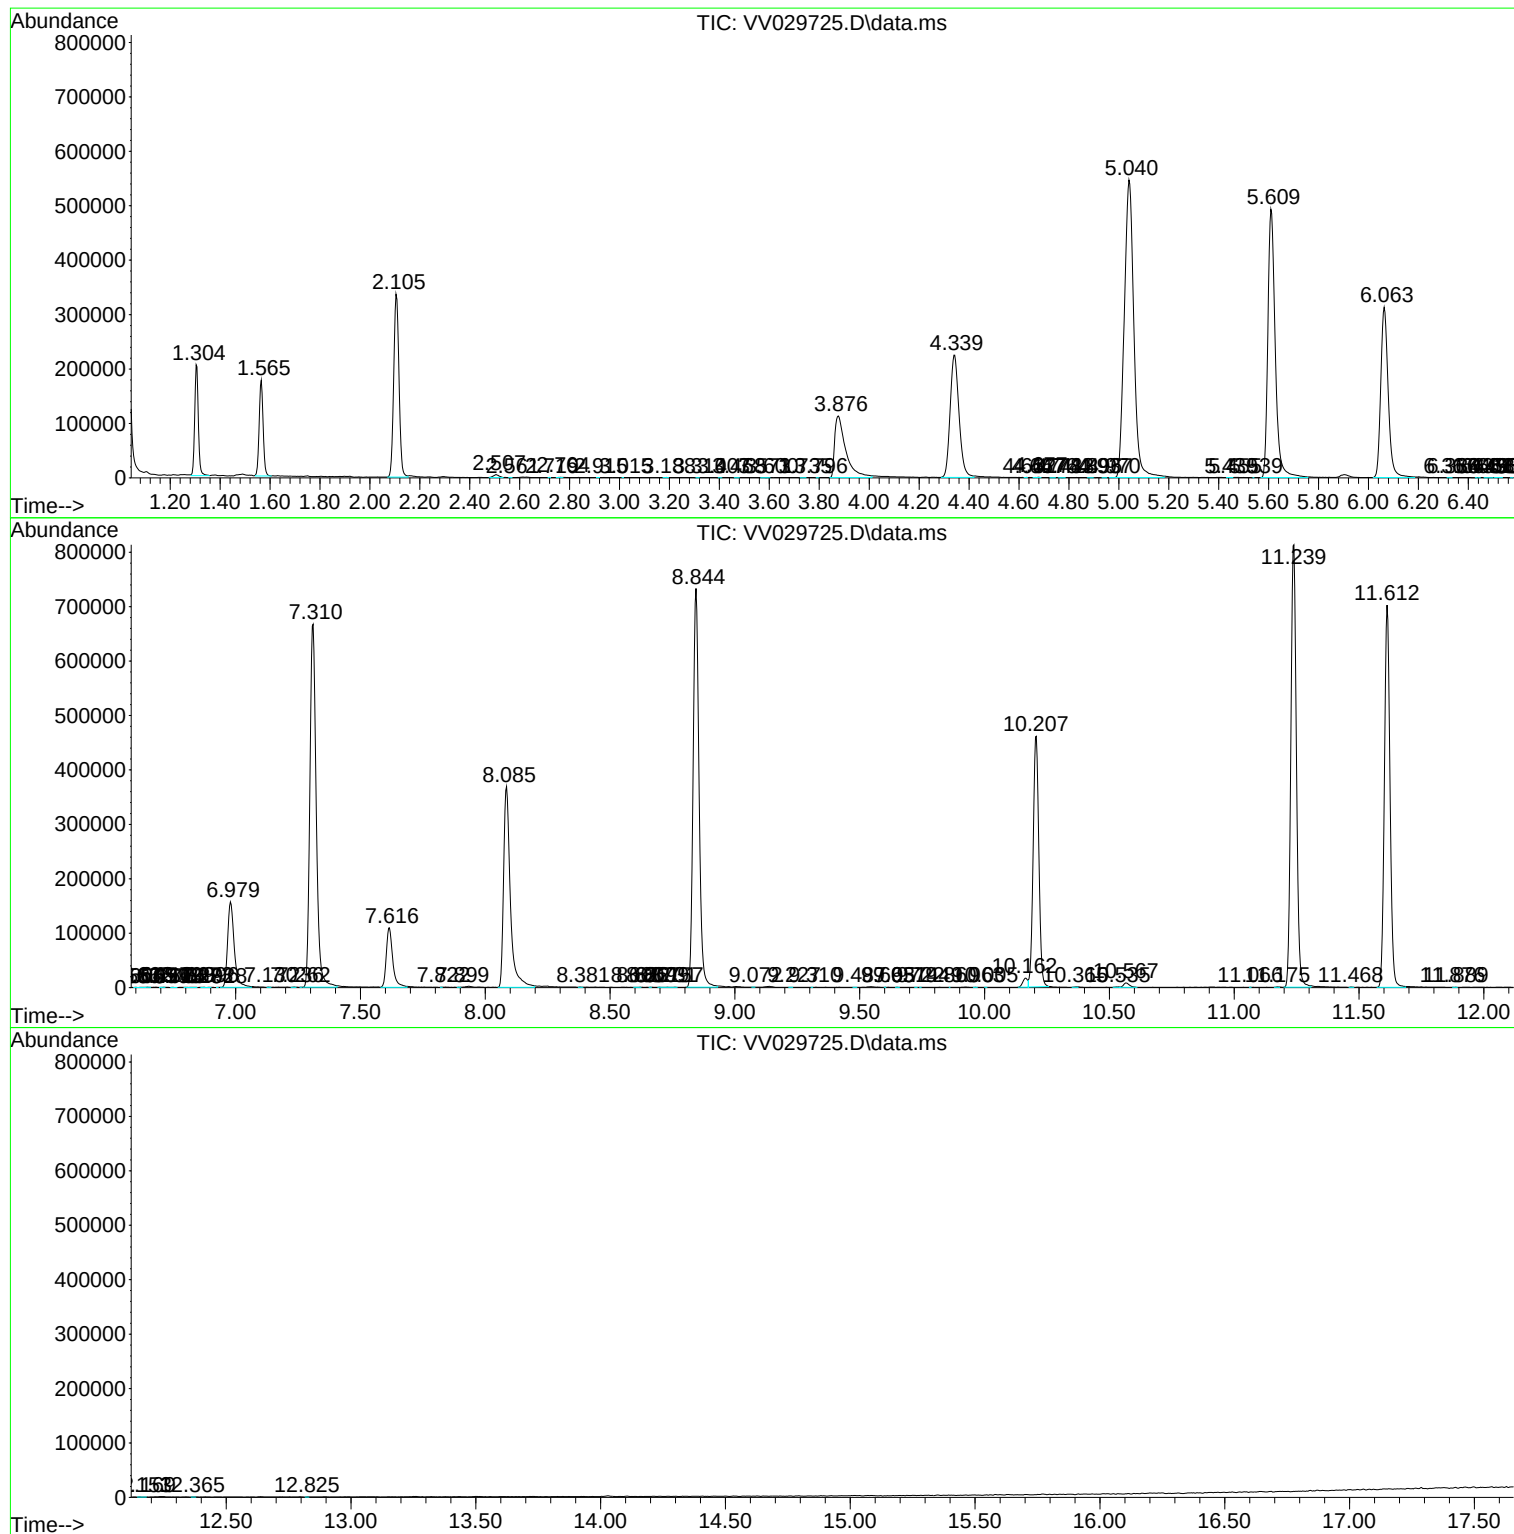

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029725.D
Acq On : 19 Dec 2022 16:36
Operator : SY/MD
Sample : N6093-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029725.D
Acq On : 19 Dec 2022 16:36
Operator : SY/MD
Sample : N6093-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc