

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
 Data File : VV029727.D
 Acq On : 19 Dec 2022 17:23
 Operator : SY/MD
 Sample : N6093-07 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	202687	204257	14.27%	1.741%
2	1.564	156	163	179	rVB	176971	200387	14.00%	1.708%
3	2.105	321	331	346	rBV	335399	478457	33.43%	4.078%
4	2.371	411	414	415	rBV	306	143	0.01%	0.001%
5	2.503	448	455	467	rVB	5267	8017	0.56%	0.068%
6	2.587	478	481	482	rBV	316	205	0.01%	0.002%
7	2.709	516	519	520	rBV	173	78	0.01%	0.001%
8	2.834	556	558	562	rVB2	325	150	0.01%	0.001%
9	2.854	562	564	570	rBV2	244	182	0.01%	0.002%
10	2.934	586	589	593	rBV2	210	214	0.01%	0.002%
11	3.002	609	610	611	rBV2	154	49	0.00%	0.000%
12	3.063	627	629	630	rBV	202	55	0.00%	0.000%
13	3.185	665	667	674	rVB3	337	329	0.02%	0.003%
14	3.217	674	677	679	rBV2	165	121	0.01%	0.001%
15	3.278	692	696	698	rBV2	113	94	0.01%	0.001%
16	3.346	713	717	721	rVB2	292	247	0.02%	0.002%
17	3.365	721	723	725	rBV2	293	86	0.01%	0.001%
18	3.378	725	727	729	rBV	121	76	0.01%	0.001%
19	3.513	766	769	775	rVB2	354	259	0.02%	0.002%
20	3.542	775	778	783	rBV2	130	138	0.01%	0.001%
21	3.568	783	786	791	rBV2	169	176	0.01%	0.001%
22	3.616	797	801	803	rBV2	140	108	0.01%	0.001%
23	3.879	868	883	929	rBV2	112717	362402	25.32%	3.088%
24	4.339	1011	1026	1056	rBV	223243	551435	38.53%	4.699%
25	4.674	1127	1130	1134	rVB2	469	315	0.02%	0.003%
26	4.690	1134	1135	1136	rBV	244	48	0.00%	0.000%
27	4.709	1139	1141	1143	rBV	143	77	0.01%	0.001%
28	4.722	1143	1145	1146	rBV	121	43	0.00%	0.000%
29	4.767	1154	1159	1164	rVB2	279	228	0.02%	0.002%
30	4.786	1164	1165	1167	rBV	140	52	0.00%	0.000%
31	4.834	1176	1180	1185	rBV2	186	186	0.01%	0.002%
32	4.870	1188	1191	1195	rVB2	112	79	0.01%	0.001%
33	4.892	1196	1198	1201	rBV	109	70	0.00%	0.001%
34	4.928	1206	1209	1215	rVB2	240	201	0.01%	0.002%
35	4.960	1215	1219	1224	rBV3	285	260	0.02%	0.002%
36	5.040	1225	1244	1286	rBV2	541446	1431131	100.00%	12.196%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029727.D
 Acq On : 19 Dec 2022 17:23
 Operator : SY/MD
 Sample : N6093-07 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.330	1332	1334	1340	rVB2	257	208	0.01%	0.002%
38	5.468	1372	1377	1378	rBV2	234	209	0.01%	0.002%
39	5.519	1390	1393	1395	rBV2	263	180	0.01%	0.002%
40	5.609	1408	1421	1455	rBV	504297	1036442	72.42%	8.833%
41	5.899	1502	1511	1528	rVB5	5503	11806	0.82%	0.101%
42	6.063	1546	1562	1598	rBV	313307	650984	45.49%	5.548%
43	6.281	1626	1630	1631	rBV	120	83	0.01%	0.001%
44	6.333	1644	1646	1649	rBV	120	56	0.00%	0.000%
45	6.368	1654	1657	1662	rVB	249	152	0.01%	0.001%
46	6.481	1690	1692	1695	rBV	104	58	0.00%	0.000%
47	6.519	1699	1704	1707	rVB2	224	217	0.02%	0.002%
48	6.580	1721	1723	1725	rVB	142	59	0.00%	0.001%
49	6.699	1757	1760	1762	rVB2	208	114	0.01%	0.001%
50	6.738	1770	1772	1773	rBV	174	57	0.00%	0.000%
51	6.979	1835	1847	1873	rBV	153149	286136	19.99%	2.439%
52	7.307	1937	1949	1986	rBV	647646	1164250	81.35%	9.922%
53	7.612	2034	2044	2073	rBV	107855	195367	13.65%	1.665%
54	7.818	2106	2108	2112	rBV3	302	248	0.02%	0.002%
55	7.863	2120	2122	2126	rVB2	422	259	0.02%	0.002%
56	7.882	2126	2128	2131	rBV	273	180	0.01%	0.002%
57	7.899	2131	2133	2135	rBV2	270	175	0.01%	0.001%
58	8.014	2164	2169	2173	rBV2	326	307	0.02%	0.003%
59	8.085	2181	2191	2229	rBV	376771	695021	48.56%	5.923%
60	8.365	2277	2278	2281	rVB	394	149	0.01%	0.001%
61	8.474	2309	2312	2317	rBV3	446	324	0.02%	0.003%
62	8.564	2338	2340	2343	rBV2	180	137	0.01%	0.001%
63	8.583	2345	2346	2348	rBV2	194	59	0.00%	0.001%
64	8.661	2367	2370	2371	rBV	177	107	0.01%	0.001%
65	8.696	2380	2381	2383	rVB	420	86	0.01%	0.001%
66	8.718	2385	2388	2391	rBV	308	190	0.01%	0.002%
67	8.741	2392	2395	2400	rBV2	211	160	0.01%	0.001%
68	8.799	2411	2413	2415	rBV3	259	97	0.01%	0.001%
69	8.844	2415	2427	2462	rBV	749637	1240321	86.67%	10.570%
70	9.175	2528	2530	2533	rBV2	180	78	0.01%	0.001%
71	9.204	2534	2539	2540	rBV3	219	169	0.01%	0.001%
72	9.255	2552	2555	2557	rBV	237	110	0.01%	0.001%
73	9.271	2557	2560	2567	rBV2	229	282	0.02%	0.002%
74	9.352	2583	2585	2588	rVB	298	151	0.01%	0.001%
75	9.365	2588	2589	2590	rVB	228	44	0.00%	0.000%
76	9.378	2590	2593	2595	rBV2	99	67	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029727.D
 Acq On : 19 Dec 2022 17:23
 Operator : SY/MD
 Sample : N6093-07 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.439	2609	2612	2617	rBV2	148	117	0.01%	0.001%
78	9.673	2684	2685	2686	rBV2	112	37	0.00%	0.000%
79	9.828	2729	2733	2739	rBV2	283	311	0.02%	0.003%
80	9.892	2750	2753	2756	rBV2	295	178	0.01%	0.002%
81	9.921	2757	2762	2767	rVV4	401	466	0.03%	0.004%
82	9.972	2776	2778	2783	rVB2	190	114	0.01%	0.001%
83	10.091	2812	2815	2818	rBV	367	236	0.02%	0.002%
84	10.165	2828	2838	2841	rBV2	16543	23556	1.65%	0.201%
85	10.204	2841	2850	2873	rVB	470567	739122	51.65%	6.299%
86	10.378	2897	2904	2909	rBV3	1312	1635	0.11%	0.014%
87	10.567	2956	2963	2978	rVB2	8060	12920	0.90%	0.110%
88	10.886	3059	3062	3065	rBV2	369	233	0.02%	0.002%
89	10.905	3065	3068	3069	rBV2	350	211	0.01%	0.002%
90	11.107	3128	3131	3132	rBV	261	160	0.01%	0.001%
91	11.149	3140	3144	3147	rBV	506	326	0.02%	0.003%
92	11.236	3159	3171	3198	rBV	836433	1297438	90.66%	11.057%
93	11.468	3241	3243	3245	rBV2	441	283	0.02%	0.002%
94	11.612	3274	3288	3313	rBV	721141	1128739	78.87%	9.619%
95	12.078	3430	3433	3435	rBV2	338	214	0.01%	0.002%
96	12.336	3511	3513	3524	rVB5	1388	1425	0.10%	0.012%
97	12.638	3603	3607	3612	rBV3	821	848	0.06%	0.007%




Sum of corrected areas: 11734023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029727.D
Acq On : 19 Dec 2022 17:23
Operator : SY/MD
Sample : N6093-07 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

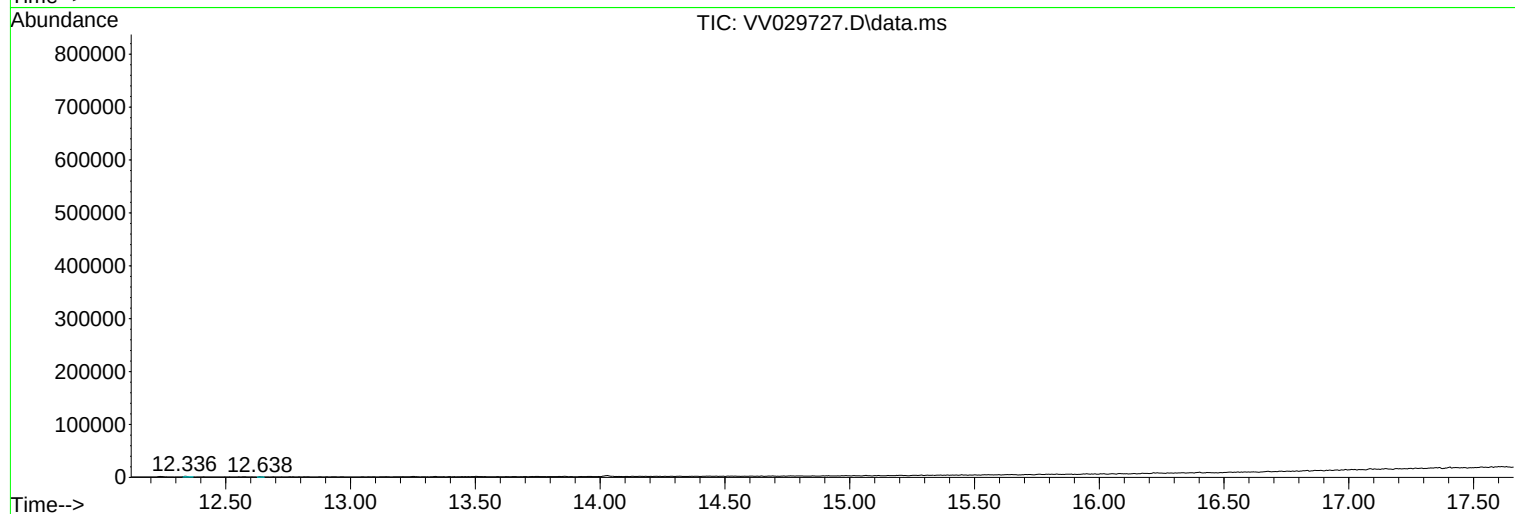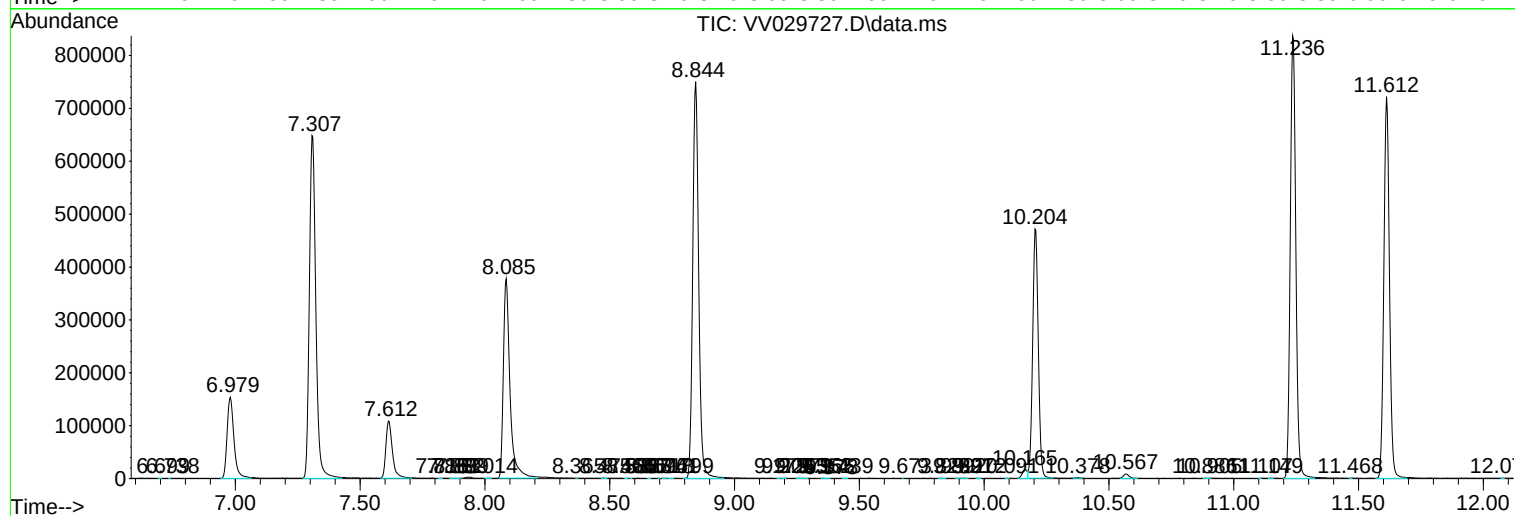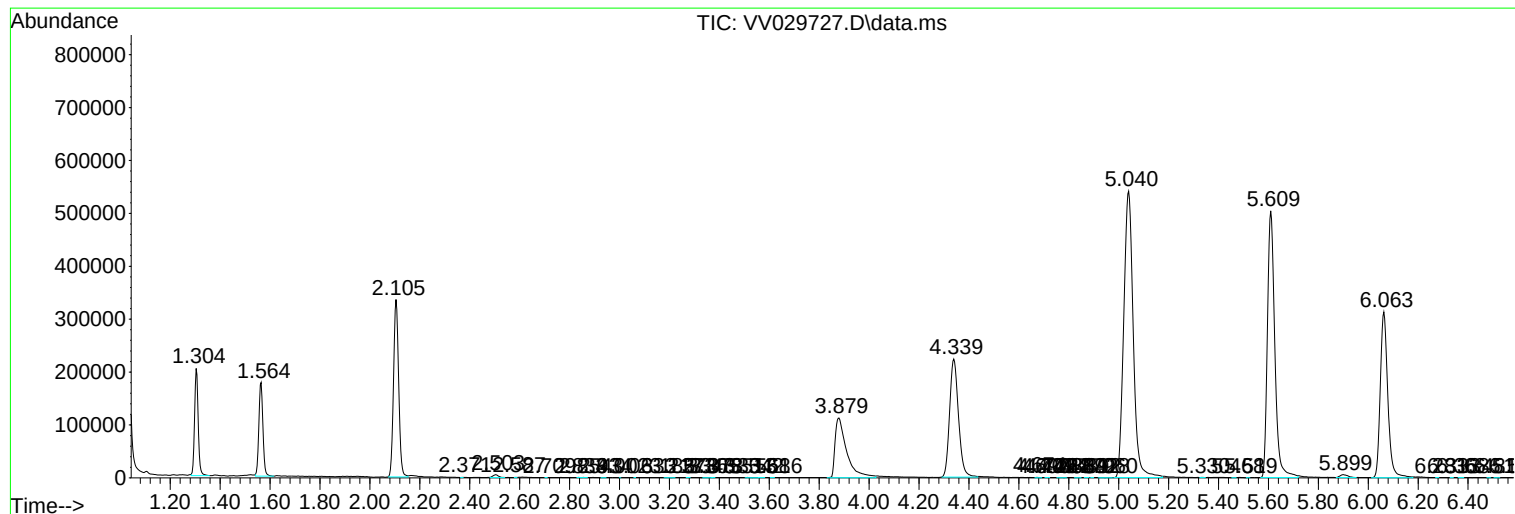

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029727.D
Acq On : 19 Dec 2022 17:23
Operator : SY/MD
Sample : N6093-07 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029727.D
Acq On : 19 Dec 2022 17:23
Operator : SY/MD
Sample : N6093-07 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------