

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029730.D
 Acq On : 19 Dec 2022 18:33
 Operator : SY/MD
 Sample : N6075-11 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	196654	195935	14.76%	1.787%
2	1.565	155	163	178	rVB	161006	185744	14.00%	1.694%
3	2.105	320	331	346	rBV	317127	450738	33.97%	4.111%
4	2.436	432	434	437	rVB	297	115	0.01%	0.001%
5	2.503	447	455	467	rBV2	4220	6416	0.48%	0.059%
6	2.616	483	490	493	rBV4	740	1136	0.09%	0.010%
7	2.687	509	512	516	rBV2	254	229	0.02%	0.002%
8	2.857	563	565	567	rVB	230	77	0.01%	0.001%
9	2.873	567	570	571	rBV	117	63	0.00%	0.001%
10	2.954	594	595	598	rVB2	246	63	0.00%	0.001%
11	2.976	598	602	604	rBV	236	187	0.01%	0.002%
12	3.111	641	644	646	rBV2	192	139	0.01%	0.001%
13	3.272	692	694	696	rVB	156	62	0.00%	0.001%
14	3.323	706	710	713	rBV	204	172	0.01%	0.002%
15	3.362	720	722	723	rBV	318	92	0.01%	0.001%
16	3.394	731	732	734	rBV	122	51	0.00%	0.000%
17	3.452	747	750	753	rBV	146	110	0.01%	0.001%
18	3.571	783	787	790	rBV2	153	120	0.01%	0.001%
19	3.587	790	792	794	rBV	117	62	0.00%	0.001%
20	3.722	830	834	837	rBV	163	134	0.01%	0.001%
21	3.773	846	850	852	rBV2	127	104	0.01%	0.001%
22	3.876	872	882	927	rBV2	103365	324778	24.47%	2.962%
23	4.339	1010	1026	1058	rBV	206895	518126	39.04%	4.726%
24	4.616	1109	1112	1113	rBV	167	81	0.01%	0.001%
25	4.638	1117	1119	1120	rBV	134	51	0.00%	0.000%
26	4.671	1126	1129	1133	rVB	257	200	0.02%	0.002%
27	4.703	1136	1139	1141	rBV	74	39	0.00%	0.000%
28	4.741	1144	1151	1156	rBV2	211	244	0.02%	0.002%
29	4.777	1159	1162	1164	rBV3	152	86	0.01%	0.001%
30	4.793	1164	1167	1169	rVB2	138	76	0.01%	0.001%
31	4.915	1202	1205	1207	rBV2	98	50	0.00%	0.000%
32	4.931	1207	1210	1212	rBV2	124	95	0.01%	0.001%
33	4.966	1218	1221	1224	rVB	84	44	0.00%	0.000%
34	4.979	1224	1225	1226	rBV	174	38	0.00%	0.000%
35	5.040	1226	1244	1273	rBV2	501580	1327044	100.00%	12.103%
36	5.381	1348	1350	1352	rBV	188	108	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029730.D
 Acq On : 19 Dec 2022 18:33
 Operator : SY/MD
 Sample : N6075-11 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.503	1386	1388	1391	rVB2	177	79	0.01%	0.001%
38	5.526	1392	1395	1396	rBV2	151	84	0.01%	0.001%
39	5.555	1403	1404	1406	rVB2	153	32	0.00%	0.000%
40	5.609	1406	1421	1453	rBV	486898	996759	75.11%	9.091%
41	5.899	1502	1511	1532	rVB4	4838	10918	0.82%	0.100%
42	6.063	1548	1562	1591	rBV	289455	600144	45.22%	5.474%
43	6.278	1625	1629	1632	rBV3	319	152	0.01%	0.001%
44	6.320	1641	1642	1644	rBV	183	69	0.01%	0.001%
45	6.359	1652	1654	1655	rBV	120	47	0.00%	0.000%
46	6.368	1655	1657	1658	rBV	82	35	0.00%	0.000%
47	6.400	1664	1667	1669	rBV	149	90	0.01%	0.001%
48	6.426	1673	1675	1678	rVB2	111	53	0.00%	0.000%
49	6.445	1678	1681	1684	rBV	174	135	0.01%	0.001%
50	6.513	1699	1702	1704	rBV2	200	104	0.01%	0.001%
51	6.542	1710	1711	1712	rBV2	147	45	0.00%	0.000%
52	6.580	1721	1723	1724	rBV	161	50	0.00%	0.000%
53	6.603	1728	1730	1732	rBV2	30	13	0.00%	0.000%
54	6.645	1733	1743	1747	rBV4	612	982	0.07%	0.009%
55	6.725	1765	1768	1770	rVB2	281	137	0.01%	0.001%
56	6.744	1770	1774	1778	rVB2	206	150	0.01%	0.001%
57	6.918	1826	1828	1829	rBV2	163	55	0.00%	0.001%
58	6.931	1831	1832	1833	rVV2	157	46	0.00%	0.000%
59	6.979	1836	1847	1878	rBV	143753	267304	20.14%	2.438%
60	7.146	1897	1899	1903	rBV3	308	216	0.02%	0.002%
61	7.236	1924	1927	1930	rVB3	386	223	0.02%	0.002%
62	7.307	1937	1949	1984	rBV	601541	1081086	81.47%	9.860%
63	7.613	2033	2044	2063	rBV	102495	182327	13.74%	1.663%
64	7.831	2109	2112	2116	rVB2	464	381	0.03%	0.003%
65	8.085	2180	2191	2227	rBV	340141	637921	48.07%	5.818%
66	8.497	2316	2319	2321	rBV3	457	315	0.02%	0.003%
67	8.529	2326	2329	2332	rVB	450	321	0.02%	0.003%
68	8.551	2332	2336	2337	rBV	171	104	0.01%	0.001%
69	8.564	2337	2340	2344	rVB3	544	345	0.03%	0.003%
70	8.600	2349	2351	2353	rBV2	249	137	0.01%	0.001%
71	8.658	2367	2369	2371	rBV2	292	75	0.01%	0.001%
72	8.670	2371	2373	2375	rVV	208	92	0.01%	0.001%
73	8.686	2376	2378	2383	rVB2	268	151	0.01%	0.001%
74	8.844	2414	2427	2456	rBV	724377	1195056	90.05%	10.900%
75	9.137	2514	2518	2521	rBV3	547	436	0.03%	0.004%
76	9.204	2537	2539	2542	rVB2	199	91	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029730.D
 Acq On : 19 Dec 2022 18:33
 Operator : SY/MD
 Sample : N6075-11 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.281	2560	2563	2566	rBV2	128	117	0.01%	0.001%
78	9.294	2566	2567	2568	rVV2	162	44	0.00%	0.000%
79	9.307	2568	2571	2576	rVB	248	200	0.02%	0.002%
80	9.330	2576	2578	2580	rBV	148	89	0.01%	0.001%
81	9.535	2639	2642	2644	rBV2	428	250	0.02%	0.002%
82	9.651	2675	2678	2683	rBV2	219	176	0.01%	0.002%
83	9.918	2759	2761	2769	rVB3	381	386	0.03%	0.004%
84	10.040	2796	2799	2801	rBV2	215	134	0.01%	0.001%
85	10.066	2805	2807	2810	rBV2	188	109	0.01%	0.001%
86	10.162	2827	2837	2840	rBV2	16060	20381	1.54%	0.186%
87	10.204	2841	2850	2872	rVB	419458	675320	50.89%	6.159%
88	10.526	2948	2950	2951	rBV2	253	94	0.01%	0.001%
89	10.567	2955	2963	2973	rVV2	7231	11552	0.87%	0.105%
90	10.622	2979	2980	2983	rBV	232	135	0.01%	0.001%
91	10.715	3004	3009	3012	rBV	275	269	0.02%	0.002%
92	10.863	3053	3055	3057	rVB	246	123	0.01%	0.001%
93	10.899	3064	3066	3067	rBV2	219	82	0.01%	0.001%
94	10.944	3078	3080	3084	rVB3	363	193	0.01%	0.002%
95	11.175	3148	3152	3155	rBV4	380	383	0.03%	0.003%
96	11.236	3159	3171	3195	rBV	787133	1227152	92.47%	11.192%
97	11.612	3273	3288	3310	rBV	649811	1037468	78.18%	9.462%




Sum of corrected areas: 10964226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029730.D
Acq On : 19 Dec 2022 18:33
Operator : SY/MD
Sample : N6075-11 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

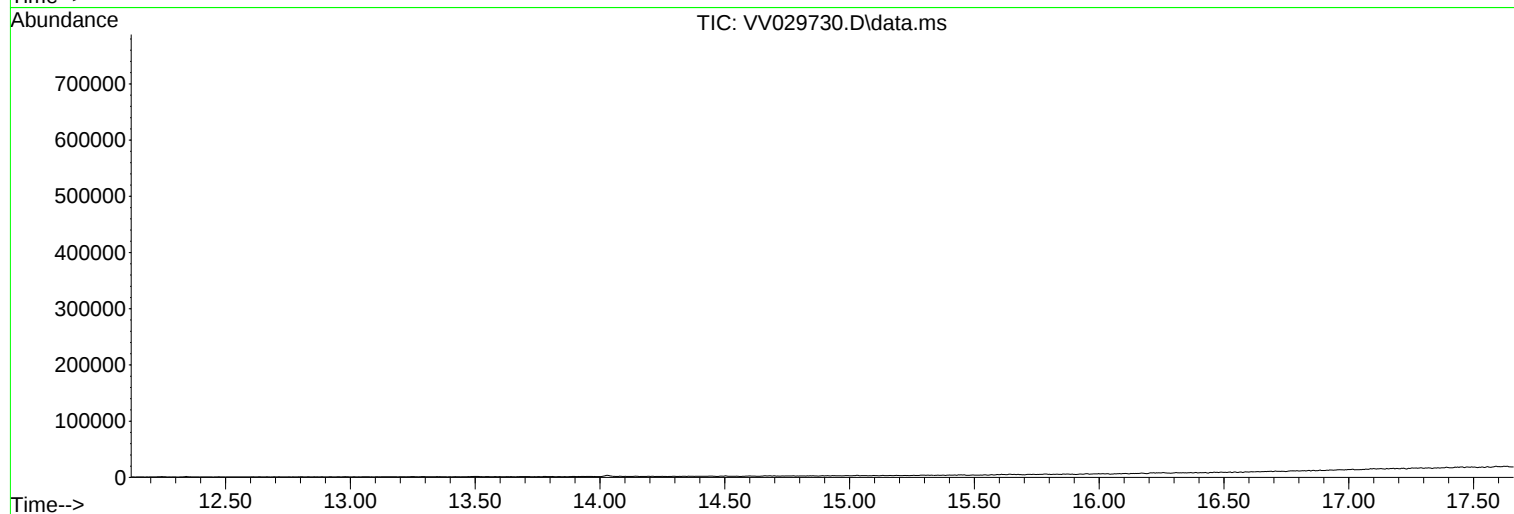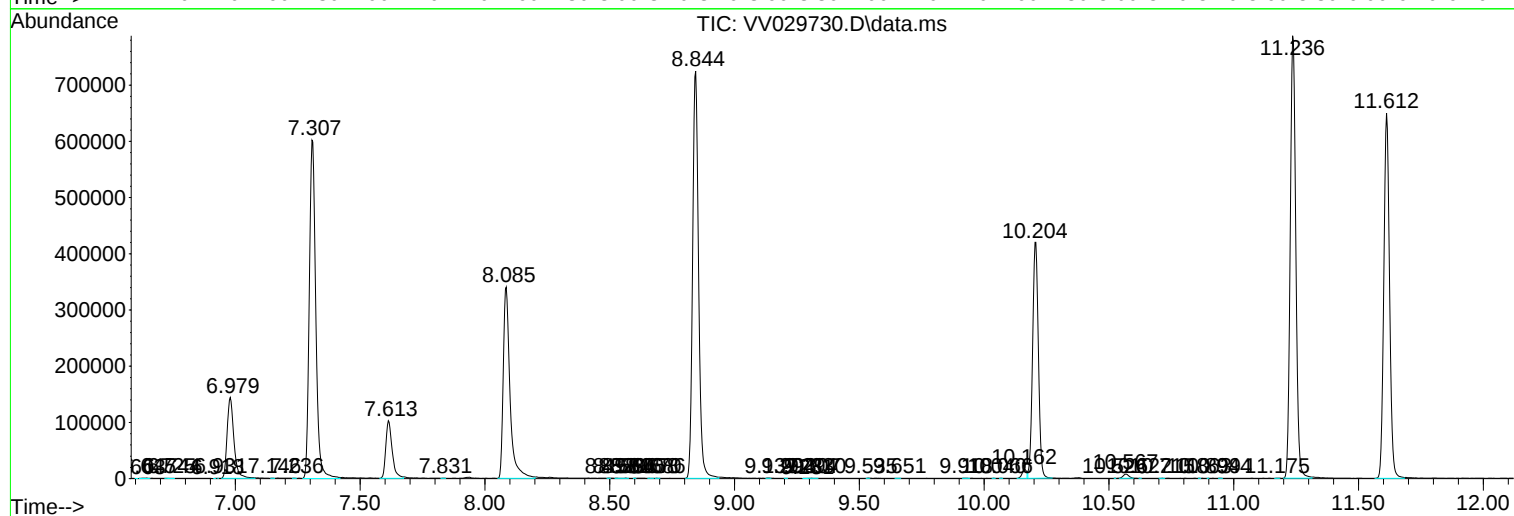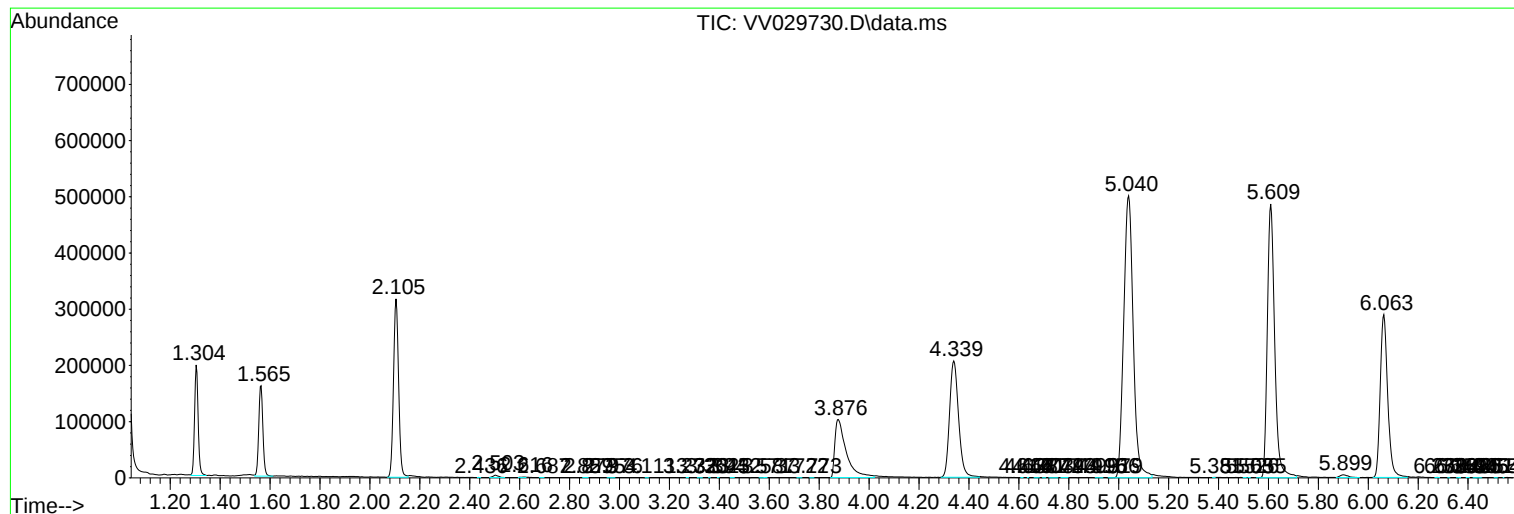

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029730.D
Acq On : 19 Dec 2022 18:33
Operator : SY/MD
Sample : N6075-11 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029730.D
Acq On : 19 Dec 2022 18:33
Operator : SY/MD
Sample : N6075-11 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------