

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029731.D
 Acq On : 19 Dec 2022 18:57
 Operator : SY/MD
 Sample : N6075-12 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	190987	191684	14.25%	1.834%
2	1.565	156	163	176	rVB	164877	186960	13.90%	1.789%
3	2.105	321	331	345	rBV	311041	445004	33.09%	4.257%
4	2.429	431	432	436	rBV	259	212	0.02%	0.002%
5	2.503	447	455	466	rVB2	6687	11274	0.84%	0.108%
6	2.577	473	478	480	rBV2	140	141	0.01%	0.001%
7	2.651	498	501	504	rBV	271	222	0.02%	0.002%
8	2.719	520	522	526	rBV	148	94	0.01%	0.001%
9	2.770	534	538	541	rVB2	212	141	0.01%	0.001%
10	2.851	560	563	568	rBV	184	171	0.01%	0.002%
11	2.970	596	600	603	rBV2	107	107	0.01%	0.001%
12	3.121	642	647	649	rBV	227	205	0.02%	0.002%
13	3.195	666	670	672	rBV2	159	119	0.01%	0.001%
14	3.307	699	705	708	rBV2	120	130	0.01%	0.001%
15	3.323	708	710	715	rVV2	177	133	0.01%	0.001%
16	3.372	720	725	729	rVV2	158	169	0.01%	0.002%
17	3.474	753	757	761	rBV2	349	259	0.02%	0.002%
18	3.507	761	767	771	rBV2	229	227	0.02%	0.002%
19	3.609	797	799	804	rVB	162	109	0.01%	0.001%
20	3.799	854	858	864	rBV2	248	261	0.02%	0.002%
21	3.880	868	883	923	rBV2	100630	322795	24.00%	3.088%
22	4.339	1010	1026	1063	rBV	207100	520261	38.68%	4.977%
23	4.590	1100	1104	1109	rBV2	280	338	0.03%	0.003%
24	4.658	1124	1125	1129	rVB2	340	140	0.01%	0.001%
25	4.748	1149	1153	1156	rBV2	169	107	0.01%	0.001%
26	4.789	1160	1166	1167	rBV2	209	154	0.01%	0.001%
27	4.928	1205	1209	1211	rBV	263	155	0.01%	0.001%
28	5.040	1226	1244	1291	rVV2	507603	1344950	100.00%	12.867%
29	5.310	1325	1328	1335	rBV4	279	282	0.02%	0.003%
30	5.404	1354	1357	1361	rVB2	342	250	0.02%	0.002%
31	5.429	1362	1365	1368	rVB2	173	76	0.01%	0.001%
32	5.471	1372	1378	1380	rBV3	261	330	0.02%	0.003%
33	5.539	1397	1399	1401	rVV	151	72	0.01%	0.001%
34	5.609	1408	1421	1465	rBV	402919	840463	62.49%	8.041%
35	5.899	1501	1511	1529	rVB5	4997	11297	0.84%	0.108%
36	5.989	1537	1539	1542	rBV2	206	119	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029731.D
 Acq On : 19 Dec 2022 18:57
 Operator : SY/MD
 Sample : N6075-12 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1547	1562	1597	rBV	291029	606140	45.07%	5.799%
38	6.381	1658	1661	1663	rVV	195	127	0.01%	0.001%
39	6.391	1663	1664	1666	rVV	197	89	0.01%	0.001%
40	6.416	1669	1672	1674	rBV	170	137	0.01%	0.001%
41	6.478	1689	1691	1694	rVB2	206	110	0.01%	0.001%
42	6.510	1699	1701	1704	rBV2	321	113	0.01%	0.001%
43	6.580	1720	1723	1727	rBV2	181	152	0.01%	0.001%
44	6.616	1731	1734	1737	rBV	464	292	0.02%	0.003%
45	6.712	1760	1764	1766	rBV	243	171	0.01%	0.002%
46	6.725	1766	1768	1770	rVV	272	128	0.01%	0.001%
47	6.738	1770	1772	1774	rVB	232	84	0.01%	0.001%
48	6.799	1789	1791	1797	rVB2	225	144	0.01%	0.001%
49	6.825	1797	1799	1804	rBV	107	76	0.01%	0.001%
50	6.979	1835	1847	1874	rBV	144596	267408	19.88%	2.558%
51	7.124	1889	1892	1895	rBV2	269	168	0.01%	0.002%
52	7.223	1920	1923	1926	rVB2	314	225	0.02%	0.002%
53	7.240	1926	1928	1929	rBV2	220	84	0.01%	0.001%
54	7.307	1936	1949	1981	rBV	609154	1086266	80.77%	10.392%
55	7.613	2033	2044	2065	rBV	101436	182230	13.55%	1.743%
56	7.728	2078	2080	2083	rVB2	771	394	0.03%	0.004%
57	7.796	2098	2101	2106	rVB3	488	410	0.03%	0.004%
58	7.870	2121	2124	2127	rBV3	322	240	0.02%	0.002%
59	7.934	2135	2144	2153	rVB2	2761	4391	0.33%	0.042%
60	8.085	2180	2191	2229	rBV	338558	639147	47.52%	6.115%
61	8.358	2273	2276	2280	rVB3	638	450	0.03%	0.004%
62	8.526	2323	2328	2331	rBV3	715	539	0.04%	0.005%
63	8.545	2332	2334	2337	rBV3	306	144	0.01%	0.001%
64	8.571	2337	2342	2346	rBV3	487	403	0.03%	0.004%
65	8.587	2346	2347	2350	rBV2	200	84	0.01%	0.001%
66	8.603	2350	2352	2354	rBV	367	160	0.01%	0.002%
67	8.680	2373	2376	2381	rVB	492	314	0.02%	0.003%
68	8.844	2414	2427	2453	rBV	606831	1002857	74.56%	9.594%
69	9.214	2538	2542	2543	rBV	340	167	0.01%	0.002%
70	9.249	2550	2553	2555	rBV	221	152	0.01%	0.001%
71	9.323	2572	2576	2579	rBV3	457	235	0.02%	0.002%
72	9.538	2639	2643	2645	rBV2	416	253	0.02%	0.002%
73	9.770	2712	2715	2716	rBV	199	122	0.01%	0.001%
74	9.921	2759	2762	2767	rVB3	328	189	0.01%	0.002%
75	9.944	2767	2769	2771	rVV2	210	88	0.01%	0.001%
76	9.963	2772	2775	2778	rVV2	338	223	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
 Data File : VV029731.D
 Acq On : 19 Dec 2022 18:57
 Operator : SY/MD
 Sample : N6075-12 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.992	2782	2784	2787	rVB3	281	153	0.01%	0.001%
78	10.162	2828	2837	2840	rBV2	14681	19342	1.44%	0.185%
79	10.204	2841	2850	2876	rVB	433954	687665	51.13%	6.579%
80	10.374	2894	2903	2910	rBV4	2580	3334	0.25%	0.032%
81	10.461	2929	2930	2937	rVB2	283	187	0.01%	0.002%
82	10.529	2946	2951	2953	rBV2	463	404	0.03%	0.004%
83	10.571	2955	2964	2974	rVV2	7134	11077	0.82%	0.106%
84	10.841	3047	3048	3050	rVB	281	83	0.01%	0.001%
85	10.857	3050	3053	3054	rBV	340	196	0.01%	0.002%
86	10.953	3081	3083	3085	rBV	275	154	0.01%	0.001%
87	11.072	3118	3120	3121	rBV	242	87	0.01%	0.001%
88	11.146	3140	3143	3148	rVB3	916	856	0.06%	0.008%
89	11.178	3150	3153	3156	rBV2	359	256	0.02%	0.002%
90	11.236	3159	3171	3198	rBV	675439	1043948	77.62%	9.987%
91	11.455	3237	3239	3245	rBV3	280	222	0.02%	0.002%
92	11.551	3267	3269	3274	rBV	289	196	0.01%	0.002%
93	11.612	3275	3288	3312	rBV	648583	1008090	74.95%	9.644%
94	11.892	3371	3375	3378	rBV2	426	329	0.02%	0.003%
95	11.944	3389	3391	3395	rBV2	279	209	0.02%	0.002%
96	12.236	3475	3482	3483	rBV3	686	755	0.06%	0.007%
97	12.291	3497	3499	3501	rBV	339	131	0.01%	0.001%
98	12.394	3529	3531	3533	rBV2	302	136	0.01%	0.001%
99	12.725	3630	3634	3638	rBV2	373	373	0.03%	0.004%
100	12.796	3654	3656	3659	rBV	243	158	0.01%	0.002%




Sum of corrected areas: 10452858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029731.D
Acq On : 19 Dec 2022 18:57
Operator : SY/MD
Sample : N6075-12 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

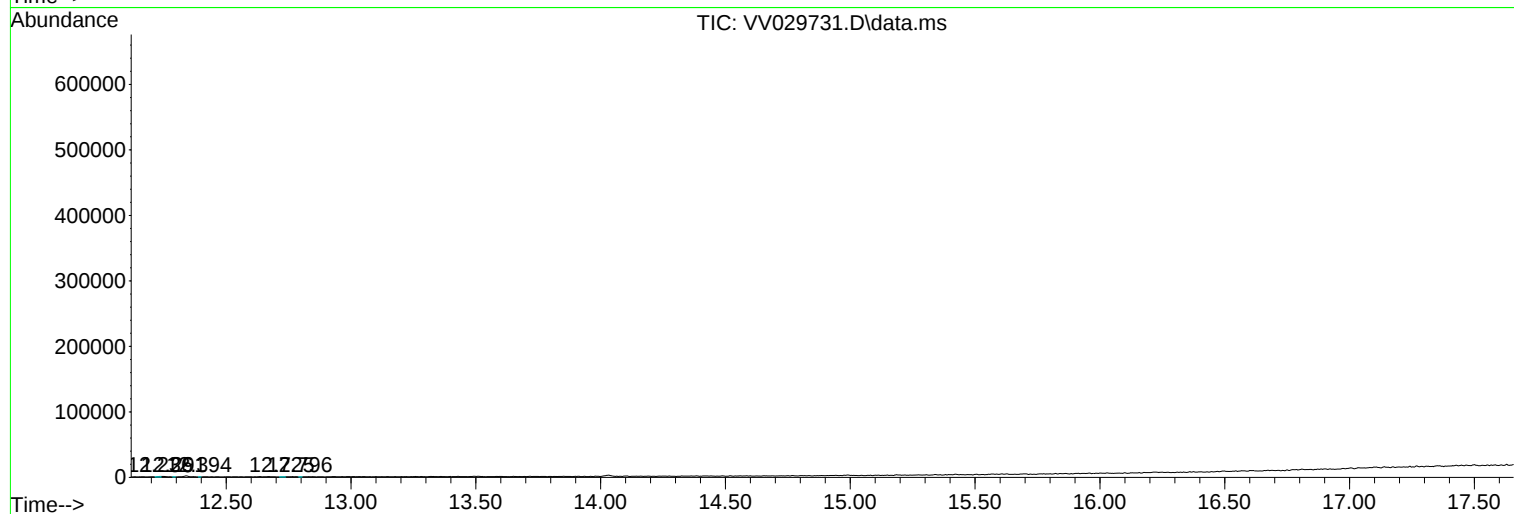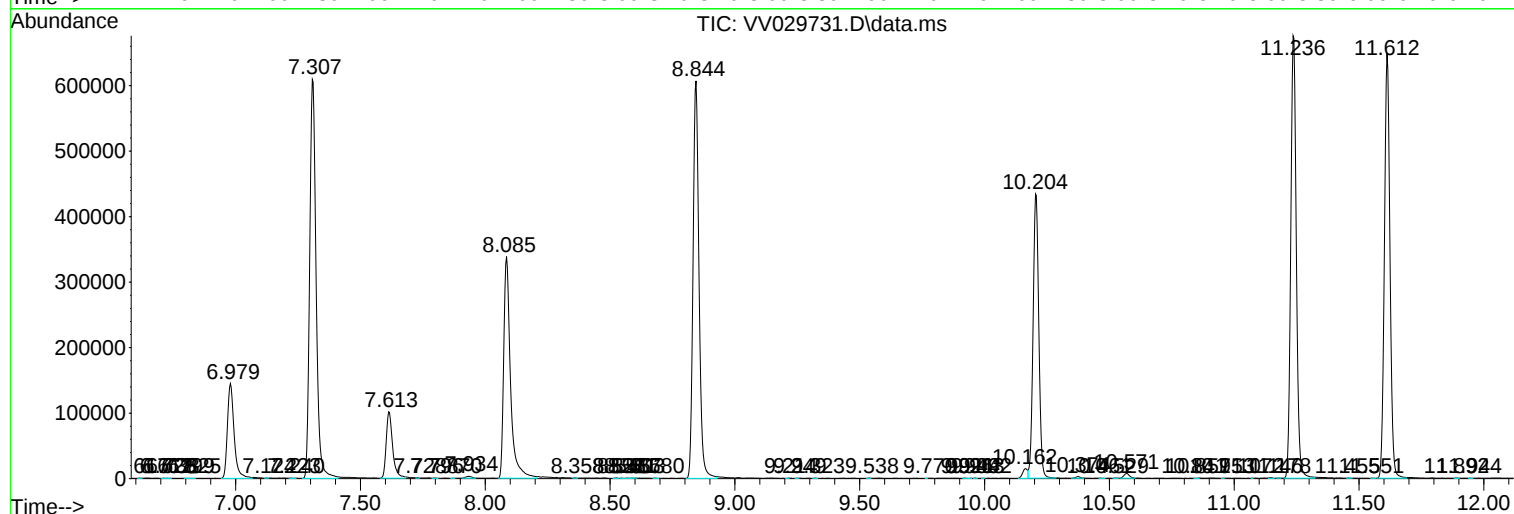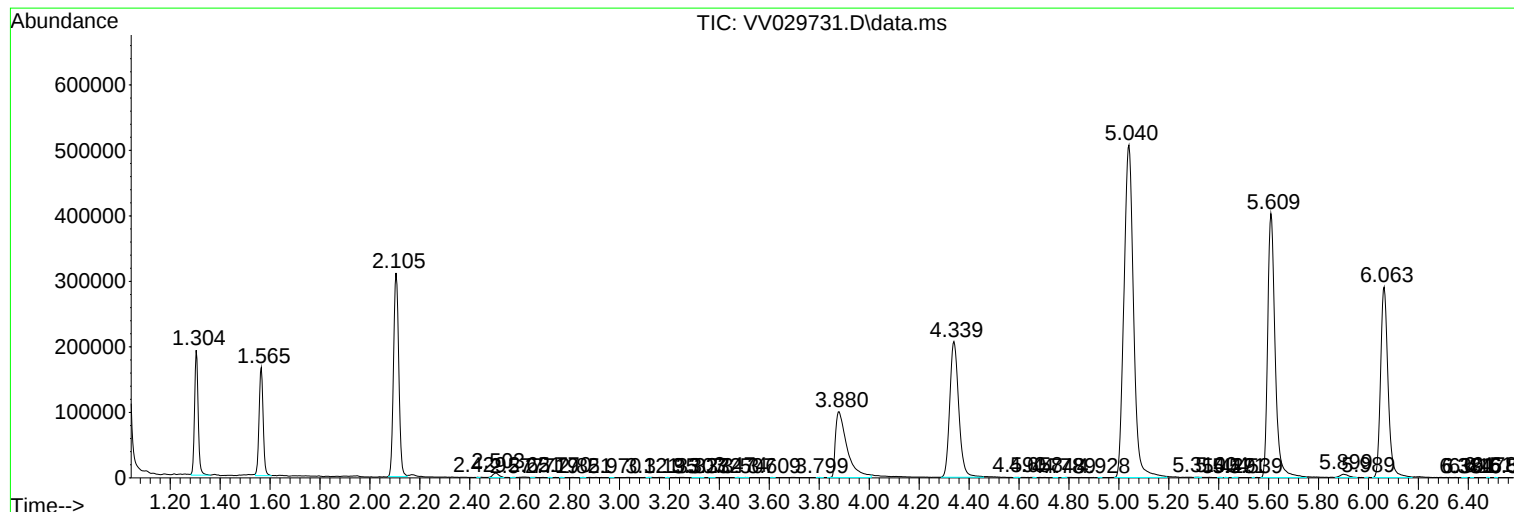

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029731.D
Acq On : 19 Dec 2022 18:57
Operator : SY/MD
Sample : N6075-12 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029731.D
Acq On : 19 Dec 2022 18:57
Operator : SY/MD
Sample : N6075-12 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------