

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029732.D
 Acq On : 19 Dec 2022 19:20
 Operator : SY/MD
 Sample : N6075-13 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	201222	197233	14.81%	1.794%
2	1.561	155	162	177	rVB	157111	179193	13.46%	1.630%
3	2.105	319	331	344	rBV	311438	444465	33.38%	4.043%
4	2.249	373	376	379	rBV4	552	402	0.03%	0.004%
5	2.500	447	454	465	rVB2	4360	7069	0.53%	0.064%
6	2.616	481	490	498	rBV3	902	1827	0.14%	0.017%
7	2.732	523	526	530	rVV3	272	214	0.02%	0.002%
8	2.760	532	535	538	rVV2	260	179	0.01%	0.002%
9	3.143	649	654	656	rBV2	338	234	0.02%	0.002%
10	3.236	677	683	689	rBV2	189	322	0.02%	0.003%
11	3.423	735	741	744	rBV2	182	243	0.02%	0.002%
12	3.876	867	882	916	rBV2	107696	341649	25.66%	3.108%
13	4.339	1009	1026	1052	rBV	207942	518949	38.97%	4.721%
14	4.674	1127	1130	1138	rVV3	386	404	0.03%	0.004%
15	4.722	1141	1145	1148	rVV2	221	171	0.01%	0.002%
16	5.040	1226	1244	1291	rBV2	505052	1331520	100.00%	12.112%
17	5.278	1315	1318	1321	rVB2	309	189	0.01%	0.002%
18	5.394	1350	1354	1361	rVV3	308	428	0.03%	0.004%
19	5.452	1365	1372	1374	rVB3	237	254	0.02%	0.002%
20	5.484	1379	1382	1386	rVB3	302	230	0.02%	0.002%
21	5.609	1404	1421	1459	rBV	483080	999319	75.05%	9.090%
22	5.902	1502	1512	1528	rVB4	4592	10243	0.77%	0.093%
23	6.063	1548	1562	1599	rBV	286966	603186	45.30%	5.487%
24	6.188	1599	1601	1603	rBV2	549	311	0.02%	0.003%
25	6.268	1624	1626	1630	rVB2	373	224	0.02%	0.002%
26	6.346	1644	1650	1654	rBV2	214	231	0.02%	0.002%
27	6.426	1670	1675	1679	rBV2	380	393	0.03%	0.004%
28	6.577	1717	1722	1727	rVB2	242	329	0.02%	0.003%
29	6.738	1767	1772	1774	rVB2	283	213	0.02%	0.002%
30	6.764	1774	1780	1782	rBV2	215	174	0.01%	0.002%
31	6.889	1815	1819	1822	rBV2	235	186	0.01%	0.002%
32	6.979	1836	1847	1872	rBV	142826	265441	19.94%	2.415%
33	7.198	1912	1915	1918	rBV3	476	380	0.03%	0.003%
34	7.230	1923	1925	1929	rVB3	312	188	0.01%	0.002%
35	7.310	1936	1950	1979	rBV	598968	1079597	81.08%	9.821%
36	7.612	2034	2044	2067	rBV	102492	179685	13.49%	1.635%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029732.D
 Acq On : 19 Dec 2022 19:20
 Operator : SY/MD
 Sample : N6075-13 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.760	2087	2090	2093	rVB3	414	246	0.02%	0.002%
38	7.818	2103	2108	2109	rBV2	450	321	0.02%	0.003%
39	7.866	2119	2123	2125	rBV2	476	225	0.02%	0.002%
40	7.931	2131	2143	2156	rVB2	2484	4662	0.35%	0.042%
41	8.085	2180	2191	2223	rBV	343412	638949	47.99%	5.812%
42	8.252	2240	2243	2248	rVB5	785	763	0.06%	0.007%
43	8.413	2291	2293	2297	rVB2	450	350	0.03%	0.003%
44	8.445	2297	2303	2305	rBV	481	513	0.04%	0.005%
45	8.519	2322	2326	2329	rBV4	452	376	0.03%	0.003%
46	8.609	2351	2354	2358	rBV3	327	254	0.02%	0.002%
47	8.757	2396	2400	2404	rBV2	236	212	0.02%	0.002%
48	8.844	2412	2427	2460	rBV	730425	1191540	89.49%	10.839%
49	9.091	2501	2504	2509	rVB2	408	328	0.02%	0.003%
50	9.136	2514	2518	2521	rBV5	513	479	0.04%	0.004%
51	9.281	2559	2563	2565	rBV	323	210	0.02%	0.002%
52	9.333	2574	2579	2581	rBV	490	315	0.02%	0.003%
53	9.542	2641	2644	2646	rBV	421	258	0.02%	0.002%
54	9.696	2687	2692	2693	rBV2	272	176	0.01%	0.002%
55	9.918	2754	2761	2764	rBV3	332	408	0.03%	0.004%
56	9.985	2779	2782	2787	rBV3	326	276	0.02%	0.003%
57	10.072	2799	2809	2812	rBV3	370	464	0.03%	0.004%
58	10.162	2827	2837	2840	rBV2	14868	19183	1.44%	0.174%
59	10.207	2841	2851	2872	rVB	430295	681042	51.15%	6.195%
60	10.320	2883	2886	2892	rBV2	250	269	0.02%	0.002%
61	10.374	2896	2903	2911	rVB3	1676	2392	0.18%	0.022%
62	10.448	2923	2926	2931	rVB4	304	262	0.02%	0.002%
63	10.522	2947	2949	2952	rVV2	430	302	0.02%	0.003%
64	10.567	2955	2963	2978	rVV2	7497	12022	0.90%	0.109%
65	10.712	3003	3008	3013	rBV2	269	249	0.02%	0.002%
66	10.786	3028	3031	3033	rBV	247	184	0.01%	0.002%
67	10.902	3065	3067	3071	rBV2	343	207	0.02%	0.002%
68	10.998	3094	3097	3102	rVB2	228	224	0.02%	0.002%
69	11.040	3107	3110	3113	rBV2	270	185	0.01%	0.002%
70	11.236	3160	3171	3195	rVV	796635	1221774	91.76%	11.114%
71	11.496	3249	3252	3256	rBV3	294	234	0.02%	0.002%
72	11.558	3268	3271	3274	rBV2	466	344	0.03%	0.003%
73	11.612	3274	3288	3316	rVV	634558	1035468	77.77%	9.419%
74	11.770	3334	3337	3342	rVB3	420	286	0.02%	0.003%
75	11.792	3342	3344	3348	rBV3	381	206	0.02%	0.002%
76	11.889	3370	3374	3380	rVB2	373	278	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029732.D
 Acq On : 19 Dec 2022 19:20
 Operator : SY/MD
 Sample : N6075-13 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

77	11.988	3399	3405	3409	rBV3	440	540	0.04%	0.005%
78	12.050	3420	3424	3426	rBV2	271	183	0.01%	0.002%
79	12.278	3492	3495	3498	rBV	312	236	0.02%	0.002%
80	12.336	3505	3513	3521	rBV5	1310	1910	0.14%	0.017%
81	12.419	3536	3539	3540	rBV2	328	174	0.01%	0.002%
82	12.471	3551	3555	3558	rBV2	430	462	0.03%	0.004%
83	12.487	3558	3560	3566	rVB5	349	277	0.02%	0.003%
84	12.532	3571	3574	3577	rBV2	253	215	0.02%	0.002%
85	12.631	3601	3605	3610	rVB3	566	388	0.03%	0.004%
86	12.914	3689	3693	3696	rBV4	335	320	0.02%	0.003%
87	13.008	3719	3722	3726	rVB3	398	344	0.03%	0.003%
88	13.030	3726	3729	3730	rBV2	357	186	0.01%	0.002%
89	13.130	3755	3760	3763	rBV3	514	532	0.04%	0.005%
90	13.185	3774	3777	3779	rBV3	288	224	0.02%	0.002%
91	13.358	3828	3831	3833	rBV2	298	208	0.02%	0.002%
92	13.419	3848	3850	3853	rVB2	397	184	0.01%	0.002%
93	13.480	3866	3869	3871	rBV2	561	327	0.02%	0.003%
94	13.493	3871	3873	3875	rBV2	393	250	0.02%	0.002%
95	13.574	3895	3898	3902	rBV2	561	418	0.03%	0.004%
96	13.673	3926	3929	3933	rBV2	380	372	0.03%	0.003%
97	13.786	3961	3964	3972	rBV4	519	694	0.05%	0.006%
98	14.033	4033	4041	4049	rVB2	1539	2530	0.19%	0.023%
99	14.178	4084	4086	4087	rBV	477	188	0.01%	0.002%
100	14.300	4121	4124	4125	rBV2	552	255	0.02%	0.002%




Sum of corrected areas: 10993128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029732.D
Acq On : 19 Dec 2022 19:20
Operator : SY/MD
Sample : N6075-13 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

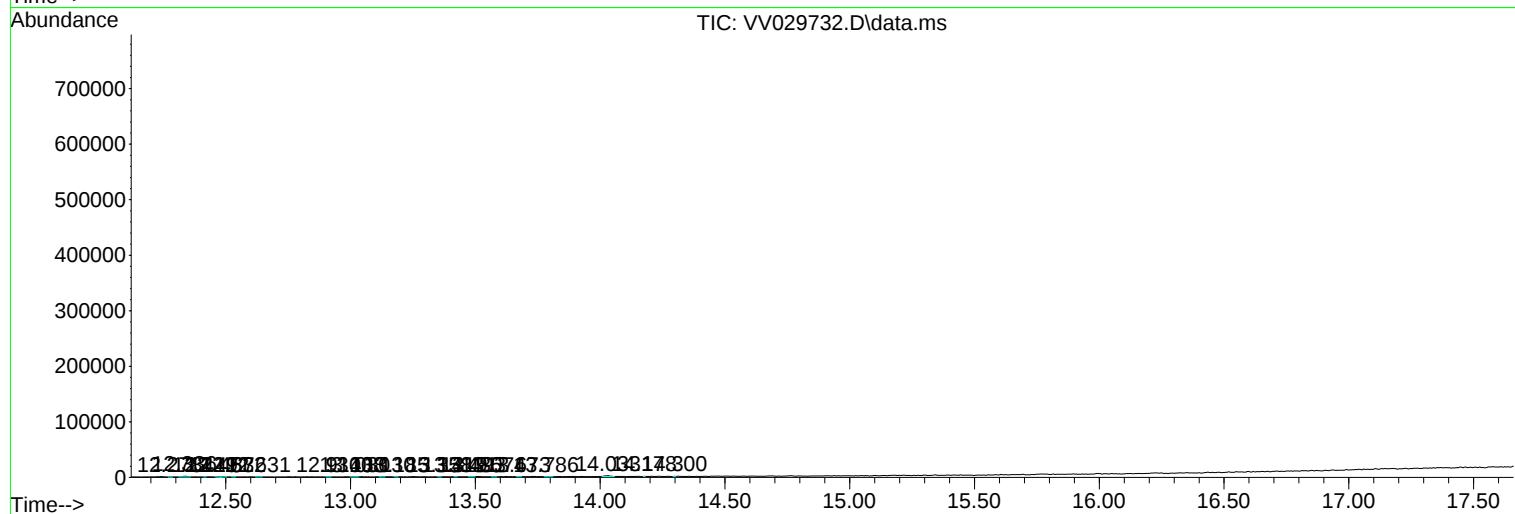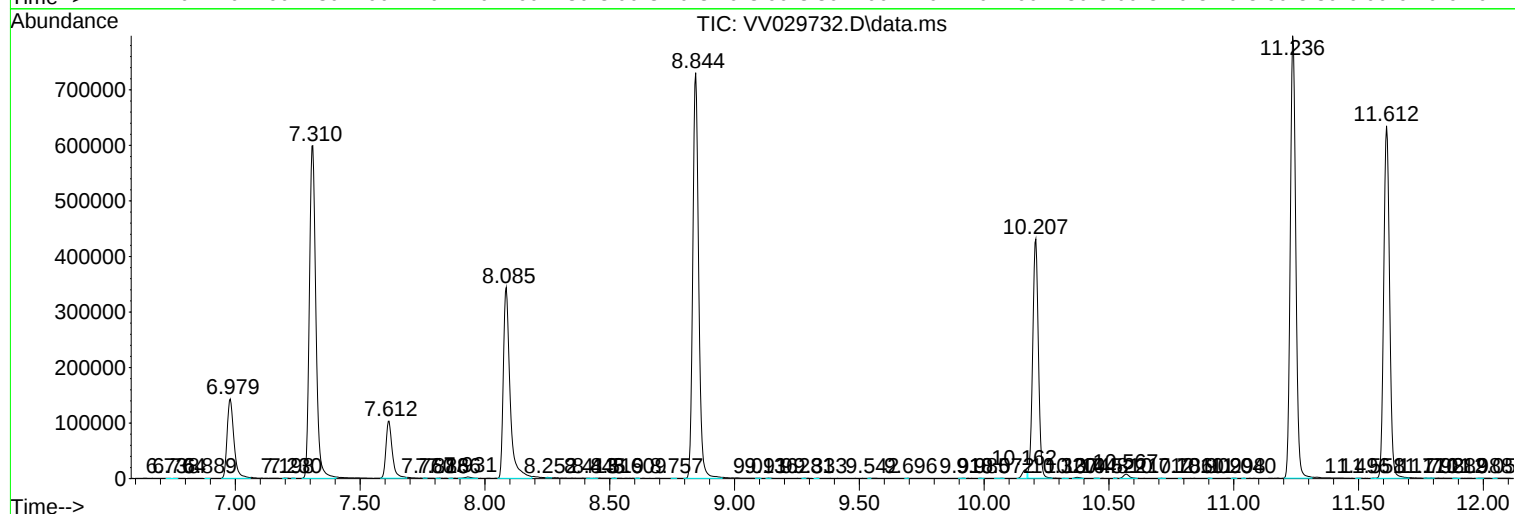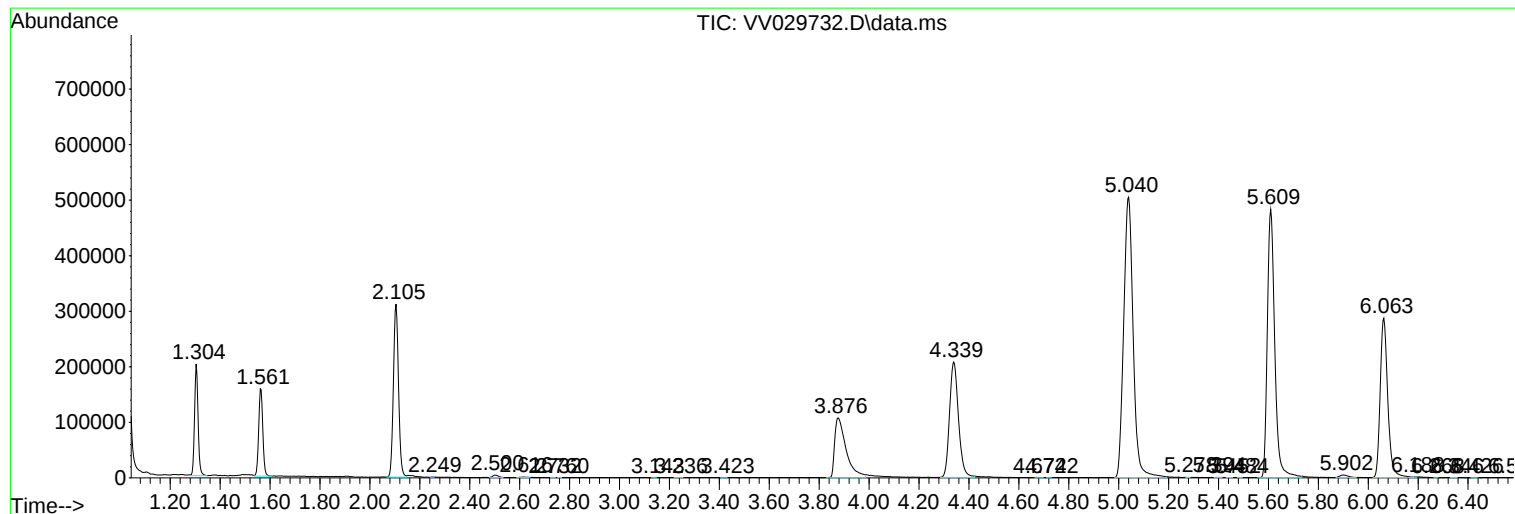

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029732.D
Acq On : 19 Dec 2022 19:20
Operator : SY/MD
Sample : N6075-13 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029732.D
Acq On : 19 Dec 2022 19:20
Operator : SY/MD
Sample : N6075-13 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------