

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029733.D
 Acq On : 19 Dec 2022 19:44
 Operator : SY/MD
 Sample : N6075-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VW029733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	202870	197735	13.91%	1.696%
2	1.561	155	162	177	rVB	172709	193181	13.59%	1.657%
3	2.105	320	331	344	rBV	328010	468487	32.97%	4.018%
4	2.503	447	455	465	rVB	5311	8021	0.56%	0.069%
5	2.558	468	472	477	rBV2	184	155	0.01%	0.001%
6	2.584	479	480	481	rVB	315	61	0.00%	0.001%
7	2.616	481	490	491	rBV2	1273	1717	0.12%	0.015%
8	2.732	523	526	529	rVB3	275	185	0.01%	0.002%
9	2.818	549	553	559	rVB3	282	215	0.02%	0.002%
10	2.950	591	594	596	rBV2	166	105	0.01%	0.001%
11	2.995	605	608	614	rVB2	158	111	0.01%	0.001%
12	3.024	614	617	619	rBV2	231	142	0.01%	0.001%
13	3.082	632	635	637	rBV2	246	103	0.01%	0.001%
14	3.105	639	642	644	rBV	242	135	0.01%	0.001%
15	3.169	653	662	664	rBV2	228	324	0.02%	0.003%
16	3.227	675	680	684	rBV2	211	221	0.02%	0.002%
17	3.301	696	703	706	rBV2	191	219	0.02%	0.002%
18	3.323	708	710	713	rVV2	112	69	0.00%	0.001%
19	3.400	730	734	739	rVB2	298	318	0.02%	0.003%
20	3.429	739	743	745	rBV2	126	112	0.01%	0.001%
21	3.490	758	762	765	rBV2	145	155	0.01%	0.001%
22	3.536	771	776	779	rBV2	192	178	0.01%	0.002%
23	3.577	786	789	791	rBV2	120	75	0.01%	0.001%
24	3.638	802	808	810	rBV2	108	120	0.01%	0.001%
25	3.876	869	882	934	rBV2	122703	403876	28.42%	3.464%
26	4.339	1010	1026	1054	rBV	221253	548552	38.60%	4.705%
27	4.584	1099	1102	1105	rVB2	419	306	0.02%	0.003%
28	4.606	1105	1109	1110	rBV2	227	171	0.01%	0.001%
29	4.671	1124	1129	1130	rBV	291	219	0.02%	0.002%
30	4.764	1155	1158	1163	rVB2	153	137	0.01%	0.001%
31	4.822	1172	1176	1178	rBV	153	89	0.01%	0.001%
32	4.857	1185	1187	1189	rVB	178	78	0.01%	0.001%
33	4.880	1191	1194	1197	rBV2	144	102	0.01%	0.001%
34	4.925	1205	1208	1213	rBV3	235	181	0.01%	0.002%
35	4.960	1213	1219	1224	rBV3	261	347	0.02%	0.003%
36	5.037	1225	1243	1286	rBV2	534238	1421071	100.00%	12.189%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029733.D
 Acq On : 19 Dec 2022 19:44
 Operator : SY/MD
 Sample : N6075-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.465	1374	1376	1378	rBV	278	149	0.01%	0.001%
38	5.535	1395	1398	1401	rVV2	290	198	0.01%	0.002%
39	5.609	1408	1421	1465	rBV	499251	1032056	72.63%	8.852%
40	5.899	1502	1511	1526	rVB4	5101	11032	0.78%	0.095%
41	6.063	1547	1562	1594	rBV	309148	645797	45.44%	5.539%
42	6.288	1627	1632	1637	rBV2	208	207	0.01%	0.002%
43	6.326	1642	1644	1648	rVB2	245	131	0.01%	0.001%
44	6.365	1654	1656	1658	rVB2	202	65	0.00%	0.001%
45	6.503	1697	1699	1703	rBV2	152	78	0.01%	0.001%
46	6.523	1703	1705	1708	rBV	139	110	0.01%	0.001%
47	6.600	1726	1729	1733	rBV	116	121	0.01%	0.001%
48	6.622	1733	1736	1739	rBV2	219	154	0.01%	0.001%
49	6.641	1739	1742	1745	rBV4	401	234	0.02%	0.002%
50	6.690	1754	1757	1758	rBV	243	90	0.01%	0.001%
51	6.725	1767	1768	1772	rVB	191	84	0.01%	0.001%
52	6.777	1783	1784	1789	rVB2	178	107	0.01%	0.001%
53	6.854	1805	1808	1811	rBV	179	126	0.01%	0.001%
54	6.870	1811	1813	1819	rVV	199	168	0.01%	0.001%
55	6.924	1827	1830	1835	rBV2	159	164	0.01%	0.001%
56	6.979	1835	1847	1872	rBV	152748	282224	19.86%	2.421%
57	7.153	1896	1901	1904	rBV4	622	669	0.05%	0.006%
58	7.307	1934	1949	1982	rBV	650778	1151703	81.04%	9.878%
59	7.568	2028	2030	2033	rBV2	599	328	0.02%	0.003%
60	7.613	2034	2044	2069	rVV	108619	191927	13.51%	1.646%
61	7.889	2127	2130	2133	rBV2	335	314	0.02%	0.003%
62	7.937	2136	2145	2153	rVB4	2248	4060	0.29%	0.035%
63	8.085	2180	2191	2229	rBV	382615	708424	49.85%	6.076%
64	8.461	2306	2308	2312	rVB3	435	283	0.02%	0.002%
65	8.506	2320	2322	2325	rBV3	410	240	0.02%	0.002%
66	8.526	2325	2328	2332	rVV3	463	359	0.03%	0.003%
67	8.548	2334	2335	2337	rVB2	276	103	0.01%	0.001%
68	8.590	2346	2348	2349	rBV	236	93	0.01%	0.001%
69	8.622	2356	2358	2359	rBV	154	63	0.00%	0.001%
70	8.648	2363	2366	2368	rBV	161	88	0.01%	0.001%
71	8.722	2386	2389	2393	rBV3	276	216	0.02%	0.002%
72	8.844	2413	2427	2454	rBV	748029	1230345	86.58%	10.553%
73	9.169	2526	2528	2530	rBV	266	116	0.01%	0.001%
74	9.236	2546	2549	2550	rBV	162	101	0.01%	0.001%
75	9.272	2557	2560	2562	rBV2	338	170	0.01%	0.001%
76	9.313	2570	2573	2577	rBV	243	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
 Data File : VV029733.D
 Acq On : 19 Dec 2022 19:44
 Operator : SY/MD
 Sample : N6075-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.333	2577	2579	2582	rVB2	191	85	0.01%	0.001%
78	9.397	2596	2599	2601	rBV2	390	202	0.01%	0.002%
79	9.439	2608	2612	2616	rBV	290	231	0.02%	0.002%
80	9.461	2616	2619	2621	rBV	212	124	0.01%	0.001%
81	9.567	2649	2652	2657	rBV3	231	219	0.02%	0.002%
82	9.715	2696	2698	2701	rBV	209	100	0.01%	0.001%
83	9.757	2708	2711	2714	rBV3	223	145	0.01%	0.001%
84	9.873	2745	2747	2750	rBV2	156	99	0.01%	0.001%
85	10.165	2825	2838	2841	rBV2	16545	23981	1.69%	0.206%
86	10.207	2841	2851	2873	rVB	467658	734559	51.69%	6.300%
87	10.374	2897	2903	2911	rVB5	1714	2435	0.17%	0.021%
88	10.522	2948	2949	2950	rBV5	276	85	0.01%	0.001%
89	10.567	2956	2963	2977	rVB2	7695	12350	0.87%	0.106%
90	10.831	3043	3045	3046	rBV2	203	81	0.01%	0.001%
91	10.866	3053	3056	3059	rBV	299	247	0.02%	0.002%
92	10.911	3066	3070	3079	rVB3	708	715	0.05%	0.006%
93	10.950	3080	3082	3084	rBV	173	98	0.01%	0.001%
94	11.175	3149	3152	3153	rBV	472	257	0.02%	0.002%
95	11.239	3159	3172	3197	rBV	821891	1263580	88.92%	10.838%
96	11.551	3268	3269	3275	rBV2	320	224	0.02%	0.002%
97	11.612	3276	3288	3313	rBV	704467	1107624	77.94%	9.500%
98	11.908	3377	3380	3382	rBV3	504	304	0.02%	0.003%
99	12.111	3438	3443	3448	rVB2	417	425	0.03%	0.004%
100	13.249	3794	3797	3801	rBV3	759	612	0.04%	0.005%




Sum of corrected areas: 11659084

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029733.D
Acq On : 19 Dec 2022 19:44
Operator : SY/MD
Sample : N6075-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

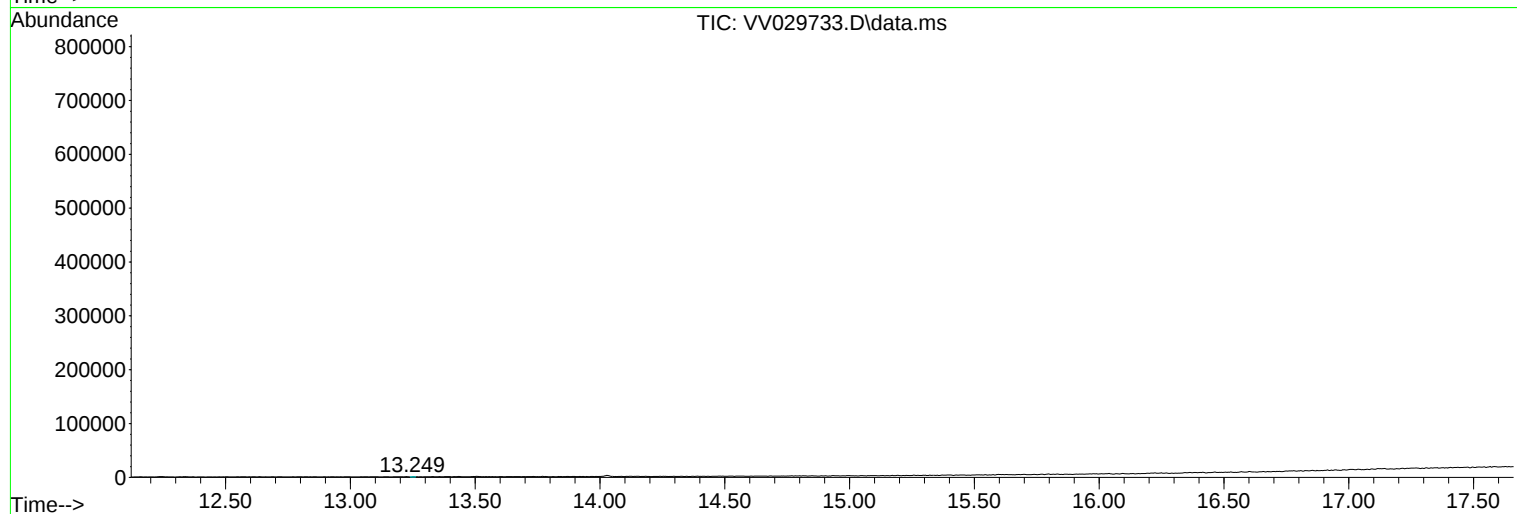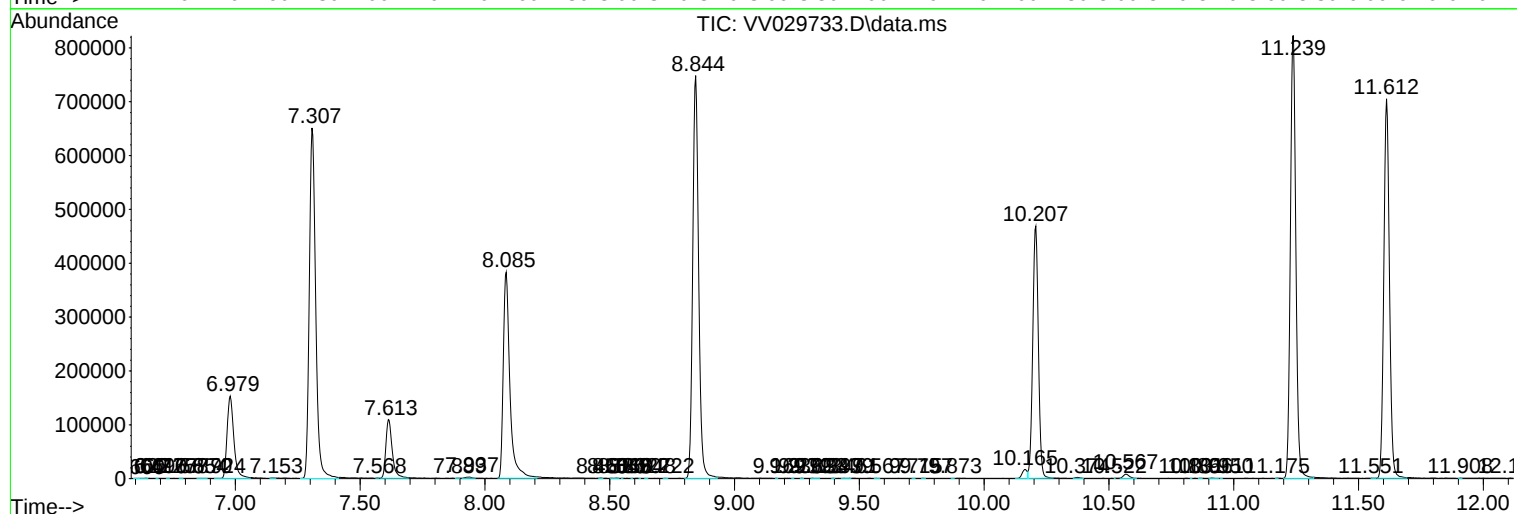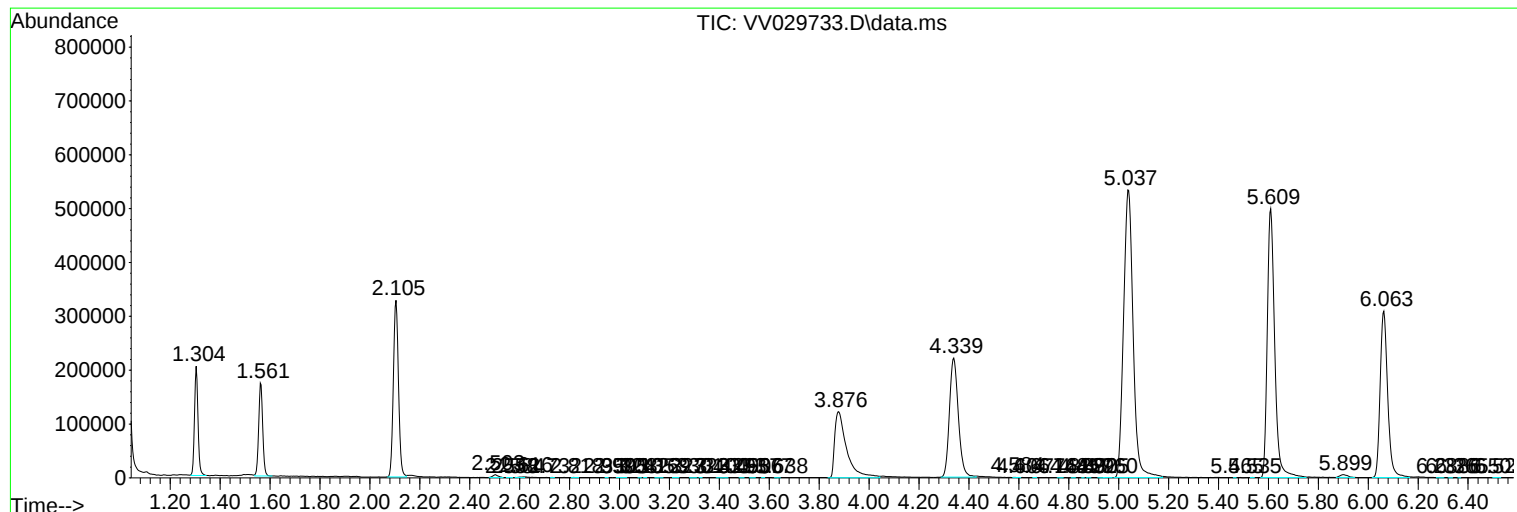

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029733.D
Acq On : 19 Dec 2022 19:44
Operator : SY/MD
Sample : N6075-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029733.D
Acq On : 19 Dec 2022 19:44
Operator : SY/MD
Sample : N6075-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------