

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
 Data File : VV029734.D
 Acq On : 19 Dec 2022 20:07
 Operator : SY/MD
 Sample : N6075-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	199374	194686	14.11%	1.724%
2	1.564	155	163	177	rVB	162683	183647	13.31%	1.626%
3	2.105	320	331	344	rBV	318095	457441	33.15%	4.050%
4	2.507	447	456	468	rVB3	4056	6737	0.49%	0.060%
5	2.561	470	473	476	rVB2	348	211	0.02%	0.002%
6	2.577	476	478	481	rBV2	128	98	0.01%	0.001%
7	2.609	482	488	500	rVB4	1154	2336	0.17%	0.021%
8	2.699	512	516	520	rBV	273	257	0.02%	0.002%
9	2.773	534	539	543	rVB3	382	336	0.02%	0.003%
10	2.908	577	581	587	rBV	214	246	0.02%	0.002%
11	3.002	605	610	613	rBV2	130	140	0.01%	0.001%
12	3.053	625	626	630	rVB2	176	79	0.01%	0.001%
13	3.207	671	674	677	rVB2	150	107	0.01%	0.001%
14	3.494	758	763	765	rBV	147	127	0.01%	0.001%
15	3.555	776	782	786	rBV2	202	247	0.02%	0.002%
16	3.587	790	792	795	rVB2	195	105	0.01%	0.001%
17	3.613	795	800	801	rBV2	93	80	0.01%	0.001%
18	3.683	815	822	824	rBV2	117	145	0.01%	0.001%
19	3.696	824	826	832	rVV	222	158	0.01%	0.001%
20	3.738	835	839	843	rVB2	117	114	0.01%	0.001%
21	3.773	848	850	854	rVB	124	77	0.01%	0.001%
22	3.876	871	882	920	rBV2	115621	363290	26.33%	3.217%
23	4.339	1009	1026	1054	rBV2	214554	533275	38.65%	4.722%
24	4.580	1098	1101	1102	rBV	499	271	0.02%	0.002%
25	4.661	1124	1126	1130	rVB3	378	230	0.02%	0.002%
26	4.696	1132	1137	1140	rBV3	247	303	0.02%	0.003%
27	4.735	1146	1149	1151	rBV	226	111	0.01%	0.001%
28	4.850	1181	1185	1190	rBV	313	250	0.02%	0.002%
29	4.899	1197	1200	1203	rVB2	121	71	0.01%	0.001%
30	4.921	1203	1207	1212	rVB2	239	168	0.01%	0.001%
31	4.950	1212	1216	1221	rVB2	213	175	0.01%	0.002%
32	4.973	1221	1223	1225	rBV2	132	78	0.01%	0.001%
33	5.040	1225	1244	1291	rBV2	517242	1379858	100.00%	12.218%
34	5.320	1328	1331	1333	rBV	297	176	0.01%	0.002%
35	5.420	1360	1362	1364	rBV	167	91	0.01%	0.001%
36	5.465	1372	1376	1385	rVB3	335	460	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121922\
 Data File : VW029734.D
 Acq On : 19 Dec 2022 20:07
 Operator : SY/MD
 Sample : N6075-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.510	1385	1390	1394	rBV2	150	211	0.02%	0.002%
38	5.564	1402	1407	1408	rBV	127	83	0.01%	0.001%
39	5.609	1408	1421	1468	rBV	491780	1015454	73.59%	8.991%
40	5.899	1502	1511	1527	rVB4	4928	10722	0.78%	0.095%
41	5.985	1536	1538	1540	rBV	193	89	0.01%	0.001%
42	6.063	1548	1562	1599	rBV	299651	624102	45.23%	5.526%
43	6.307	1637	1638	1644	rVB2	163	95	0.01%	0.001%
44	6.355	1651	1653	1656	rVB	257	117	0.01%	0.001%
45	6.535	1706	1709	1711	rBV2	169	99	0.01%	0.001%
46	6.596	1725	1728	1731	rBV	132	73	0.01%	0.001%
47	6.619	1731	1735	1737	rBV2	283	188	0.01%	0.002%
48	6.686	1752	1756	1758	rBV	269	227	0.02%	0.002%
49	6.789	1785	1788	1793	rBV2	223	195	0.01%	0.002%
50	6.850	1805	1807	1809	rBV2	152	87	0.01%	0.001%
51	6.915	1822	1827	1828	rBV	217	158	0.01%	0.001%
52	6.979	1836	1847	1880	rBV	148074	274629	19.90%	2.432%
53	7.124	1889	1892	1897	rVB4	614	478	0.03%	0.004%
54	7.310	1936	1950	1972	rBV	623709	1106956	80.22%	9.801%
55	7.612	2034	2044	2067	rBV	103584	185745	13.46%	1.645%
56	7.751	2085	2087	2091	rVB2	448	254	0.02%	0.002%
57	7.831	2107	2112	2114	rBV3	340	327	0.02%	0.003%
58	7.937	2137	2145	2153	rBV4	2299	3823	0.28%	0.034%
59	8.085	2180	2191	2229	rBV	357699	665100	48.20%	5.889%
60	8.362	2275	2277	2278	rBV	535	205	0.01%	0.002%
61	8.455	2302	2306	2309	rVB3	487	393	0.03%	0.003%
62	8.542	2330	2333	2338	rVB4	475	326	0.02%	0.003%
63	8.580	2344	2345	2348	rBV	237	82	0.01%	0.001%
64	8.638	2360	2363	2367	rBV2	286	225	0.02%	0.002%
65	8.661	2367	2370	2375	rVV2	534	415	0.03%	0.004%
66	8.709	2383	2385	2387	rBV2	255	117	0.01%	0.001%
67	8.728	2390	2391	2394	rVB2	223	71	0.01%	0.001%
68	8.764	2400	2402	2404	rBV	259	112	0.01%	0.001%
69	8.776	2404	2406	2409	rVB	213	140	0.01%	0.001%
70	8.844	2411	2427	2452	rBV	723166	1205462	87.36%	10.674%
71	9.181	2529	2532	2535	rVV2	163	115	0.01%	0.001%
72	9.252	2552	2554	2558	rBV2	279	202	0.01%	0.002%
73	9.333	2577	2579	2581	rBV2	281	146	0.01%	0.001%
74	9.442	2611	2613	2616	rVB	227	76	0.01%	0.001%
75	9.513	2634	2635	2637	rBV	216	71	0.01%	0.001%
76	9.526	2637	2639	2643	rVV2	499	320	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
 Data File : VV029734.D
 Acq On : 19 Dec 2022 20:07
 Operator : SY/MD
 Sample : N6075-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.545	2643	2645	2648	rVV3	307	137	0.01%	0.001%
78	9.564	2648	2651	2654	rVB3	325	221	0.02%	0.002%
79	9.664	2680	2682	2684	rVB2	177	77	0.01%	0.001%
80	9.712	2694	2697	2698	rBV	211	123	0.01%	0.001%
81	9.854	2738	2741	2744	rBV	295	167	0.01%	0.001%
82	9.921	2758	2762	2763	rBV	293	202	0.01%	0.002%
83	10.162	2828	2837	2840	rBV	15316	20047	1.45%	0.178%
84	10.207	2842	2851	2875	rVB	453153	705274	51.11%	6.245%
85	10.374	2894	2903	2910	rBV4	2495	3186	0.23%	0.028%
86	10.571	2956	2964	2975	rVB2	7368	11557	0.84%	0.102%
87	10.902	3064	3067	3070	rBV2	456	296	0.02%	0.003%
88	11.120	3131	3135	3138	rBV3	290	235	0.02%	0.002%
89	11.143	3139	3142	3144	rBV	247	157	0.01%	0.001%
90	11.239	3159	3172	3203	rBV	788359	1253926	90.87%	11.103%
91	11.445	3232	3236	3238	rBV2	373	257	0.02%	0.002%
92	11.490	3247	3250	3253	rBV2	292	196	0.01%	0.002%
93	11.532	3261	3263	3266	rBV	242	171	0.01%	0.002%
94	11.564	3269	3273	3276	rBV	389	406	0.03%	0.004%
95	11.612	3276	3288	3308	rBV	680469	1072346	77.71%	9.495%
96	12.008	3409	3411	3413	rBV	318	132	0.01%	0.001%
97	12.329	3509	3511	3512	rBV	460	187	0.01%	0.002%
98	12.638	3604	3607	3608	rBV2	571	297	0.02%	0.003%
99	13.053	3733	3736	3740	rBV2	537	382	0.03%	0.003%
100	13.580	3898	3900	3901	rBV	489	100	0.01%	0.001%




Sum of corrected areas: 11293950

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029734.D
Acq On : 19 Dec 2022 20:07
Operator : SY/MD
Sample : N6075-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

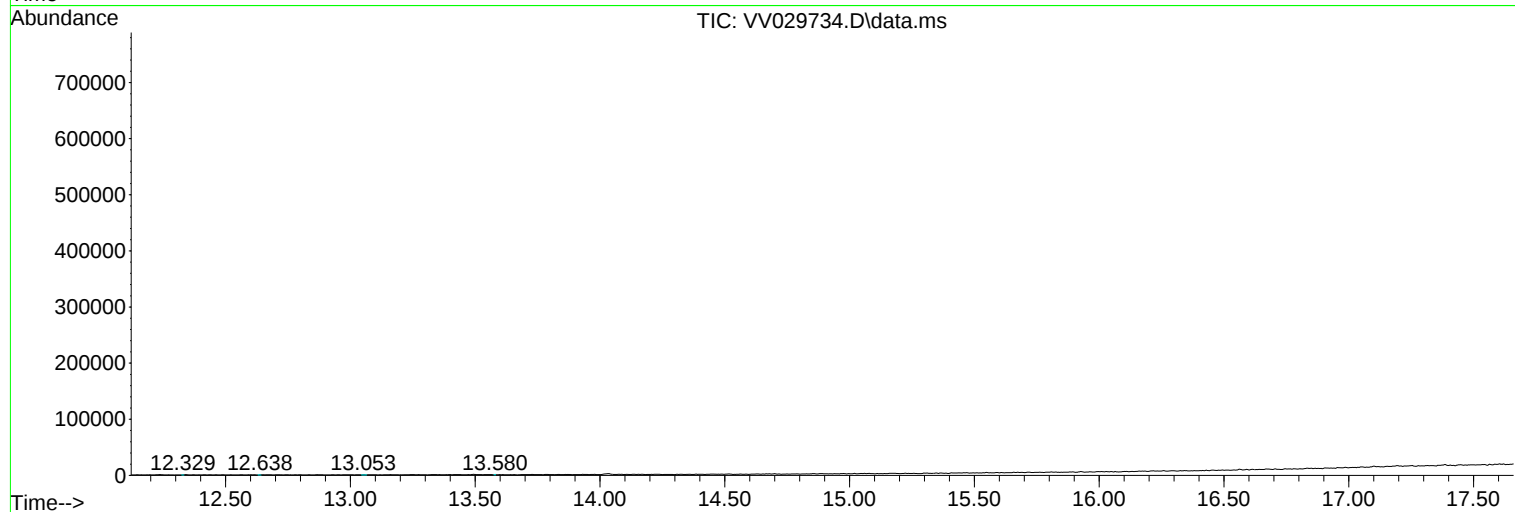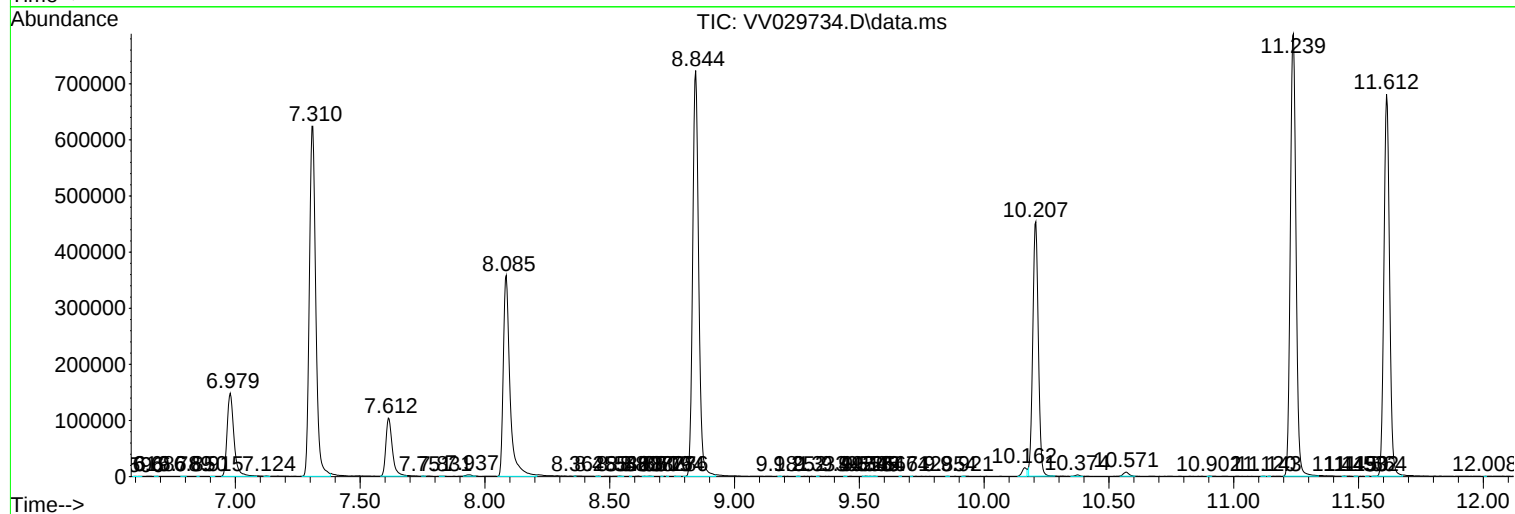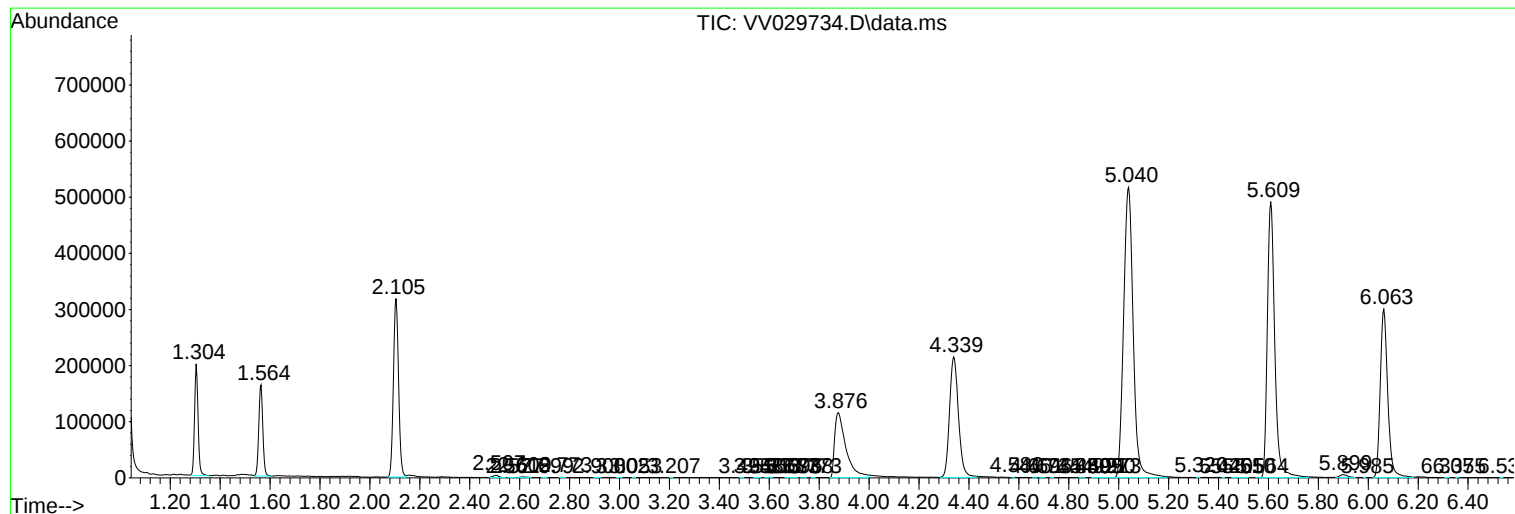

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029734.D
Acq On : 19 Dec 2022 20:07
Operator : SY/MD
Sample : N6075-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029734.D
Acq On : 19 Dec 2022 20:07
Operator : SY/MD
Sample : N6075-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------