
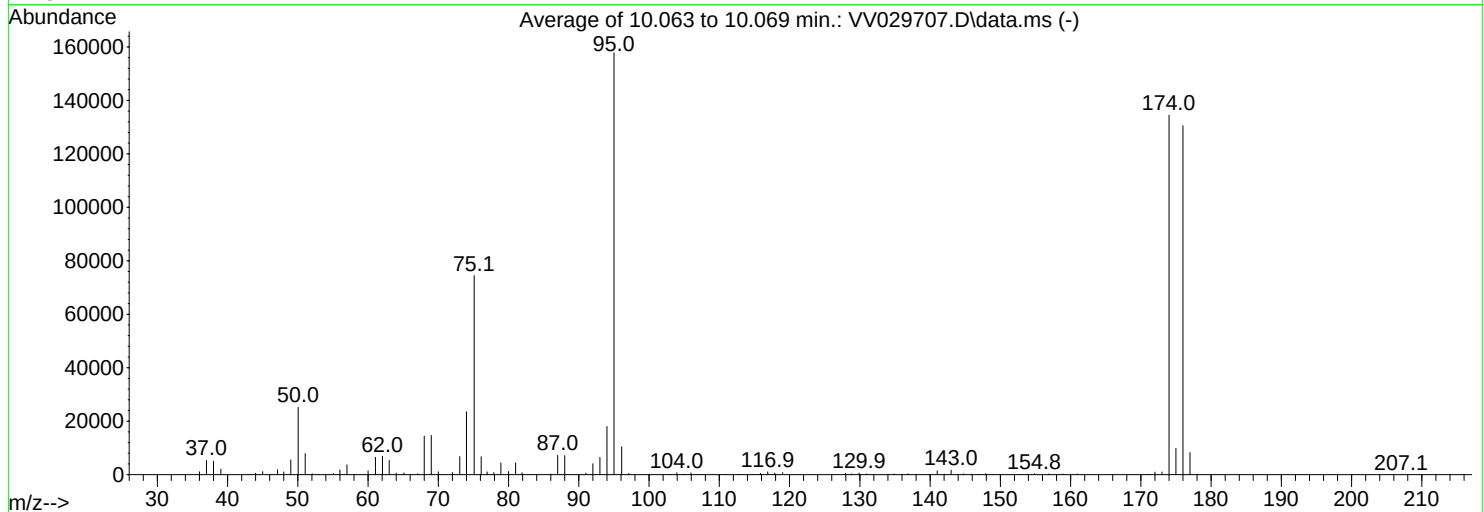


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121922\
Data File : VV029707.D
Acq On : 19 Dec 2022 09:08
Operator : SY/MD
Sample : BFB357
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB357

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Title : VOC Analysis
Last Update : Wed Dec 21 00:15:13 2022

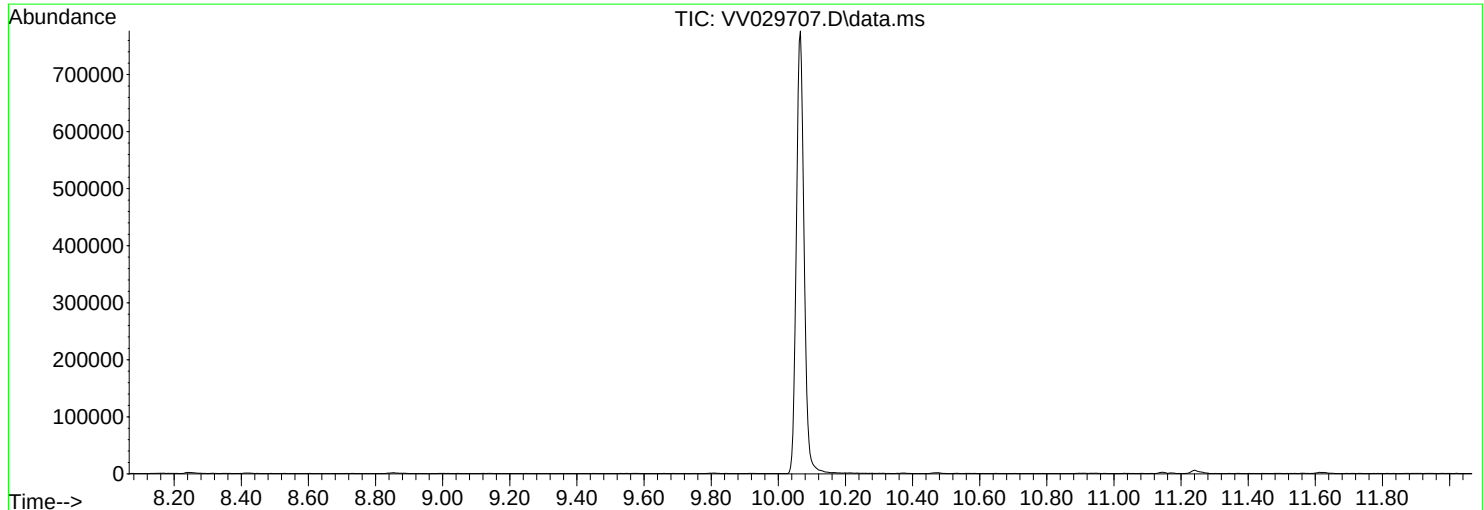

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	25189	PASS
75	95	30	80	47.2	74443	PASS
95	95	100	100	100.0	157803	PASS
96	95	5	9	6.6	10431	PASS
173	174	0.00	2	0.8	1050	PASS
174	95	50	120	85.2	134421	PASS
175	174	5	9	7.3	9845	PASS
176	174	95	105	97.1	130576	PASS
177	176	5	10	6.3	8247	PASS

m/z	Abundance
39.90	267.0
44.00	414.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

m/z	Abundance
36.00	1000.0
37.00	5502.0
38.00	5193.0
39.10	2175.0
40.00	269.0
42.90	105.0
44.00	925.0
45.00	1212.0
46.10	103.0
47.10	1717.0
48.00	1082.0
49.00	5605.0
50.10	25960.0
51.10	8012.0
52.00	333.0
52.90	139.0
55.10	403.0
56.00	1820.0
57.00	3710.0
58.20	124.0
60.00	1388.0
61.00	6664.0
62.10	6985.0
63.00	5445.0
64.00	640.0
65.10	747.0
67.10	322.0
68.00	14751.0
69.00	14770.0
70.00	1107.0
72.00	836.0
73.00	7019.0
74.00	24200.0
75.10	76224.0
76.10	6847.0
76.90	1059.0
77.90	733.0
78.90	4504.0
80.00	1110.0
81.00	4596.0
81.90	714.0
83.10	114.0
86.00	238.0
87.00	7381.0
88.00	7432.0
91.00	555.0
92.00	4046.0
93.00	6593.0
94.00	18264.0
95.00	160064.0
96.10	10904.0
97.10	381.0
104.00	694.0
105.00	167.0
106.00	688.0
106.90	154.0
110.10	111.0
110.90	176.0
112.70	134.0
114.70	131.0
115.90	547.0
116.90	1011.0
117.90	580.0
119.00	688.0
128.00	574.0
128.90	310.0
129.90	629.0
131.00	270.0
134.90	249.0
136.80	268.0
141.00	1415.0
142.10	197.0
143.00	1672.0
143.80	119.0
144.80	336.0
145.80	195.0
146.90	109.0
147.90	395.0
148.90	116.0
150.00	133.0
153.80	120.0
154.90	396.0
156.90	225.0
158.90	203.0
160.90	232.0
171.00	108.0
172.00	892.0
173.00	1500.0
174.00	133056.0
175.00	9597.0
176.00	128896.0
177.00	8215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

178.00

217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

m/z	Abundance
36.00	1138.0
37.00	5500.0
38.00	5206.0
39.00	2089.0
39.90	267.0
43.00	121.0
44.00	973.0
45.00	1185.0
47.10	1907.0
48.00	1051.0
49.00	5722.0
50.10	25960.0
51.00	8178.0
52.00	330.0
52.90	138.0
55.10	413.0
56.00	1874.0
57.00	3804.0
58.20	146.0
60.00	1430.0
61.10	6713.0
62.10	7096.0
63.00	5557.0
64.00	661.0
65.10	685.0
67.10	289.0
68.00	14839.0
69.00	15113.0
70.00	1077.0
72.00	786.0
73.10	6932.0
74.00	24112.0
75.10	76808.0
76.10	6866.0
77.00	1087.0
77.90	817.0
78.90	4539.0
80.00	1201.0
81.00	4552.0
81.90	758.0
83.00	110.0
86.00	265.0
87.00	7426.0
88.00	7243.0
91.00	539.0
92.00	4137.0
93.00	6664.0
94.00	18688.0
95.00	163072.0
96.10	10735.0
97.10	415.0
103.90	714.0
104.90	193.0
105.90	682.0
107.00	125.0
110.10	131.0
110.90	151.0
112.80	135.0
114.70	103.0
115.90	516.0
116.90	1068.0
117.90	612.0
119.00	788.0
127.90	558.0
128.80	287.0
129.90	646.0
131.00	300.0
134.80	266.0
136.90	296.0
139.80	108.0
141.00	1495.0
142.10	190.0
143.00	1761.0
143.80	123.0
144.80	306.0
145.90	213.0
147.00	110.0
147.90	383.0
150.00	140.0
153.80	114.0
154.80	357.0
156.90	217.0
158.90	227.0
161.00	245.0
171.00	149.0
172.00	1003.0
173.00	1650.0
174.00	138816.0
175.00	10150.0
176.00	134976.0
177.00	8487.0
178.00	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

207.10

119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

m/z	Abundance
36.00	1105.0
37.00	5014.0
38.00	4716.0
39.00	1853.0
39.90	249.0
43.00	140.0
44.00	924.0
45.00	1056.0
47.10	1839.0
48.00	882.0
49.00	5268.0
50.00	23648.0
51.00	7521.0
52.10	319.0
52.90	108.0
55.00	397.0
56.00	1740.0
57.00	3398.0
58.10	140.0
60.00	1314.0
61.10	6076.0
62.00	6341.0
63.00	5010.0
64.00	586.0
65.10	618.0
66.90	314.0
68.00	13713.0
69.00	14070.0
70.00	998.0
72.00	706.0
73.10	6320.0
74.00	22256.0
75.10	70296.0
76.10	6331.0
77.00	1007.0
77.90	757.0
78.90	4013.0
80.00	1150.0
81.00	4059.0
81.90	770.0
86.00	248.0
87.00	6755.0
88.00	6646.0
91.00	464.0
92.00	4022.0
93.00	6084.0
94.00	17192.0
95.00	150272.0
96.10	9655.0
97.10	391.0
103.10	107.0
103.90	699.0
104.90	197.0
105.90	643.0
107.00	105.0
110.00	115.0
110.90	122.0
112.90	147.0
115.80	467.0
116.90	1024.0
117.90	572.0
119.00	796.0
127.90	518.0
128.90	234.0
129.90	554.0
131.00	282.0
134.80	280.0
136.90	292.0
139.80	107.0
141.00	1415.0
141.90	159.0
143.00	1636.0
143.90	112.0
144.80	236.0
145.90	226.0
147.00	112.0
147.90	344.0
150.00	114.0
152.90	102.0
153.80	102.0
154.80	352.0
156.80	230.0
158.90	223.0
161.00	214.0
171.00	148.0
172.00	960.0
174.00	131392.0
175.00	9788.0
176.00	127856.0
177.00	8040.0
178.00	168.0
207.10	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357