
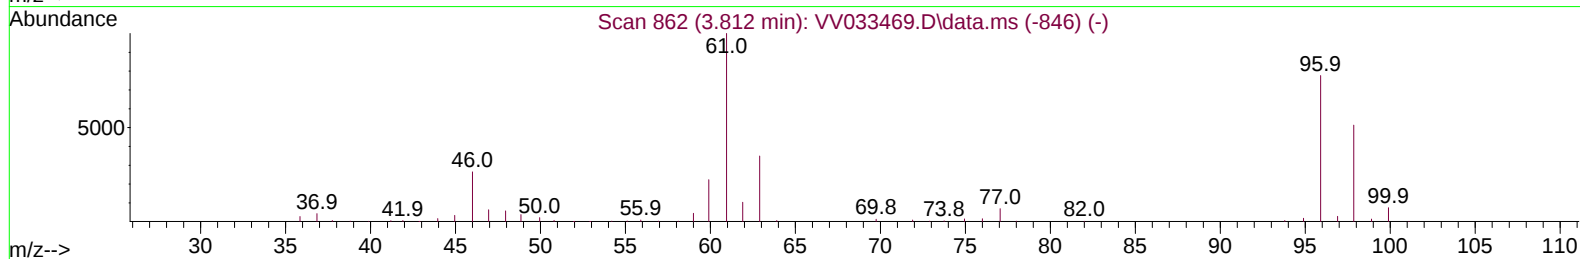
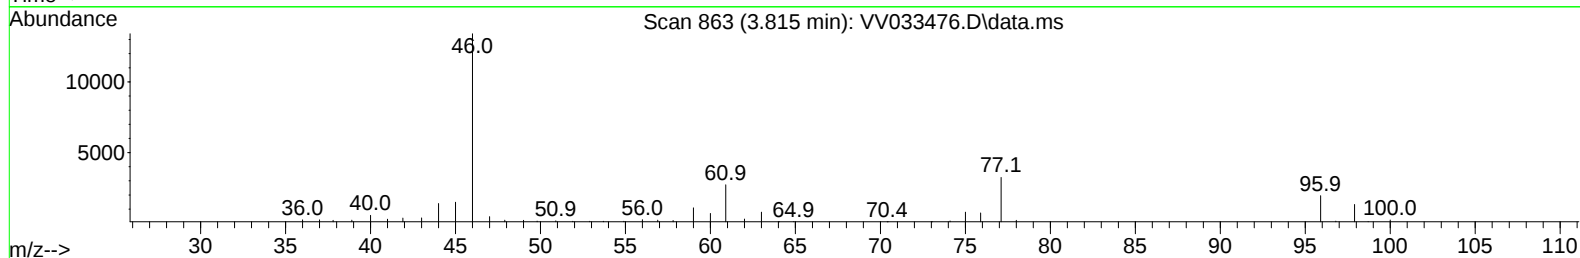


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033476.D
Acq On : 19 Dec 2023 14:35
Operator : SY/MD
Sample : 05912-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 20 00:26:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 20 00:24:21 2023
Response via : Initial Calibration

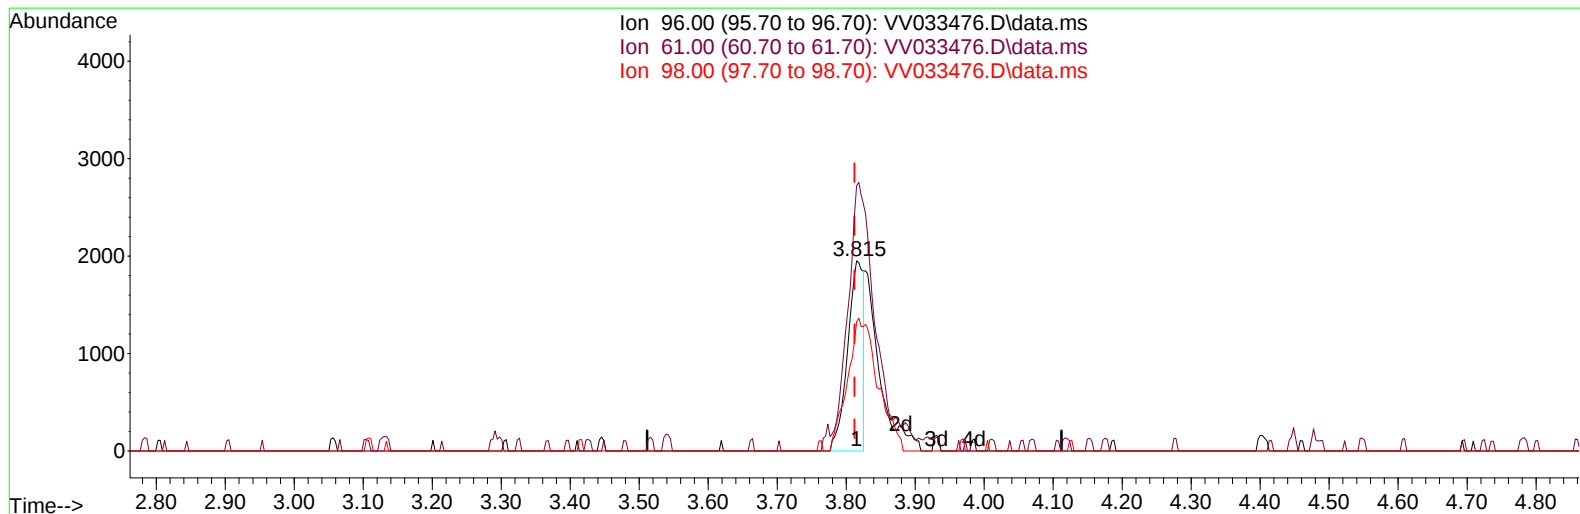

TIC: VV033476.D\data.ms

(20) cis-1,2-Dichloroethene (T)**3.815min (+ 0.003) 1.52 ug/L****response 3068**

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	117.00	139.60
98.00	63.30	74.03
0.00	0.00	0.00