

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033473.D
 Acq On : 19 Dec 2023 13:26
 Operator : SY/MD
 Sample : 05912-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 20 00:25:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 20 00:24:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	278752	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	287024	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	116359	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	109840	51.168	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 102.340%			
7) Chloroethane-d5	1.532	69	94032	48.812	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 97.620%			
11) 1,1-Dichloroethene-d2	2.060	65	48212	45.117	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 90.240%			
21) 2-Butanone-d5	3.786	46	86176	79.654	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 79.650%			
24) Chloroform-d	4.249	84	185063	43.583	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 87.160%			
26) 1,2-Dichloroethane-d4	4.941	65	121569	46.605	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 93.200%			
32) Benzene-d6	4.960	84	361616	46.778	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 93.560%			
36) 1,2-Dichloropropane-d6	5.989	67	115375	49.175	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 98.360%			
41) Toluene-d8	7.243	98	294990	41.703	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 83.400%			
43) trans-1,3-Dichloroprop...	7.551	79	45789	39.822	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 79.640%			
47) 2-Hexanone-d5	8.024	63	57607	73.000	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 73.000%			
56) 1,1,2,2-Tetrachloroeth...	10.153	84	138350	41.028	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 82.060%			
66) 1,2-Dichlorobenzene-d4	11.561	152	109641	50.143	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 100.280%			
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.551	75	2436	0.804	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033473.D
Acq On : 19 Dec 2023 13:26
Operator : SY/MD
Sample : 05912-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 20 00:25:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 20 00:24:21 2023
Response via : Initial Calibration

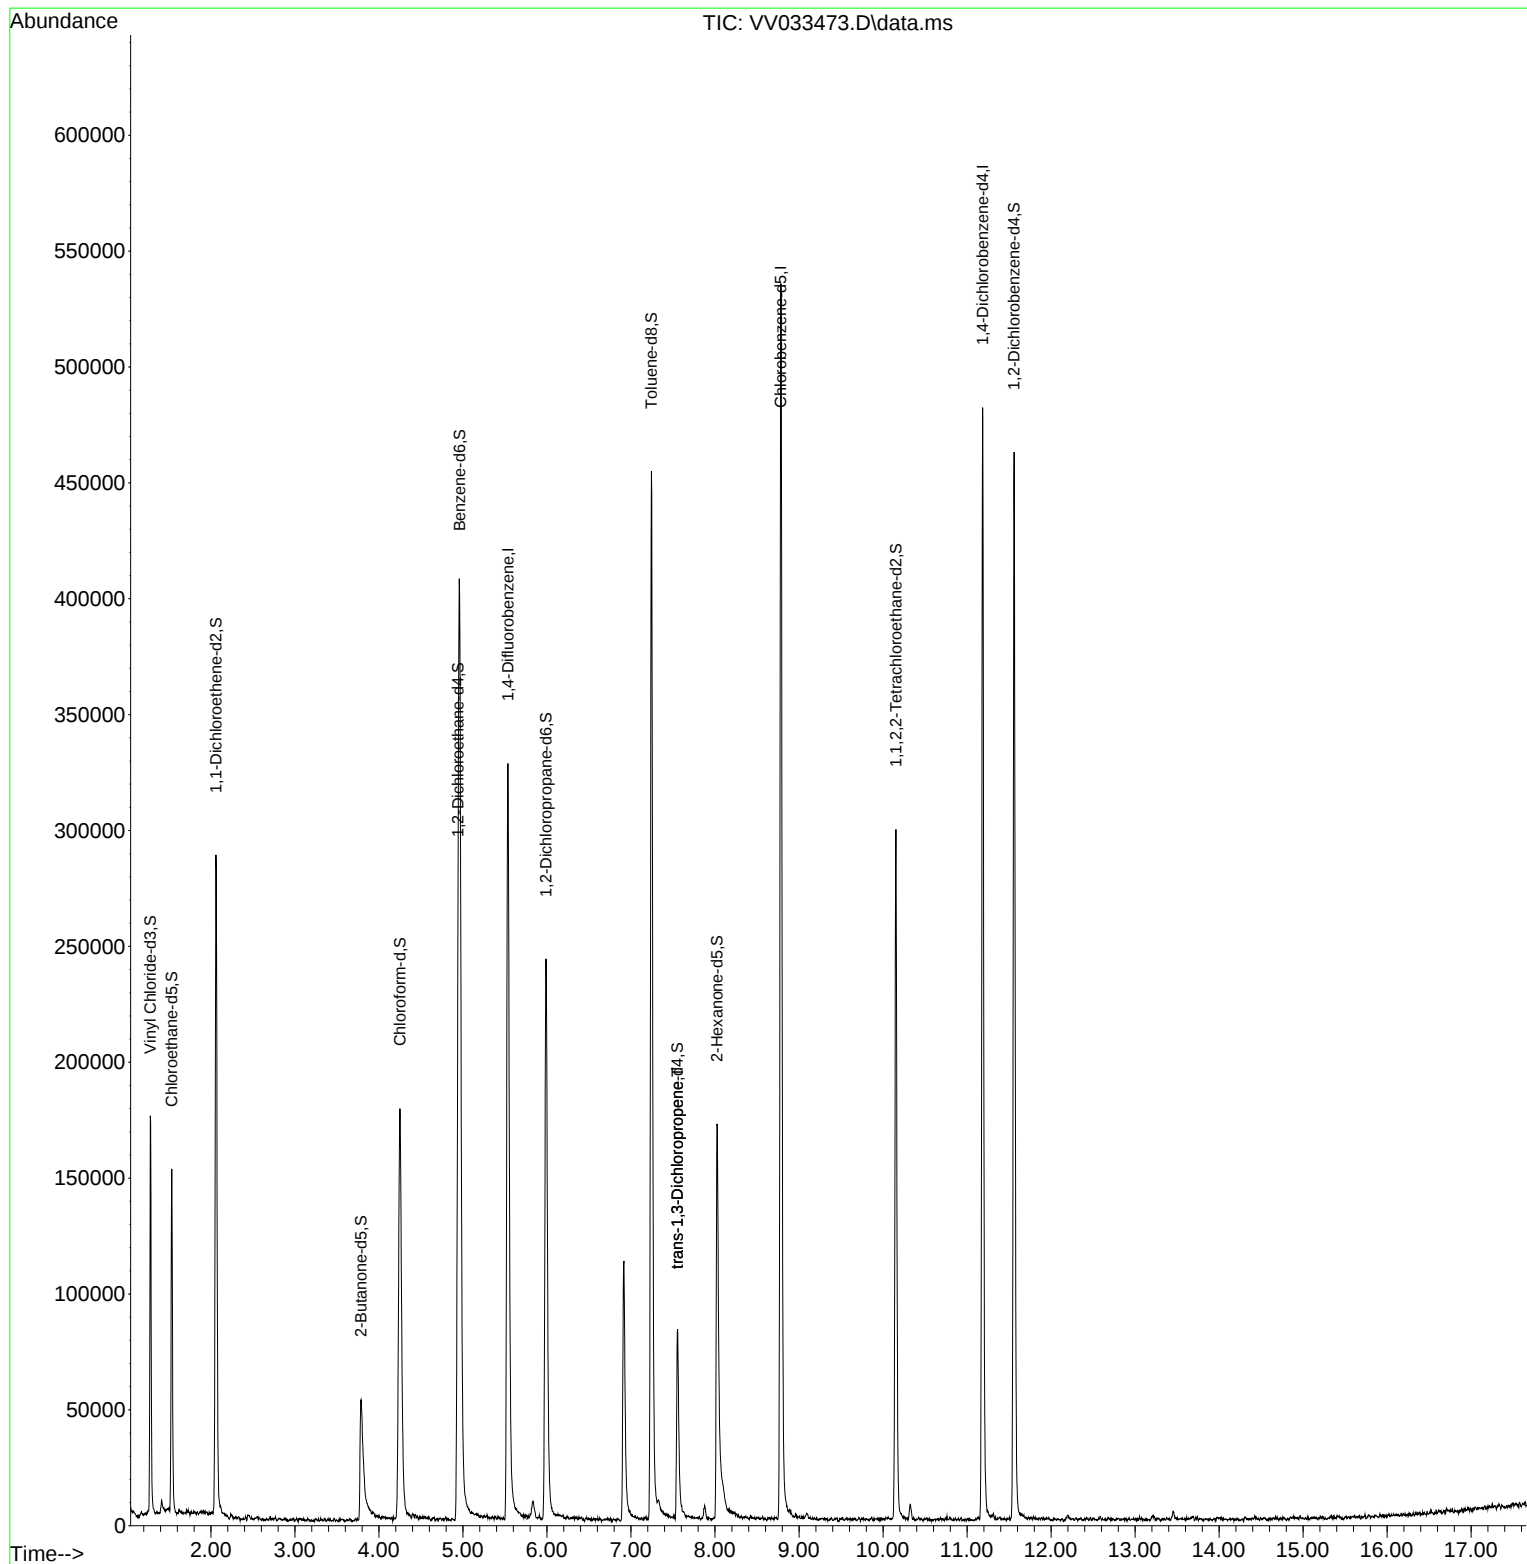

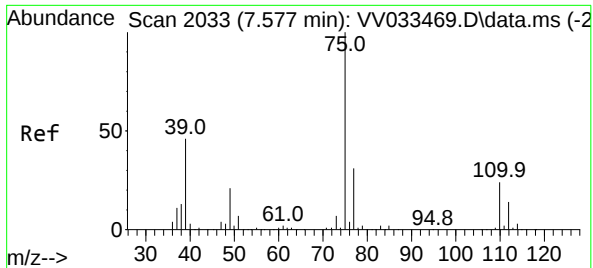

#44
 trans-1,3-Dichloropropene
 Concen: 0.804 ug/L
 RT: 7.551 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV033473.D
 Acq: 19 Dec 2023 13:26

Instrument :
 MSVOA_V
 ClientSampleId :

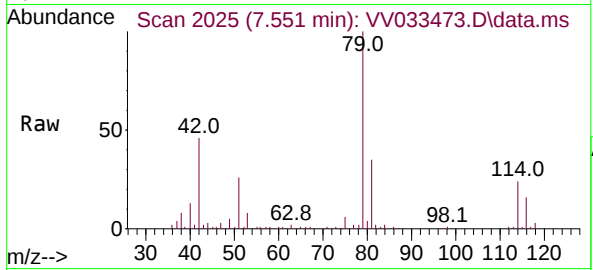

Tgt Ion: 75 Resp: 2436
 Ion Ratio Lower Upper
 75 100
 77 38.2 22.4 41.6

