

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033471.D
 Acq On : 19 Dec 2023 12:39
 Operator : SY/MD
 Sample : VV1219WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	174492	183118	16.27%	2.230%
2	1.532	146	153	171	rVB	152977	182907	16.25%	2.227%
3	2.059	308	317	331	rBV	287664	418133	37.15%	5.092%
4	2.336	400	403	405	rBV4	1121	671	0.06%	0.008%
5	2.394	419	421	424	rBV3	1131	839	0.07%	0.010%
6	2.596	480	484	487	rBV5	1627	1108	0.10%	0.013%
7	2.670	505	507	511	rBV4	966	493	0.04%	0.006%
8	2.741	526	529	530	rVB3	952	476	0.04%	0.006%
9	2.754	530	533	536	rVB5	1011	641	0.06%	0.008%
10	2.780	536	541	548	rBV8	1162	1363	0.12%	0.017%
11	2.873	565	570	573	rBV5	1286	1093	0.10%	0.013%
12	2.963	596	598	601	rVB3	815	450	0.04%	0.005%
13	2.979	601	603	606	rBV4	1046	621	0.06%	0.008%
14	3.002	608	610	613	rVB4	1553	699	0.06%	0.009%
15	3.030	618	619	623	rVB3	940	636	0.06%	0.008%
16	3.098	638	640	643	rBV4	902	714	0.06%	0.009%
17	3.172	660	663	666	rBV3	837	668	0.06%	0.008%
18	3.278	694	696	700	rVB5	968	737	0.07%	0.009%
19	3.297	700	702	706	rVB6	997	637	0.06%	0.008%
20	3.320	706	709	710	rBV3	897	434	0.04%	0.005%
21	3.365	719	723	725	rBV5	917	674	0.06%	0.008%
22	3.522	768	772	776	rBV4	1173	1244	0.11%	0.015%
23	3.558	779	783	785	rBV4	852	727	0.06%	0.009%
24	3.619	799	802	806	rVB5	1117	689	0.06%	0.008%
25	3.731	833	837	841	rBV6	617	578	0.05%	0.007%
26	3.783	845	853	877	rBV	60352	168658	14.99%	2.054%
27	4.047	933	935	938	rBV4	1160	575	0.05%	0.007%
28	4.249	984	998	1023	rBV	178604	452170	40.18%	5.506%
29	4.706	1136	1140	1144	rBV6	1354	880	0.08%	0.011%
30	4.956	1201	1218	1246	rBV2	419045	1125460	100.00%	13.705%
31	5.413	1354	1360	1364	rBV9	1659	1613	0.14%	0.020%
32	5.532	1386	1397	1420	rBV	317367	662852	58.90%	8.072%
33	5.989	1527	1539	1568	rBV3	243400	512904	45.57%	6.246%
34	6.513	1700	1702	1703	rBV3	1159	554	0.05%	0.007%
35	6.616	1732	1734	1735	rBV	978	429	0.04%	0.005%
36	6.699	1756	1760	1762	rBV4	1145	967	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033471.D
 Acq On : 19 Dec 2023 12:39
 Operator : SY/MD
 Sample : VV1219WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.731	1766	1770	1772	rBV4	1414	1231	0.11%	0.015%
38	6.834	1800	1802	1806	rVB4	1329	800	0.07%	0.010%
39	6.911	1817	1826	1847	rBV	116648	221465	19.68%	2.697%
40	7.143	1894	1898	1902	rBV	5582	4773	0.42%	0.058%
41	7.243	1917	1929	1952	rBV	468035	835587	74.24%	10.175%
42	7.551	2017	2025	2044	rBV	83604	153583	13.65%	1.870%
43	7.947	2145	2148	2149	rBV3	1614	873	0.08%	0.011%
44	8.024	2163	2172	2191	rBV	205102	393470	34.96%	4.791%
45	8.570	2339	2342	2345	rBV4	884	531	0.05%	0.006%
46	8.783	2398	2408	2432	rBV	521463	868043	77.13%	10.570%
47	9.262	2554	2557	2558	rBV3	802	449	0.04%	0.005%
48	9.358	2582	2587	2592	rBV7	1439	1315	0.12%	0.016%
49	9.435	2607	2611	2613	rBV5	1204	998	0.09%	0.012%
50	9.496	2626	2630	2631	rBV4	1377	964	0.09%	0.012%
51	9.741	2704	2706	2709	rBV2	989	504	0.04%	0.006%
52	9.799	2723	2724	2727	rBV3	834	474	0.04%	0.006%
53	9.863	2740	2744	2746	rBV4	1412	1201	0.11%	0.015%
54	9.950	2768	2771	2773	rBV4	886	587	0.05%	0.007%
55	9.982	2778	2781	2784	rBV4	1360	1025	0.09%	0.012%
56	9.995	2784	2785	2788	rVV2	621	358	0.03%	0.004%
57	10.014	2790	2791	2795	rVB3	1353	522	0.05%	0.006%
58	10.152	2824	2834	2856	rVB	308740	491430	43.66%	5.984%
59	10.416	2914	2916	2919	rVB4	1326	438	0.04%	0.005%
60	10.451	2925	2927	2928	rBV	1128	599	0.05%	0.007%
61	10.619	2976	2979	2982	rBV4	1211	874	0.08%	0.011%
62	10.715	3006	3009	3014	rBV6	1140	850	0.08%	0.010%
63	10.738	3014	3016	3018	rBV3	788	461	0.04%	0.006%
64	10.779	3026	3029	3031	rBV4	599	378	0.03%	0.005%
65	10.795	3032	3034	3039	rVB6	1720	1118	0.10%	0.014%
66	10.821	3039	3042	3046	rBV4	1267	1037	0.09%	0.013%
67	10.988	3091	3094	3097	rVB4	1741	1205	0.11%	0.015%
68	11.004	3097	3099	3100	rBV	949	484	0.04%	0.006%
69	11.027	3104	3106	3107	rVV2	882	462	0.04%	0.006%
70	11.056	3111	3115	3116	rBV4	690	488	0.04%	0.006%
71	11.075	3118	3121	3125	rVB6	1056	687	0.06%	0.008%
72	11.184	3144	3155	3182	rBV	465542	737483	65.53%	8.980%
73	11.390	3215	3219	3223	rBV6	1528	1405	0.12%	0.017%
74	11.561	3261	3272	3296	rBV	463609	726112	64.52%	8.842%
75	11.792	3341	3344	3346	rBV4	1396	775	0.07%	0.009%
76	11.840	3356	3359	3361	rVB4	1722	1063	0.09%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033471.D
 Acq On : 19 Dec 2023 12:39
 Operator : SY/MD
 Sample : VV1219WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.191	3464	3468	3471	rBV5	1264	961	0.09%	0.012%
78	12.647	3605	3610	3611	rBV4	1592	909	0.08%	0.011%
79	12.728	3632	3635	3637	rBV4	974	767	0.07%	0.009%
80	12.770	3643	3648	3650	rBV5	1282	1113	0.10%	0.014%
81	12.847	3668	3672	3674	rBV3	1278	710	0.06%	0.009%
82	12.860	3674	3676	3680	rVB4	1288	640	0.06%	0.008%
83	12.885	3680	3684	3686	rBV5	1281	1025	0.09%	0.012%
84	12.940	3698	3701	3704	rBV5	1383	884	0.08%	0.011%
85	13.217	3777	3787	3793	rBV5	3819	6913	0.61%	0.084%
86	13.361	3829	3832	3835	rVV5	807	724	0.06%	0.009%
87	13.545	3887	3889	3890	rBV2	805	404	0.04%	0.005%
88	13.615	3909	3911	3913	rBV3	1101	579	0.05%	0.007%
89	13.683	3928	3932	3941	rVB10	3577	5092	0.45%	0.062%
90	13.734	3946	3948	3950	rBV3	1248	583	0.05%	0.007%
91	13.766	3956	3958	3960	rBV2	698	390	0.03%	0.005%
92	13.789	3963	3965	3966	rBV2	753	401	0.04%	0.005%
93	13.799	3966	3968	3972	rVB2	1254	648	0.06%	0.008%
94	13.827	3974	3977	3978	rBV2	1200	666	0.06%	0.008%
95	13.856	3984	3986	3989	rVB4	1548	719	0.06%	0.009%
96	13.892	3994	3997	4002	rVB6	1518	958	0.09%	0.012%
97	14.159	4074	4080	4084	rBV7	1210	1315	0.12%	0.016%
98	14.284	4116	4119	4122	rBV5	1110	702	0.06%	0.009%
99	14.371	4144	4146	4147	rVB2	1187	380	0.03%	0.005%
100	14.757	4263	4266	4267	rBV3	1740	1059	0.09%	0.013%




Sum of corrected areas: 8212056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033471.D
Acq On : 19 Dec 2023 12:39
Operator : SY/MD
Sample : VV1219WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

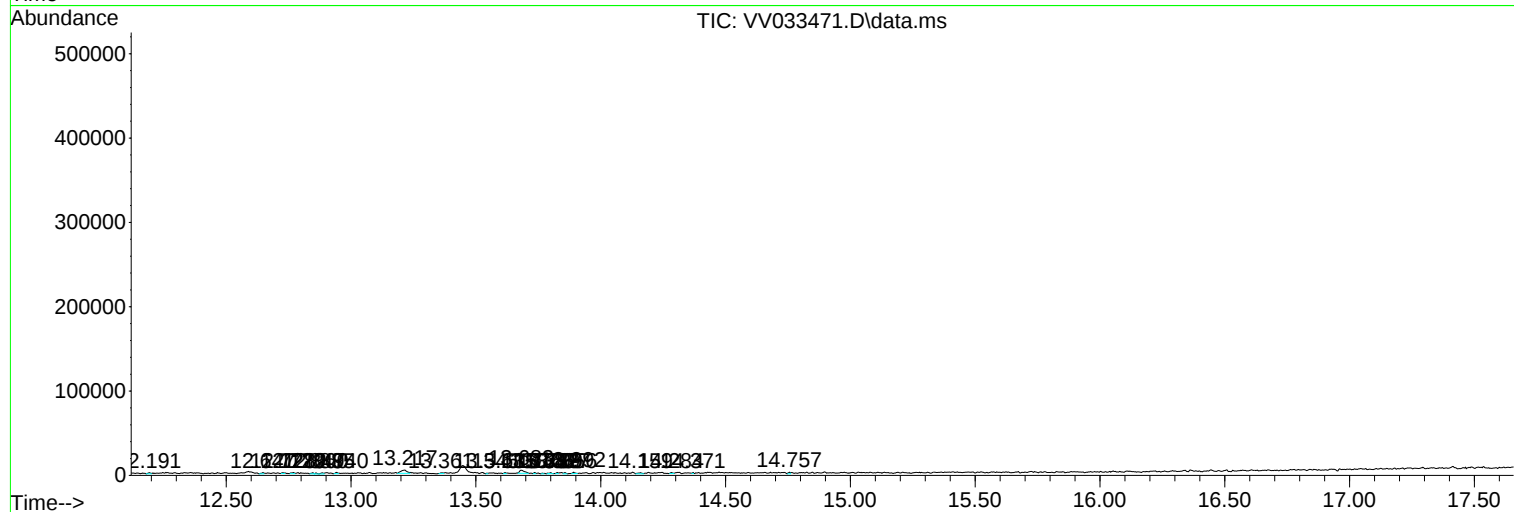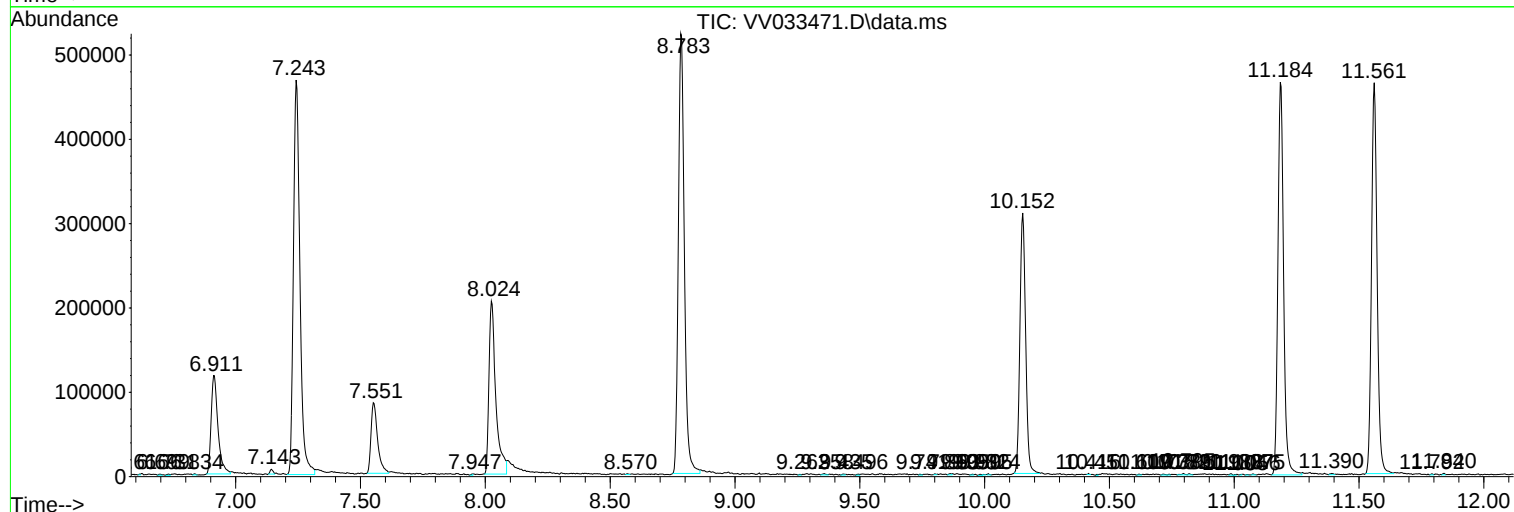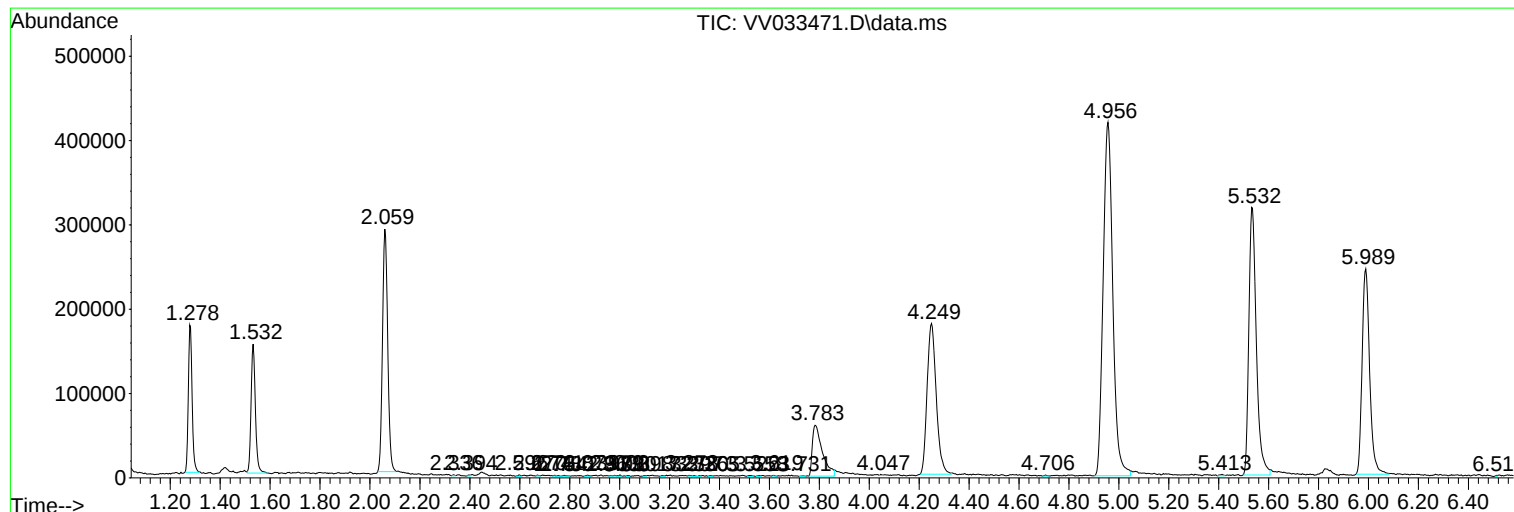

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033471.D
Acq On : 19 Dec 2023 12:39
Operator : SY/MD
Sample : VV1219WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033471.D
Acq On : 19 Dec 2023 12:39
Operator : SY/MD
Sample : VV1219WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------