

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033473.D
 Acq On : 19 Dec 2023 13:26
 Operator : SY/MD
 Sample : 05912-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	170497	178094	16.15%	2.187%
2	1.532	146	153	167	rVB	148173	173701	15.75%	2.133%
3	2.060	309	317	340	rVB	284046	420564	38.13%	5.165%
4	2.439	431	435	437	rBV5	2402	2040	0.18%	0.025%
5	2.619	486	491	493	rVB6	964	784	0.07%	0.010%
6	2.706	513	518	521	rBV7	1674	1276	0.12%	0.016%
7	2.725	521	524	525	rBV3	888	434	0.04%	0.005%
8	2.806	545	549	550	rBV4	946	667	0.06%	0.008%
9	3.002	607	610	613	rBV5	792	637	0.06%	0.008%
10	3.021	614	616	621	rVB6	1682	1204	0.11%	0.015%
11	3.043	621	623	626	rBV2	1444	1083	0.10%	0.013%
12	3.105	640	642	646	rVB4	1285	621	0.06%	0.008%
13	3.121	646	647	651	rBV2	642	492	0.04%	0.006%
14	3.150	653	656	658	rBV4	1122	604	0.05%	0.007%
15	3.198	668	671	673	rBV4	804	500	0.05%	0.006%
16	3.243	682	685	686	rBV3	1287	825	0.07%	0.010%
17	3.307	702	705	707	rBV4	1064	445	0.04%	0.005%
18	3.349	714	718	721	rBV5	1102	869	0.08%	0.011%
19	3.416	738	739	742	rVB3	1092	400	0.04%	0.005%
20	3.465	752	754	760	rVB4	1388	1134	0.10%	0.014%
21	3.526	769	773	774	rBV3	1260	612	0.06%	0.008%
22	3.561	779	784	786	rBV5	808	797	0.07%	0.010%
23	3.719	829	833	834	rBV4	919	519	0.05%	0.006%
24	3.741	837	840	843	rBV4	1102	732	0.07%	0.009%
25	3.786	845	854	880	rBV2	51929	150225	13.62%	1.845%
26	4.037	929	932	935	rBV5	1376	956	0.09%	0.012%
27	4.169	971	973	975	rBV2	1852	927	0.08%	0.011%
28	4.249	984	998	1024	rBV2	176057	446209	40.45%	5.480%
29	4.638	1117	1119	1123	rBV5	1095	1011	0.09%	0.012%
30	4.757	1153	1156	1157	rBV2	811	441	0.04%	0.005%
31	4.867	1187	1190	1195	rBV6	1018	1154	0.10%	0.014%
32	4.957	1201	1218	1248	rBV2	406660	1103082	100.00%	13.548%
33	5.375	1346	1348	1349	rBV2	1195	485	0.04%	0.006%
34	5.416	1359	1361	1365	rBV3	1179	647	0.06%	0.008%
35	5.535	1386	1398	1428	rBV	326460	692260	62.76%	8.502%
36	5.989	1526	1539	1562	rBV	241582	506144	45.88%	6.216%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033473.D
 Acq On : 19 Dec 2023 13:26
 Operator : SY/MD
 Sample : 05912-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.333	1644	1646	1650	rBV4	1437	1037	0.09%	0.013%
38	6.381	1657	1661	1663	rBV3	1362	869	0.08%	0.011%
39	6.461	1681	1686	1689	rBV5	1580	1718	0.16%	0.021%
40	6.529	1705	1707	1710	rBV4	1206	549	0.05%	0.007%
41	6.551	1710	1714	1717	rBV6	1202	871	0.08%	0.011%
42	6.567	1717	1719	1722	rVB4	830	534	0.05%	0.007%
43	6.789	1783	1788	1792	rBV4	1412	1653	0.15%	0.020%
44	6.834	1799	1802	1804	rBV4	1115	680	0.06%	0.008%
45	6.915	1816	1827	1848	rBV	112009	219222	19.87%	2.692%
46	7.165	1902	1905	1907	rBV4	1038	787	0.07%	0.010%
47	7.243	1918	1929	1950	rBV	452297	804726	72.95%	9.883%
48	7.555	2017	2026	2046	rBV	82018	154619	14.02%	1.899%
49	7.866	2121	2123	2124	rBV2	3155	1431	0.13%	0.018%
50	7.924	2139	2141	2145	rBV3	1257	1056	0.10%	0.013%
51	8.024	2164	2172	2210	rBV	169886	377703	34.24%	4.639%
52	8.628	2356	2360	2361	rBV3	1294	732	0.07%	0.009%
53	8.709	2383	2385	2390	rBV5	1206	1193	0.11%	0.015%
54	8.783	2397	2408	2430	rBV	533397	888491	80.55%	10.912%
55	9.185	2530	2533	2539	rVB7	1045	893	0.08%	0.011%
56	9.210	2539	2541	2544	rVB4	1236	645	0.06%	0.008%
57	9.246	2548	2552	2555	rBV6	836	669	0.06%	0.008%
58	9.484	2624	2626	2631	rBV5	1304	1401	0.13%	0.017%
59	9.744	2703	2707	2711	rBV6	1309	1400	0.13%	0.017%
60	9.892	2751	2753	2755	rBV2	1085	416	0.04%	0.005%
61	9.953	2770	2772	2774	rVB3	1262	582	0.05%	0.007%
62	9.979	2776	2780	2782	rBV5	1175	941	0.09%	0.012%
63	10.027	2793	2795	2796	rBV3	1161	399	0.04%	0.005%
64	10.153	2823	2834	2860	rBV	296978	465649	42.21%	5.719%
65	10.323	2879	2887	2896	rBV5	6697	10854	0.98%	0.133%
66	10.535	2951	2953	2957	rBV5	981	568	0.05%	0.007%
67	10.673	2993	2996	2997	rBV4	796	389	0.04%	0.005%
68	10.683	2997	2999	3002	rVV4	931	468	0.04%	0.006%
69	10.741	3014	3017	3021	rBV5	1416	1167	0.11%	0.014%
70	10.760	3021	3023	3027	rVB3	1693	785	0.07%	0.010%
71	10.895	3060	3065	3067	rBV6	1149	859	0.08%	0.011%
72	10.921	3070	3073	3074	rBV3	1135	638	0.06%	0.008%
73	10.998	3094	3097	3098	rBV3	931	560	0.05%	0.007%
74	11.024	3102	3105	3106	rBV2	984	505	0.05%	0.006%
75	11.185	3144	3155	3172	rBV	479837	752801	68.25%	9.246%
76	11.561	3258	3272	3293	rBV	460875	730237	66.20%	8.969%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033473.D
 Acq On : 19 Dec 2023 13:26
 Operator : SY/MD
 Sample : 05912-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	11.908	3378	3380	3384	rBV4	1152	531	0.05%	0.007%
78	11.927	3384	3386	3390	rBV5	780	554	0.05%	0.007%
79	12.027	3414	3417	3418	rBV2	927	498	0.05%	0.006%
80	12.072	3429	3431	3433	rBV2	709	490	0.04%	0.006%
81	12.159	3454	3458	3461	rBV5	746	621	0.06%	0.008%
82	12.181	3461	3465	3467	rBV4	1521	1444	0.13%	0.018%
83	12.326	3507	3510	3512	rBV2	893	649	0.06%	0.008%
84	12.493	3559	3562	3563	rBV3	985	490	0.04%	0.006%
85	12.564	3582	3584	3586	rBV2	936	418	0.04%	0.005%
86	12.914	3690	3693	3695	rBV3	744	575	0.05%	0.007%
87	13.033	3727	3730	3732	rBV4	1039	464	0.04%	0.006%
88	13.053	3732	3736	3737	rVV2	1620	796	0.07%	0.010%
89	13.075	3741	3743	3747	rVB5	1303	926	0.08%	0.011%
90	13.204	3777	3783	3784	rBV6	1583	1517	0.14%	0.019%
91	13.258	3798	3800	3803	rBV2	992	671	0.06%	0.008%
92	13.432	3851	3854	3855	rBV	1400	685	0.06%	0.008%
93	13.818	3972	3974	3976	rBV3	1123	636	0.06%	0.008%
94	13.979	4019	4024	4025	rBV4	1435	1399	0.13%	0.017%
95	14.049	4045	4046	4050	rBV2	1191	718	0.07%	0.009%
96	14.300	4121	4124	4126	rBV4	1852	1218	0.11%	0.015%
97	14.493	4181	4184	4187	rBV4	1353	894	0.08%	0.011%
98	14.606	4213	4219	4222	rBV7	1317	1365	0.12%	0.017%
99	14.673	4238	4240	4243	rBV3	1184	665	0.06%	0.008%
100	15.204	4403	4405	4410	rBV4	1254	739	0.07%	0.009%




Sum of corrected areas: 8142235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033473.D
Acq On : 19 Dec 2023 13:26
Operator : SY/MD
Sample : 05912-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

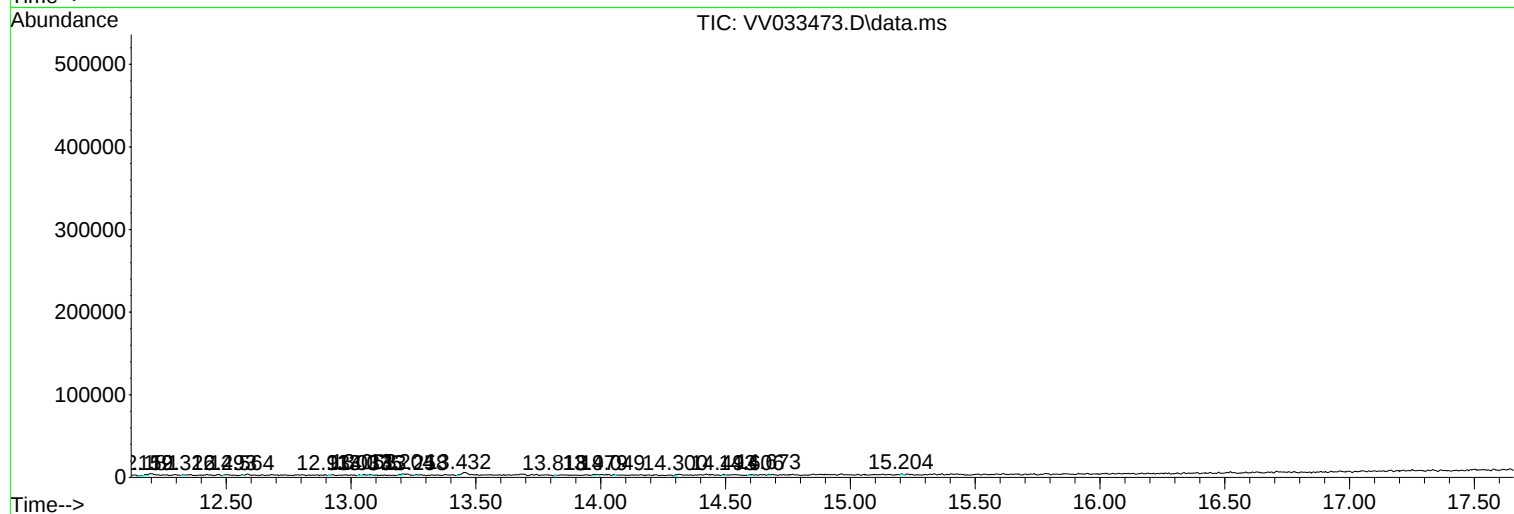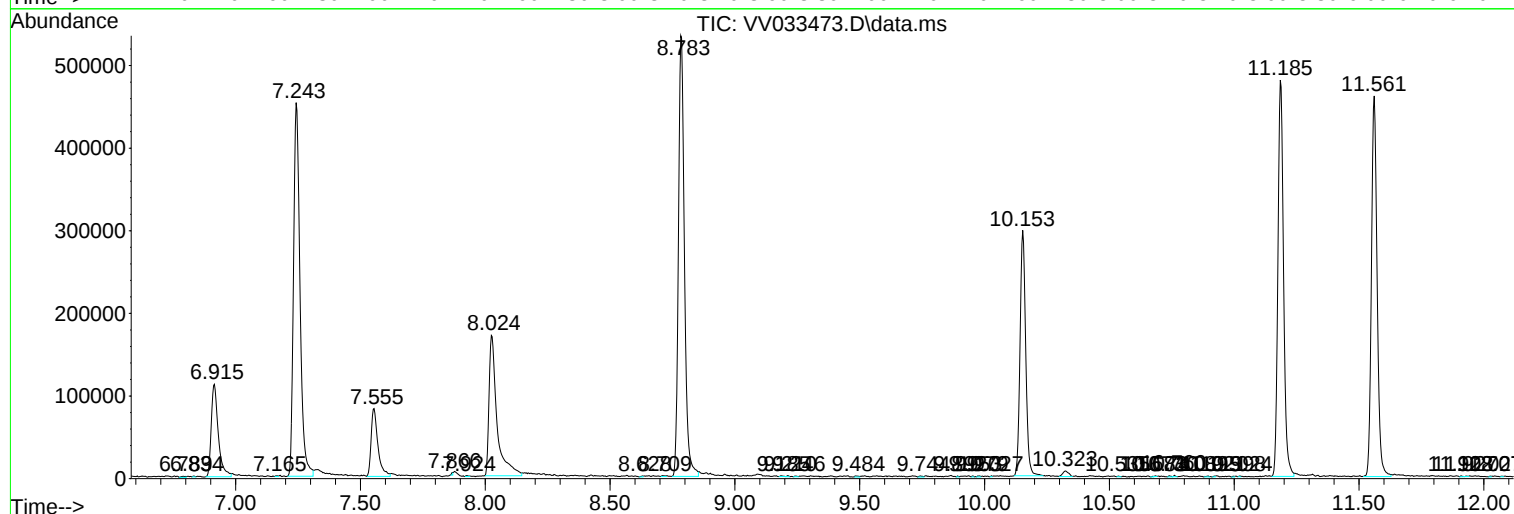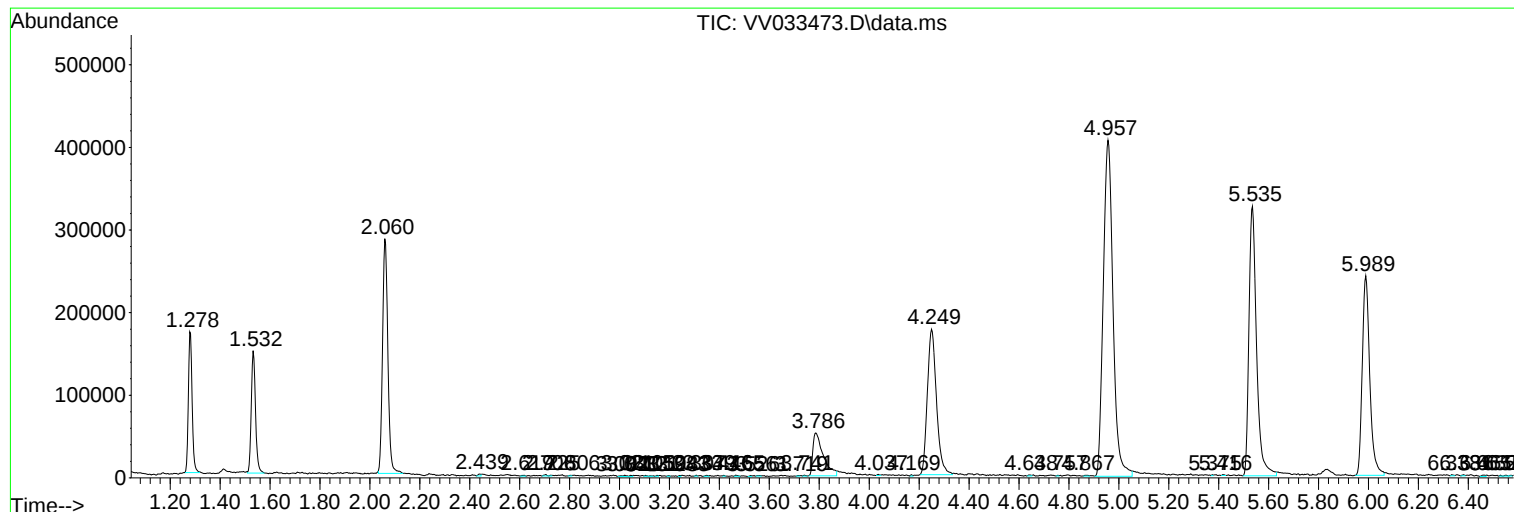

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033473.D
Acq On : 19 Dec 2023 13:26
Operator : SY/MD
Sample : 05912-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033473.D
Acq On : 19 Dec 2023 13:26
Operator : SY/MD
Sample : 05912-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc