

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033475.D
 Acq On : 19 Dec 2023 14:12
 Operator : SY/MD
 Sample : 05912-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rBV	163318	173627	16.23%	2.154%
2	1.532	146	153	166	rVB	143955	169744	15.86%	2.106%
3	2.060	308	317	330	rBV	273102	402383	37.61%	4.991%
4	2.497	451	453	454	rBV2	814	328	0.03%	0.004%
5	2.892	573	576	577	rBV3	1134	673	0.06%	0.008%
6	3.047	619	624	628	rBV6	1133	1289	0.12%	0.016%
7	3.095	636	639	640	rBV2	1262	735	0.07%	0.009%
8	3.175	661	664	666	rBV4	804	459	0.04%	0.006%
9	3.449	747	749	751	rBV2	1138	726	0.07%	0.009%
10	3.500	763	765	767	rVB3	1008	395	0.04%	0.005%
11	3.641	806	809	811	rBV3	1735	1255	0.12%	0.016%
12	3.786	844	854	891	rBV2	70075	213559	19.96%	2.649%
13	4.249	984	998	1023	rBV	175529	441130	41.23%	5.472%
14	4.809	1170	1172	1174	rBV3	935	492	0.05%	0.006%
15	4.957	1202	1218	1244	rBV2	402482	1069943	100.00%	13.272%
16	5.535	1387	1398	1429	rBV	327607	680658	63.62%	8.443%
17	5.989	1527	1539	1567	rBV	239678	499090	46.65%	6.191%
18	6.474	1687	1690	1691	rBV3	1169	750	0.07%	0.009%
19	6.709	1761	1763	1765	rVB2	793	325	0.03%	0.004%
20	6.722	1765	1767	1769	rBV2	1732	1065	0.10%	0.013%
21	6.760	1776	1779	1782	rBV4	938	653	0.06%	0.008%
22	6.850	1804	1807	1809	rBV3	1249	817	0.08%	0.010%
23	6.915	1817	1827	1846	rBV	111530	211630	19.78%	2.625%
24	7.243	1919	1929	1949	rBV	444778	784835	73.35%	9.735%
25	7.555	2017	2026	2042	rBV	80662	145496	13.60%	1.805%
26	7.792	2098	2100	2102	rVB3	1186	402	0.04%	0.005%
27	8.024	2163	2172	2202	rBV	176705	379852	35.50%	4.712%
28	8.599	2348	2351	2352	rBV3	920	609	0.06%	0.008%
29	8.648	2364	2366	2367	rBV2	812	312	0.03%	0.004%
30	8.786	2398	2409	2433	rBV	541166	900634	84.18%	11.172%
31	9.387	2594	2596	2598	rBV2	1181	354	0.03%	0.004%
32	9.419	2604	2606	2608	rBV2	815	386	0.04%	0.005%
33	9.516	2634	2636	2638	rBV3	846	329	0.03%	0.004%
34	9.590	2657	2659	2660	rBV2	700	196	0.02%	0.002%
35	9.664	2678	2682	2684	rBV5	1313	841	0.08%	0.010%
36	9.712	2695	2697	2699	rBV4	930	381	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033475.D
 Acq On : 19 Dec 2023 14:12
 Operator : SY/MD
 Sample : 05912-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	9.731	2701	2703	2706	rVB4	1253	699	0.07%	0.009%
38	9.937	2764	2767	2771	rBV6	992	729	0.07%	0.009%
39	10.005	2784	2788	2793	rVB6	1511	1303	0.12%	0.016%
40	10.152	2824	2834	2852	rBV	296972	464394	43.40%	5.761%
41	10.413	2913	2915	2916	rBV2	893	494	0.05%	0.006%
42	10.474	2932	2934	2938	rVB4	929	556	0.05%	0.007%
43	10.500	2940	2942	2945	rVB3	690	372	0.03%	0.005%
44	10.516	2945	2947	2950	rBV2	660	409	0.04%	0.005%
45	10.651	2987	2989	2992	rVB3	1297	710	0.07%	0.009%
46	10.718	3006	3010	3012	rBV3	807	467	0.04%	0.006%
47	10.837	3045	3047	3051	rVB3	1755	827	0.08%	0.010%
48	10.905	3064	3068	3072	rBV6	1698	1248	0.12%	0.015%
49	10.979	3085	3091	3093	rBV6	1030	922	0.09%	0.011%
50	11.001	3096	3098	3101	rVV4	1249	860	0.08%	0.011%
51	11.033	3106	3108	3111	rVV4	856	459	0.04%	0.006%
52	11.062	3115	3117	3120	rBV3	637	290	0.03%	0.004%
53	11.127	3134	3137	3140	rBV4	1522	1276	0.12%	0.016%
54	11.185	3145	3155	3177	rVV	485957	764687	71.47%	9.486%
55	11.339	3200	3203	3208	rBV6	1909	1727	0.16%	0.021%
56	11.397	3219	3221	3222	rBV2	979	373	0.03%	0.005%
57	11.561	3261	3272	3295	rBV	448944	714151	66.75%	8.859%
58	11.863	3363	3366	3369	rBV5	1266	1021	0.10%	0.013%
59	12.242	3482	3484	3486	rBV2	669	254	0.02%	0.003%
60	12.339	3512	3514	3515	rBV2	789	404	0.04%	0.005%
61	12.474	3552	3556	3557	rBV3	1001	582	0.05%	0.007%
62	12.561	3582	3583	3585	rVB2	1048	287	0.03%	0.004%
63	12.641	3605	3608	3611	rBV4	1426	1152	0.11%	0.014%
64	12.693	3622	3624	3625	rBV2	845	395	0.04%	0.005%
65	12.773	3647	3649	3651	rBV	903	493	0.05%	0.006%
66	12.818	3660	3663	3666	rBV3	1685	1431	0.13%	0.018%
67	13.008	3720	3722	3723	rBV2	1072	315	0.03%	0.004%
68	13.053	3732	3736	3738	rBV3	882	715	0.07%	0.009%
69	13.162	3769	3770	3776	rVB5	897	568	0.05%	0.007%
70	13.281	3805	3807	3811	rVB5	1157	564	0.05%	0.007%
71	13.606	3905	3908	3911	rBV5	1228	734	0.07%	0.009%
72	13.715	3939	3942	3945	rBV3	1586	1172	0.11%	0.015%
73	13.786	3961	3964	3967	rBV2	1430	960	0.09%	0.012%
74	13.857	3984	3986	3987	rBV	914	291	0.03%	0.004%
75	13.876	3990	3992	3993	rBV2	690	251	0.02%	0.003%
76	14.027	4037	4039	4041	rBV3	990	466	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033475.D
Acq On : 19 Dec 2023 14:12
Operator : SY/MD
Sample : 05912-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

77	14.374	4145	4147	4150	rBV3	1181	825	0.08%	0.010%
78	14.551	4198	4202	4205	rBV4	1488	1221	0.11%	0.015%
79	14.574	4205	4209	4211	rBV3	1337	1051	0.10%	0.013%
80	14.808	4280	4282	4285	rBV4	1118	678	0.06%	0.008%
81	15.004	4340	4343	4346	rBV4	1183	980	0.09%	0.012%
82	15.059	4357	4360	4364	rVB5	2249	1509	0.14%	0.019%




Sum of corrected areas: 8061625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033475.D
Acq On : 19 Dec 2023 14:12
Operator : SY/MD
Sample : 05912-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

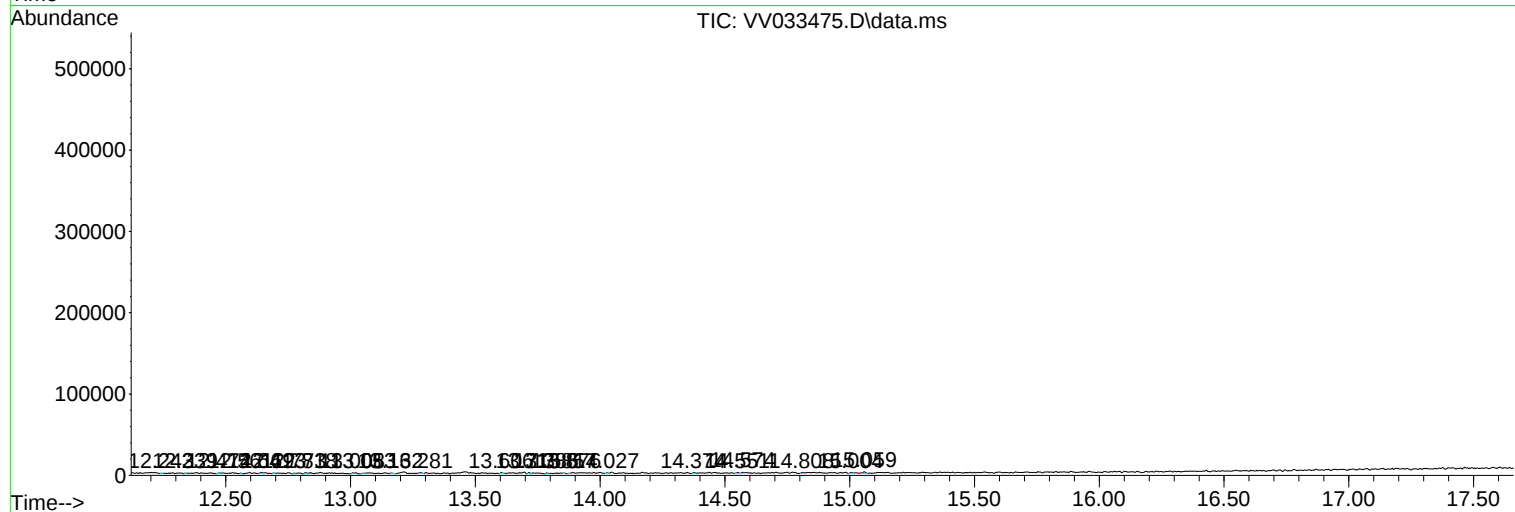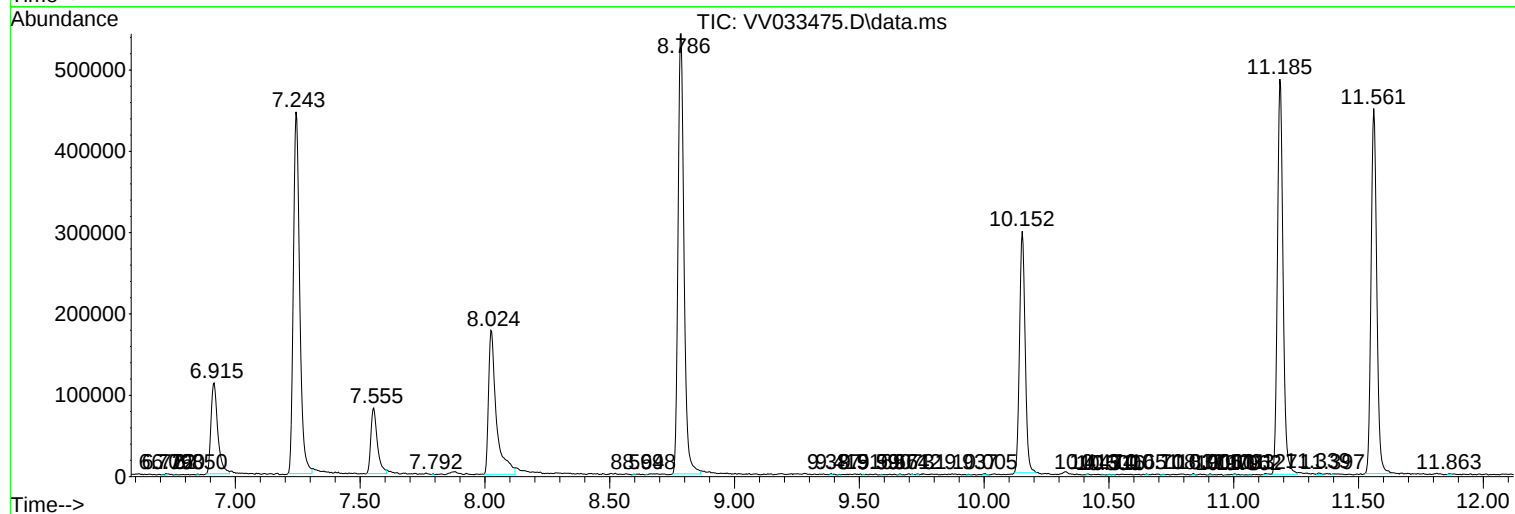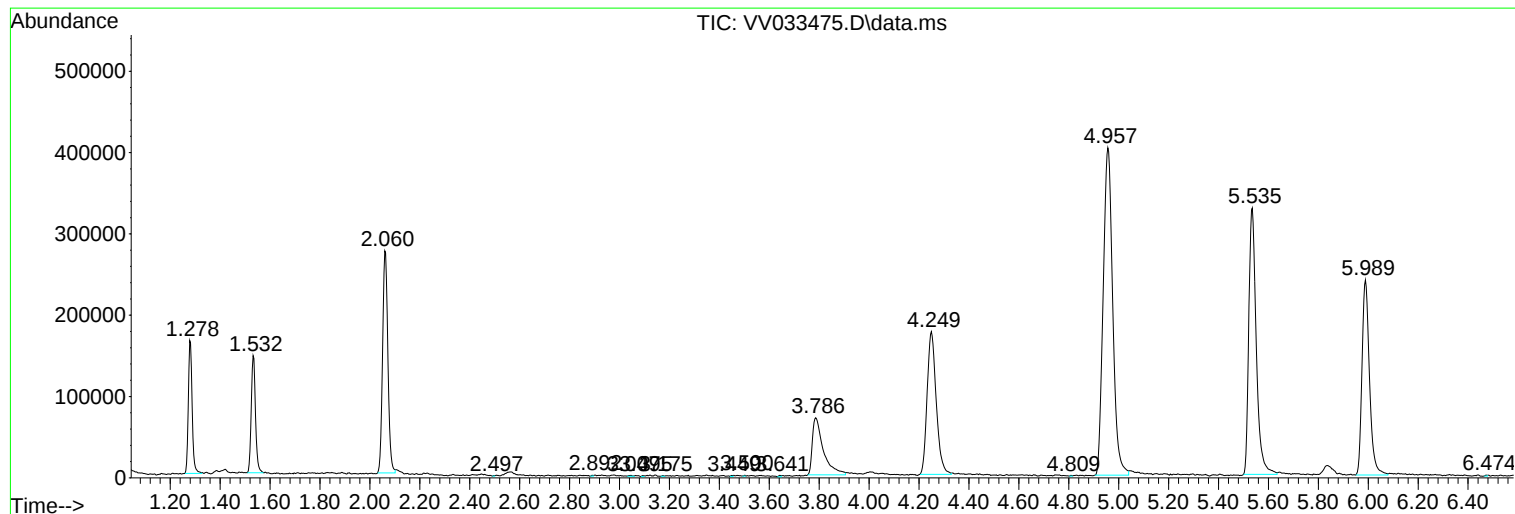

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033475.D
Acq On : 19 Dec 2023 14:12
Operator : SY/MD
Sample : 05912-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033475.D
Acq On : 19 Dec 2023 14:12
Operator : SY/MD
Sample : 05912-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc