

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033476.D
 Acq On : 19 Dec 2023 14:35
 Operator : SY/MD
 Sample : 05912-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	93	rVB	177239	185572	16.87%	2.277%
2	1.532	147	153	166	rVB	147221	172972	15.72%	2.122%
3	2.060	308	317	333	rBV	278460	412372	37.49%	5.059%
4	2.420	427	429	430	rBV2	928	385	0.03%	0.005%
5	2.609	486	488	490	rBV3	1038	591	0.05%	0.007%
6	2.667	503	506	507	rBV3	1161	506	0.05%	0.006%
7	2.828	553	556	558	rBV4	793	549	0.05%	0.007%
8	2.931	584	588	590	rBV4	755	456	0.04%	0.006%
9	2.973	595	601	602	rVV5	1071	1099	0.10%	0.013%
10	3.015	608	614	617	rBV6	1195	1197	0.11%	0.015%
11	3.108	640	643	645	rBV2	1320	758	0.07%	0.009%
12	3.227	676	680	684	rBV5	934	988	0.09%	0.012%
13	3.259	688	690	695	rVV5	819	460	0.04%	0.006%
14	3.397	729	733	734	rBV2	787	475	0.04%	0.006%
15	3.410	734	737	742	rVV5	1210	943	0.09%	0.012%
16	3.439	744	746	751	rVB4	1684	924	0.08%	0.011%
17	3.474	752	757	761	rVB6	1478	1306	0.12%	0.016%
18	3.507	761	767	770	rBV7	1466	1727	0.16%	0.021%
19	3.593	792	794	796	rVV3	996	552	0.05%	0.007%
20	3.619	799	802	804	rBV4	1664	688	0.06%	0.008%
21	3.658	812	814	816	rBV3	1132	568	0.05%	0.007%
22	3.732	833	837	838	rBV3	901	541	0.05%	0.007%
23	3.786	845	854	881	rBV	57835	188958	17.18%	2.318%
24	4.166	969	972	976	rBV4	951	773	0.07%	0.009%
25	4.249	985	998	1022	rVB	172958	439022	39.91%	5.386%
26	4.658	1123	1125	1127	rBV3	801	402	0.04%	0.005%
27	4.767	1157	1159	1163	rVB4	1001	657	0.06%	0.008%
28	4.796	1166	1168	1170	rVV3	714	406	0.04%	0.005%
29	4.957	1202	1218	1244	rBV2	413112	1100077	100.00%	13.497%
30	5.461	1373	1375	1378	rBV4	873	416	0.04%	0.005%
31	5.532	1386	1397	1431	rBV	312398	666352	60.57%	8.175%
32	5.989	1527	1539	1566	rBV	241508	504099	45.82%	6.185%
33	6.285	1629	1631	1636	rVB4	1949	1441	0.13%	0.018%
34	6.333	1643	1646	1649	rBV3	1450	1084	0.10%	0.013%
35	6.420	1671	1673	1676	rBV4	1059	546	0.05%	0.007%
36	6.500	1692	1698	1703	rBV4	1279	1338	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033476.D
 Acq On : 19 Dec 2023 14:35
 Operator : SY/MD
 Sample : 05912-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.600	1723	1729	1732	rBV7	1000	1060	0.10%	0.013%
38	6.825	1792	1799	1802	rBV6	1537	2186	0.20%	0.027%
39	6.915	1817	1827	1850	rVV	114042	220686	20.06%	2.708%
40	7.201	1912	1916	1917	rBV3	1259	1029	0.09%	0.013%
41	7.243	1919	1929	1949	rVV	454797	803869	73.07%	9.863%
42	7.555	2017	2026	2042	rBV	83025	150581	13.69%	1.847%
43	7.850	2115	2118	2119	rBV3	833	481	0.04%	0.006%
44	8.024	2163	2172	2210	rBV	180324	396711	36.06%	4.867%
45	8.420	2292	2295	2298	rVB5	1498	897	0.08%	0.011%
46	8.593	2347	2349	2356	rBV7	1114	1061	0.10%	0.013%
47	8.783	2398	2408	2426	rBV	521443	859726	78.15%	10.548%
48	9.046	2487	2490	2492	rBV4	1688	967	0.09%	0.012%
49	9.133	2513	2517	2520	rBV5	1557	1531	0.14%	0.019%
50	9.439	2606	2612	2614	rBV7	1364	1530	0.14%	0.019%
51	9.612	2662	2666	2669	rBV4	1400	1106	0.10%	0.014%
52	9.641	2673	2675	2677	rBV2	1249	512	0.05%	0.006%
53	9.741	2703	2706	2710	rVB4	1216	998	0.09%	0.012%
54	9.760	2710	2712	2715	rBV3	1159	775	0.07%	0.010%
55	9.802	2723	2725	2727	rBV2	1266	539	0.05%	0.007%
56	9.844	2735	2738	2739	rBV3	1184	802	0.07%	0.010%
57	9.918	2759	2761	2764	rVB4	1487	653	0.06%	0.008%
58	9.937	2764	2767	2771	rVB5	1084	573	0.05%	0.007%
59	9.963	2771	2775	2776	rBV4	811	569	0.05%	0.007%
60	10.072	2807	2809	2810	rBV2	973	440	0.04%	0.005%
61	10.153	2823	2834	2853	rBV	311451	496962	45.18%	6.097%
62	10.455	2922	2928	2932	rBV8	1761	1817	0.17%	0.022%
63	10.477	2933	2935	2938	rVB3	977	437	0.04%	0.005%
64	10.526	2946	2950	2951	rBV4	1214	742	0.07%	0.009%
65	10.641	2984	2986	2990	rBV4	686	421	0.04%	0.005%
66	10.731	3011	3014	3016	rVB2	846	456	0.04%	0.006%
67	10.960	3081	3085	3090	rVB6	1081	914	0.08%	0.011%
68	10.982	3090	3092	3094	rBV3	1023	524	0.05%	0.006%
69	11.046	3108	3112	3115	rBV4	1614	1329	0.12%	0.016%
70	11.185	3145	3155	3176	rBV	468260	743552	67.59%	9.123%
71	11.397	3218	3221	3226	rVB7	1445	1178	0.11%	0.014%
72	11.423	3226	3229	3234	rBV6	1475	1199	0.11%	0.015%
73	11.561	3261	3272	3290	rBV	467635	739654	67.24%	9.075%
74	11.915	3380	3382	3384	rBV2	1069	572	0.05%	0.007%
75	12.024	3414	3416	3419	rBV4	1206	797	0.07%	0.010%
76	12.284	3494	3497	3500	rVB5	1344	891	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033476.D
 Acq On : 19 Dec 2023 14:35
 Operator : SY/MD
 Sample : 05912-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.397	3530	3532	3536	rVB5	1116	773	0.07%	0.009%
78	12.419	3536	3539	3540	rBV3	1039	634	0.06%	0.008%
79	12.635	3604	3606	3610	rVB4	1245	603	0.05%	0.007%
80	12.657	3610	3613	3614	rBV3	966	472	0.04%	0.006%
81	12.744	3638	3640	3642	rBV2	905	509	0.05%	0.006%
82	12.805	3657	3659	3661	rBV3	726	427	0.04%	0.005%
83	12.850	3670	3673	3674	rBV3	951	438	0.04%	0.005%
84	12.934	3693	3699	3705	rBV8	1372	1629	0.15%	0.020%
85	12.960	3705	3707	3710	rBV3	873	639	0.06%	0.008%
86	13.095	3747	3749	3753	rVB3	874	407	0.04%	0.005%
87	13.442	3853	3857	3859	rBV4	1316	1134	0.10%	0.014%
88	13.506	3873	3877	3878	rBV4	1329	959	0.09%	0.012%
89	13.570	3894	3897	3900	rBV5	1470	767	0.07%	0.009%
90	13.599	3904	3906	3909	rVB3	1346	702	0.06%	0.009%
91	13.863	3985	3988	3991	rBV4	834	547	0.05%	0.007%
92	13.914	4000	4004	4007	rBV5	1161	1032	0.09%	0.013%
93	14.136	4069	4073	4076	rBV5	816	822	0.07%	0.010%
94	14.159	4077	4080	4083	rBV4	1253	803	0.07%	0.010%
95	14.178	4083	4086	4087	rBV2	1096	590	0.05%	0.007%
96	14.284	4115	4119	4121	rBV4	919	708	0.06%	0.009%
97	14.345	4133	4138	4139	rBV3	976	828	0.08%	0.010%
98	14.522	4190	4193	4196	rBV4	1484	1077	0.10%	0.013%
99	15.223	4407	4411	4414	rVB5	1614	1462	0.13%	0.018%
100	15.242	4414	4417	4420	rBV2	1178	813	0.07%	0.010%




Sum of corrected areas: 8150702

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033476.D
Acq On : 19 Dec 2023 14:35
Operator : SY/MD
Sample : 05912-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

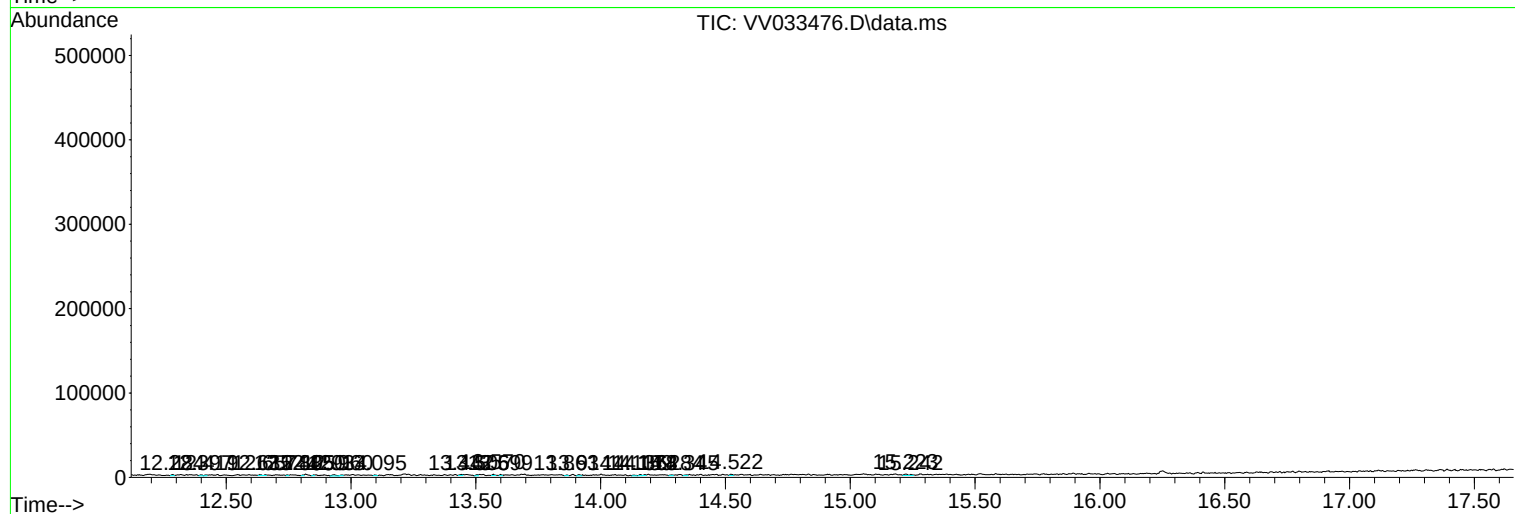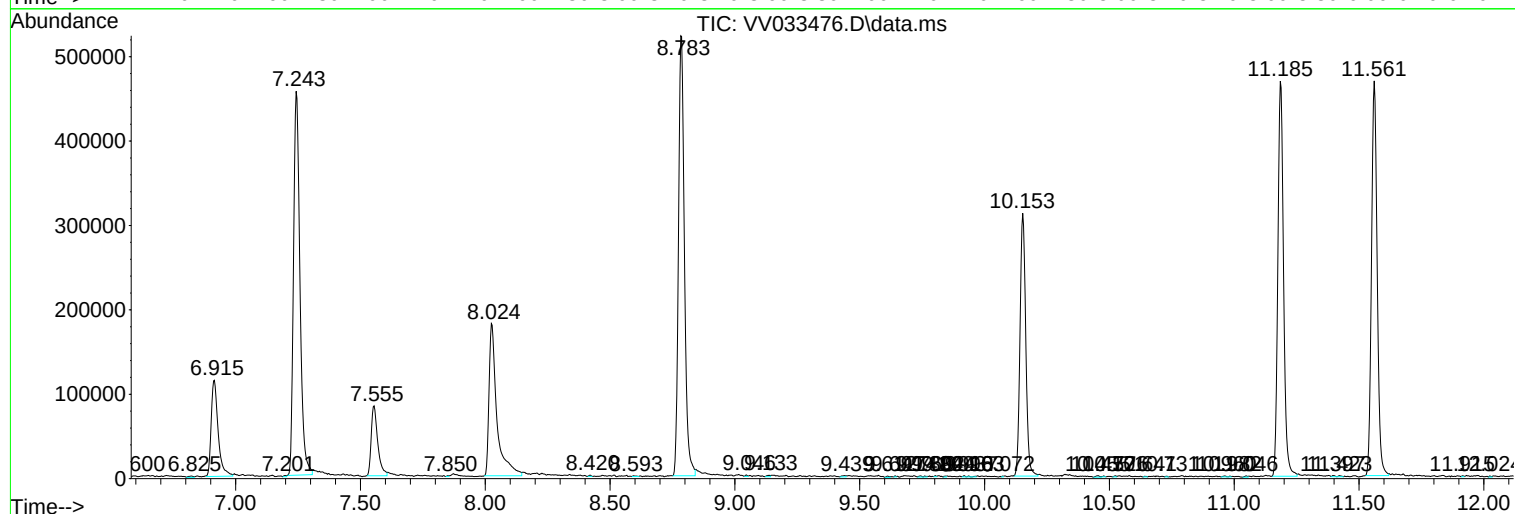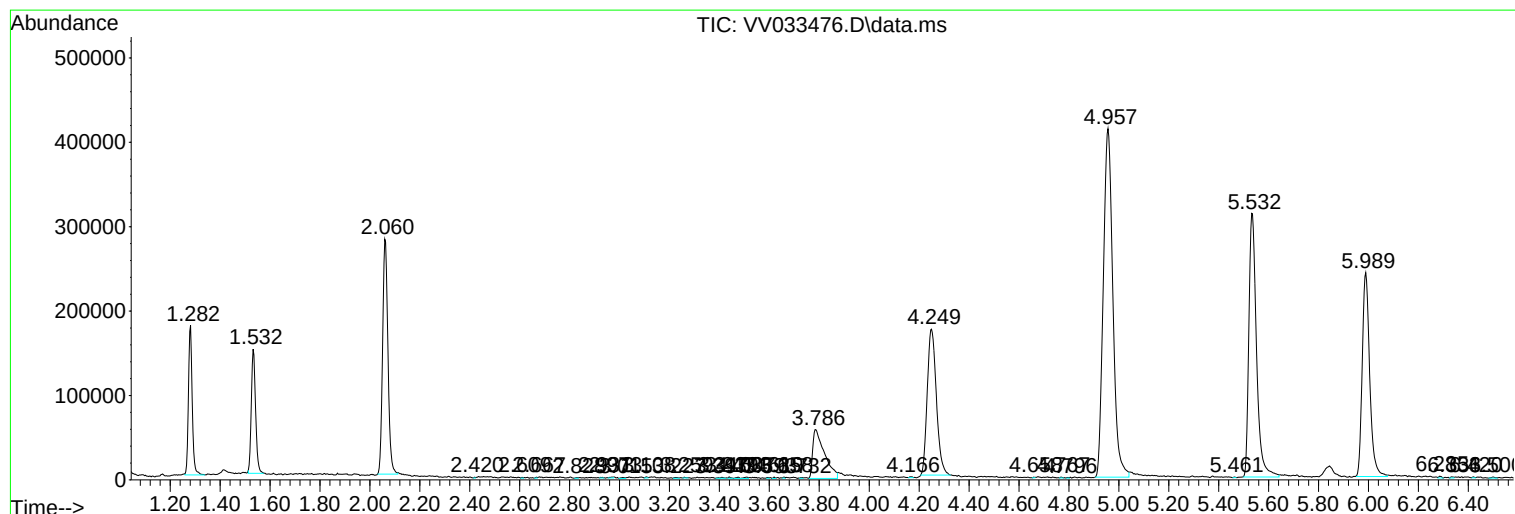

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033476.D
Acq On : 19 Dec 2023 14:35
Operator : SY/MD
Sample : 05912-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033476.D
Acq On : 19 Dec 2023 14:35
Operator : SY/MD
Sample : 05912-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc