

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033477.D
 Acq On : 19 Dec 2023 14:58
 Operator : SY/MD
 Sample : 05912-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	162191	171491	16.07%	2.181%
2	1.532	146	153	168	rVB	143158	169387	15.87%	2.154%
3	2.060	308	317	332	rBV	266199	387980	36.35%	4.935%
4	2.478	445	447	452	rBV5	1112	771	0.07%	0.010%
5	2.683	509	511	516	rBV7	1092	899	0.08%	0.011%
6	2.806	546	549	551	rBV3	1087	859	0.08%	0.011%
7	2.886	573	574	575	rBV2	848	239	0.02%	0.003%
8	2.989	605	606	610	rBV4	702	506	0.05%	0.006%
9	3.137	650	652	657	rBV6	1147	952	0.09%	0.012%
10	3.198	669	671	673	rBV3	650	370	0.03%	0.005%
11	3.246	680	686	688	rBV5	958	663	0.06%	0.008%
12	3.262	689	691	692	rBV	769	254	0.02%	0.003%
13	3.304	697	704	706	rBV7	1998	2248	0.21%	0.029%
14	3.352	717	719	720	rBV2	556	231	0.02%	0.003%
15	3.445	745	748	750	rBV3	1037	486	0.05%	0.006%
16	3.500	760	765	769	rVB8	1325	1238	0.12%	0.016%
17	3.523	769	772	775	rBV4	871	638	0.06%	0.008%
18	3.542	775	778	780	rBV4	1132	699	0.07%	0.009%
19	3.584	790	791	793	rBV	702	345	0.03%	0.004%
20	3.600	793	796	798	rVV4	1037	785	0.07%	0.010%
21	3.680	818	821	822	rBV3	855	447	0.04%	0.006%
22	3.696	822	826	829	rVV5	1013	843	0.08%	0.011%
23	3.786	846	854	879	rBV2	52986	152518	14.29%	1.940%
24	4.249	985	998	1025	rVB	167681	427657	40.06%	5.439%
25	4.696	1135	1137	1139	rBV3	1369	536	0.05%	0.007%
26	4.957	1200	1218	1245	rBV2	392666	1067420	100.00%	13.577%
27	5.532	1386	1397	1423	rBV	314435	660748	61.90%	8.404%
28	5.989	1527	1539	1559	rBV2	228783	477757	44.76%	6.077%
29	6.442	1678	1680	1681	rBV2	779	360	0.03%	0.005%
30	6.478	1687	1691	1692	rBV4	1052	568	0.05%	0.007%
31	6.564	1716	1718	1724	rVB6	787	727	0.07%	0.009%
32	6.593	1724	1727	1729	rBV4	864	603	0.06%	0.008%
33	6.728	1766	1769	1772	rBV4	1089	1002	0.09%	0.013%
34	6.915	1817	1827	1847	rBV	106895	207377	19.43%	2.638%
35	7.162	1901	1904	1907	rBV5	991	670	0.06%	0.009%
36	7.243	1919	1929	1949	rBV	434532	772654	72.39%	9.827%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033477.D
 Acq On : 19 Dec 2023 14:58
 Operator : SY/MD
 Sample : 05912-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.555	2017	2026	2054	rBV	78397	150675	14.12%	1.916%
38	7.854	2117	2119	2120	rBV2	939	295	0.03%	0.004%
39	7.931	2138	2143	2145	rBV5	1141	819	0.08%	0.010%
40	7.944	2145	2147	2149	rVB3	659	242	0.02%	0.003%
41	8.024	2163	2172	2202	rBV	169800	369728	34.64%	4.703%
42	8.686	2375	2378	2380	rBV4	1636	892	0.08%	0.011%
43	8.783	2398	2408	2434	rBV	519628	872516	81.74%	11.098%
44	9.178	2529	2531	2533	rBV3	827	298	0.03%	0.004%
45	9.262	2556	2557	2561	rVB3	1164	510	0.05%	0.006%
46	9.423	2604	2607	2608	rBV3	727	429	0.04%	0.005%
47	9.493	2627	2629	2632	rBV3	852	483	0.05%	0.006%
48	9.561	2646	2650	2653	rBV6	1459	1246	0.12%	0.016%
49	9.619	2665	2668	2675	rVB6	2283	2175	0.20%	0.028%
50	9.651	2675	2678	2680	rBV3	1373	939	0.09%	0.012%
51	9.683	2685	2688	2691	rBV4	1063	664	0.06%	0.008%
52	9.847	2738	2739	2741	rVB2	958	187	0.02%	0.002%
53	9.911	2757	2759	2764	rVB4	729	616	0.06%	0.008%
54	9.934	2764	2766	2769	rBV3	909	489	0.05%	0.006%
55	10.153	2823	2834	2860	rVB	294147	466862	43.74%	5.938%
56	10.448	2924	2926	2930	rBV5	1222	883	0.08%	0.011%
57	10.574	2963	2965	2966	rBV	528	163	0.02%	0.002%
58	10.587	2966	2969	2971	rVV4	1258	758	0.07%	0.010%
59	10.600	2971	2973	2975	rVV2	989	373	0.03%	0.005%
60	10.690	3000	3001	3003	rBV	684	297	0.03%	0.004%
61	10.699	3003	3004	3007	rVB2	975	312	0.03%	0.004%
62	10.731	3011	3014	3017	rBV4	1344	916	0.09%	0.012%
63	10.873	3054	3058	3063	rBV7	1507	1489	0.14%	0.019%
64	10.944	3074	3080	3083	rBV7	1017	1243	0.12%	0.016%
65	11.005	3097	3099	3102	rBV4	849	724	0.07%	0.009%
66	11.185	3143	3155	3176	rBV	468481	745189	69.81%	9.478%
67	11.423	3227	3229	3233	rVB4	1364	669	0.06%	0.009%
68	11.481	3245	3247	3250	rBV4	1016	702	0.07%	0.009%
69	11.513	3255	3257	3260	rBV4	1103	866	0.08%	0.011%
70	11.561	3261	3272	3291	rVV	442688	704539	66.00%	8.961%
71	11.789	3340	3343	3345	rBV4	762	623	0.06%	0.008%
72	12.021	3413	3415	3417	rBV	883	503	0.05%	0.006%
73	12.091	3434	3437	3441	rBV4	1529	1017	0.10%	0.013%
74	12.397	3530	3532	3535	rVB2	894	396	0.04%	0.005%
75	12.410	3535	3536	3537	rBV	493	132	0.01%	0.002%
76	12.480	3556	3558	3561	rVB3	1294	704	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033477.D
 Acq On : 19 Dec 2023 14:58
 Operator : SY/MD
 Sample : 05912-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.625	3601	3603	3605	rBV3	1037	517	0.05%	0.007%
78	12.689	3620	3623	3624	rBV2	820	443	0.04%	0.006%
79	12.731	3632	3636	3637	rBV3	983	578	0.05%	0.007%
80	12.908	3685	3691	3693	rBV6	1025	1005	0.09%	0.013%
81	12.972	3710	3711	3712	rBV	518	175	0.02%	0.002%
82	13.059	3735	3738	3741	rVB3	729	369	0.03%	0.005%
83	13.075	3741	3743	3747	rVB5	828	374	0.04%	0.005%
84	13.101	3747	3751	3755	rBV6	1258	1251	0.12%	0.016%
85	13.162	3767	3770	3775	rBV5	1417	1426	0.13%	0.018%
86	13.255	3796	3799	3802	rVB5	1188	605	0.06%	0.008%
87	13.313	3815	3817	3820	rBV3	721	347	0.03%	0.004%
88	13.455	3857	3861	3866	rBV5	1700	1716	0.16%	0.022%
89	13.558	3890	3893	3894	rBV2	1247	690	0.06%	0.009%
90	13.712	3939	3941	3942	rBV2	1037	485	0.05%	0.006%
91	13.734	3946	3948	3951	rVV4	1205	640	0.06%	0.008%
92	13.853	3983	3985	3987	rBV2	1211	691	0.06%	0.009%
93	14.069	4050	4052	4056	rVB4	1553	1010	0.09%	0.013%
94	14.133	4071	4072	4075	rBV	432	203	0.02%	0.003%
95	14.156	4075	4079	4081	rBV4	1045	569	0.05%	0.007%
96	14.172	4081	4084	4085	rBV3	1509	758	0.07%	0.010%
97	14.496	4182	4185	4187	rBV4	1056	728	0.07%	0.009%
98	14.866	4298	4300	4302	rBV3	994	378	0.04%	0.005%
99	15.236	4412	4415	4420	rBV7	2066	1786	0.17%	0.023%




Sum of corrected areas: 7862235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033477.D
Acq On : 19 Dec 2023 14:58
Operator : SY/MD
Sample : 05912-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

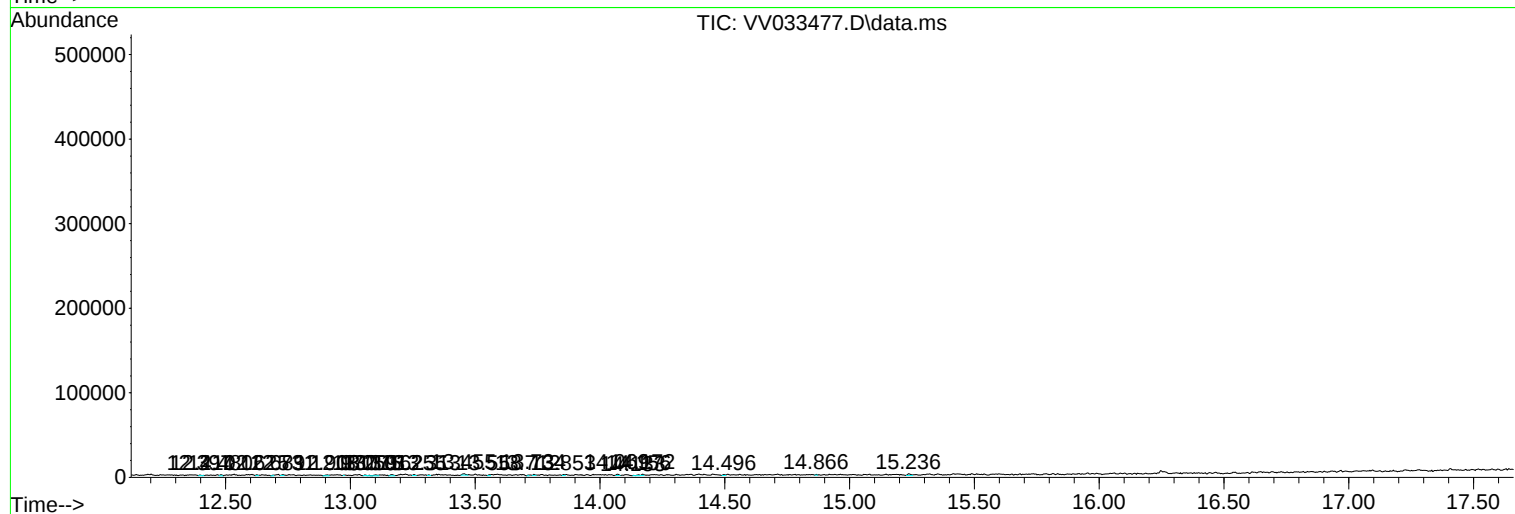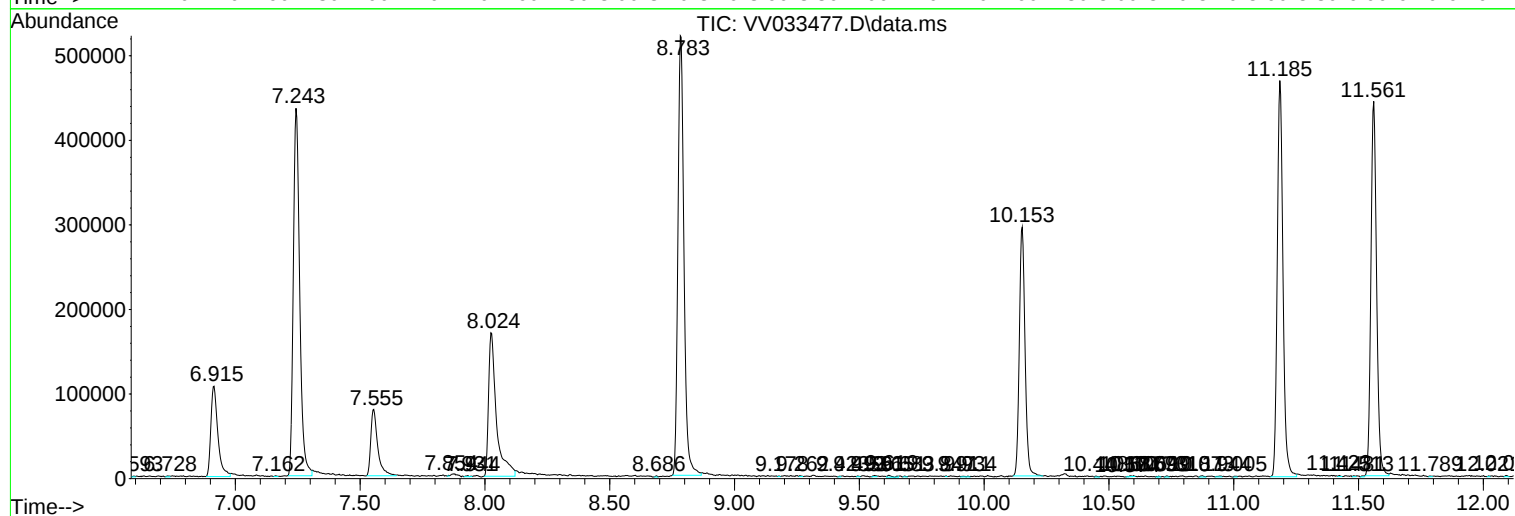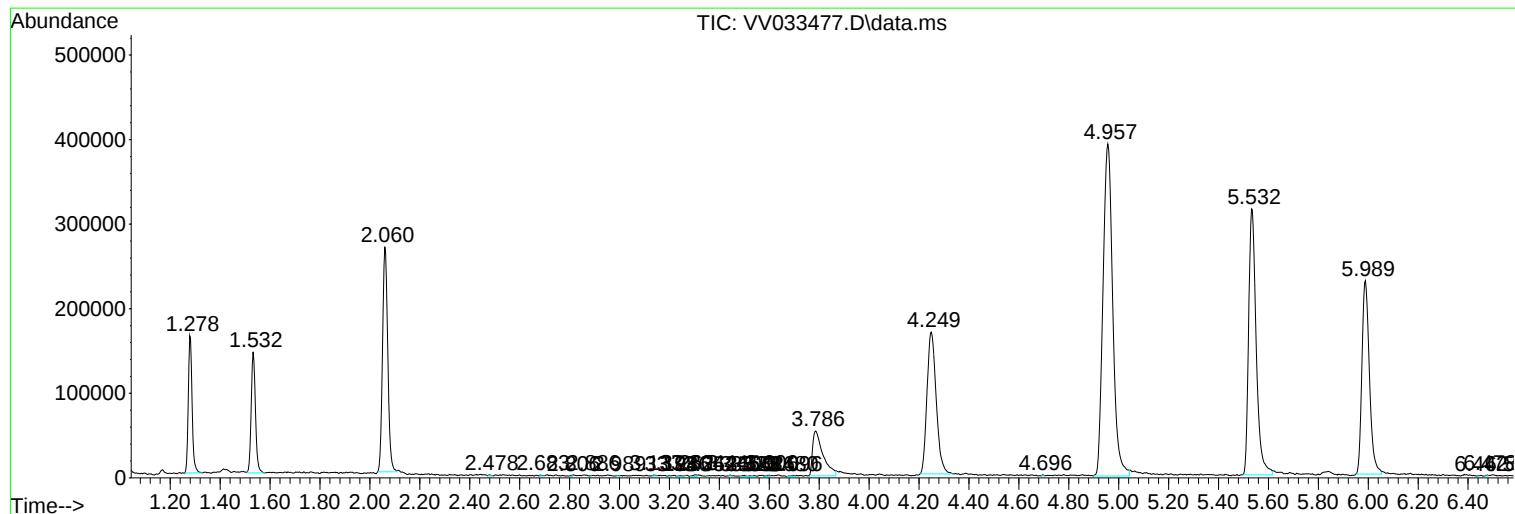

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033477.D
Acq On : 19 Dec 2023 14:58
Operator : SY/MD
Sample : 05912-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033477.D
Acq On : 19 Dec 2023 14:58
Operator : SY/MD
Sample : 05912-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc