

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033478.D
 Acq On : 19 Dec 2023 15:22
 Operator : SY/MD
 Sample : 05912-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3K9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	172034	175550	15.76%	2.134%
2	1.532	146	153	168	rVB	148625	176075	15.80%	2.141%
3	2.060	308	317	330	rBV	280011	412830	37.05%	5.019%
4	2.330	397	401	406	rBV6	1389	1708	0.15%	0.021%
5	2.429	430	432	435	rBV3	1358	1029	0.09%	0.013%
6	2.648	496	500	504	rVB6	1653	1379	0.12%	0.017%
7	2.864	563	567	570	rBV5	967	834	0.07%	0.010%
8	2.886	570	574	576	rVB5	1129	897	0.08%	0.011%
9	2.902	576	579	584	rBV5	936	875	0.08%	0.011%
10	2.979	596	603	604	rBV6	1157	1069	0.10%	0.013%
11	2.992	604	607	610	rVB4	1024	736	0.07%	0.009%
12	3.031	617	619	624	rBV6	917	730	0.07%	0.009%
13	3.201	669	672	675	rBV3	943	674	0.06%	0.008%
14	3.474	754	757	761	rVB5	1072	825	0.07%	0.010%
15	3.690	822	824	827	rVB4	1230	649	0.06%	0.008%
16	3.709	827	830	833	rBV5	1129	514	0.05%	0.006%
17	3.783	845	853	877	rBV	54644	155785	13.98%	1.894%
18	4.246	982	997	1024	rBV	173024	454206	40.76%	5.522%
19	4.690	1131	1135	1136	rBV3	1186	898	0.08%	0.011%
20	4.818	1173	1175	1179	rBV4	697	588	0.05%	0.007%
21	4.957	1199	1218	1247	rBV2	416407	1114214	100.00%	13.546%
22	5.535	1386	1398	1423	rBV	330256	692447	62.15%	8.419%
23	5.989	1527	1539	1565	rBV2	242132	504966	45.32%	6.139%
24	6.388	1658	1663	1665	rBV5	1368	1009	0.09%	0.012%
25	6.404	1665	1668	1674	rBV7	1315	1499	0.13%	0.018%
26	6.481	1690	1692	1695	rVB2	1304	668	0.06%	0.008%
27	6.506	1698	1700	1703	rBV4	1247	1028	0.09%	0.012%
28	6.812	1793	1795	1798	rBV3	1121	814	0.07%	0.010%
29	6.867	1808	1812	1814	rBV5	1253	1127	0.10%	0.014%
30	6.912	1816	1826	1849	rVV	113014	219399	19.69%	2.667%
31	7.243	1918	1929	1950	rBV	459030	811123	72.80%	9.861%
32	7.551	2017	2025	2043	rBV	82776	149200	13.39%	1.814%
33	7.789	2098	2099	2102	rVB2	1257	647	0.06%	0.008%
34	7.828	2109	2111	2116	rVB4	1314	804	0.07%	0.010%
35	7.850	2116	2118	2119	rBV2	1540	576	0.05%	0.007%
36	7.986	2157	2160	2162	rBV3	1288	934	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033478.D
 Acq On : 19 Dec 2023 15:22
 Operator : SY/MD
 Sample : 05912-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3K9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.024	2163	2172	2197	rBV	179626	378145	33.94%	4.597%
38	8.423	2294	2296	2299	rVB5	1329	563	0.05%	0.007%
39	8.571	2337	2342	2343	rBV3	1159	881	0.08%	0.011%
40	8.731	2388	2392	2394	rBV5	963	860	0.08%	0.010%
41	8.786	2398	2409	2436	rVV	542730	907364	81.44%	11.031%
42	9.313	2569	2573	2575	rVB5	1427	865	0.08%	0.011%
43	9.333	2575	2579	2580	rBV3	936	555	0.05%	0.007%
44	9.596	2658	2661	2664	rBV5	1150	695	0.06%	0.008%
45	9.696	2686	2692	2694	rVB5	1144	1171	0.11%	0.014%
46	9.722	2694	2700	2701	rBV4	1781	1539	0.14%	0.019%
47	9.757	2708	2711	2713	rBV3	2138	1318	0.12%	0.016%
48	9.812	2723	2728	2734	rBV7	1447	1561	0.14%	0.019%
49	9.860	2740	2743	2747	rBV5	1504	1462	0.13%	0.018%
50	9.879	2747	2749	2754	rVV6	1593	1115	0.10%	0.014%
51	9.915	2758	2760	2766	rVB6	1406	617	0.06%	0.008%
52	10.153	2823	2834	2852	rBV	305178	483670	43.41%	5.880%
53	10.329	2881	2889	2899	rVB	3386	6351	0.57%	0.077%
54	10.407	2911	2913	2916	rVB4	1373	556	0.05%	0.007%
55	10.461	2926	2930	2932	rBV5	1541	1073	0.10%	0.013%
56	10.522	2945	2949	2950	rBV3	1457	1029	0.09%	0.013%
57	10.648	2985	2988	2991	rBV5	1230	728	0.07%	0.009%
58	10.715	3007	3009	3014	rVB6	1200	784	0.07%	0.010%
59	10.747	3014	3019	3023	rBV7	1387	1520	0.14%	0.018%
60	10.792	3029	3033	3036	rBV6	1020	837	0.08%	0.010%
61	10.857	3048	3053	3056	rBV6	1222	1061	0.10%	0.013%
62	11.185	3144	3155	3180	rBV	489573	768422	68.97%	9.342%
63	11.365	3209	3211	3214	rBV4	1201	894	0.08%	0.011%
64	11.426	3227	3230	3234	rBV4	1547	1292	0.12%	0.016%
65	11.452	3236	3238	3243	rVB5	1636	1126	0.10%	0.014%
66	11.500	3248	3253	3256	rBV4	1811	1607	0.14%	0.020%
67	11.561	3261	3272	3291	rVV	466959	734975	65.96%	8.936%
68	11.731	3321	3325	3327	rBV4	1174	814	0.07%	0.010%
69	11.783	3339	3341	3345	rBV5	959	603	0.05%	0.007%
70	11.918	3379	3383	3385	rVB5	1280	742	0.07%	0.009%
71	12.018	3411	3414	3415	rBV3	1124	537	0.05%	0.007%
72	12.088	3433	3436	3438	rBV4	1324	966	0.09%	0.012%
73	12.484	3555	3559	3561	rBV4	1106	806	0.07%	0.010%
74	12.583	3585	3590	3593	rBV8	1671	1725	0.15%	0.021%
75	12.638	3606	3607	3613	rVB6	1477	926	0.08%	0.011%
76	12.715	3627	3631	3632	rBV3	1559	1062	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033478.D
 Acq On : 19 Dec 2023 15:22
 Operator : SY/MD
 Sample : 05912-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3K9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.876	3676	3681	3684	rBV5	1481	1025	0.09%	0.012%
78	12.947	3699	3703	3706	rBV4	1173	1033	0.09%	0.013%
79	12.976	3709	3712	3717	rVV5	1379	1163	0.10%	0.014%
80	13.008	3720	3722	3726	rVB4	777	512	0.05%	0.006%
81	13.030	3726	3729	3732	rBV3	1033	821	0.07%	0.010%
82	13.072	3740	3742	3745	rVB3	1370	542	0.05%	0.007%
83	13.120	3754	3757	3759	rVB3	1357	774	0.07%	0.009%
84	13.345	3822	3827	3831	rBV8	1288	1453	0.13%	0.018%
85	13.413	3845	3848	3850	rBV4	1066	790	0.07%	0.010%
86	13.426	3850	3852	3856	rVB3	1459	680	0.06%	0.008%
87	13.751	3949	3953	3955	rBV4	1216	904	0.08%	0.011%
88	13.844	3977	3982	3985	rBV6	1016	1098	0.10%	0.013%
89	13.882	3990	3994	3997	rVB6	804	630	0.06%	0.008%
90	13.950	4011	4015	4017	rBV5	1179	904	0.08%	0.011%
91	13.979	4021	4024	4026	rBV4	1014	624	0.06%	0.008%
92	14.091	4055	4059	4061	rBV4	1419	1076	0.10%	0.013%
93	14.371	4140	4146	4150	rVB7	1707	1906	0.17%	0.023%
94	14.394	4150	4153	4156	rBV5	1883	1519	0.14%	0.018%
95	14.423	4157	4162	4163	rBV5	1258	835	0.07%	0.010%
96	14.648	4228	4232	4234	rBV3	1042	700	0.06%	0.009%
97	14.979	4329	4335	4338	rBV4	1253	1387	0.12%	0.017%
98	15.140	4382	4385	4392	rVB8	1739	1474	0.13%	0.018%
99	15.178	4392	4397	4399	rBV6	1686	1417	0.13%	0.017%
100	15.332	4443	4445	4448	rBV4	1057	834	0.07%	0.010%




Sum of corrected areas: 8225224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033478.D
Acq On : 19 Dec 2023 15:22
Operator : SY/MD
Sample : 05912-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

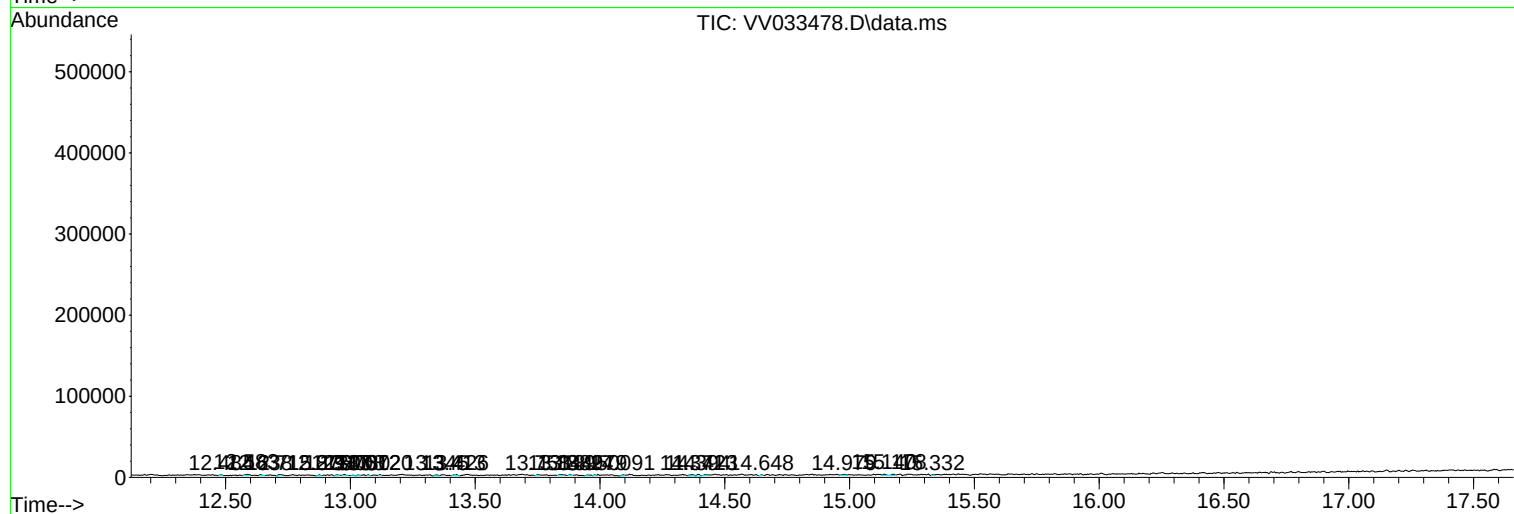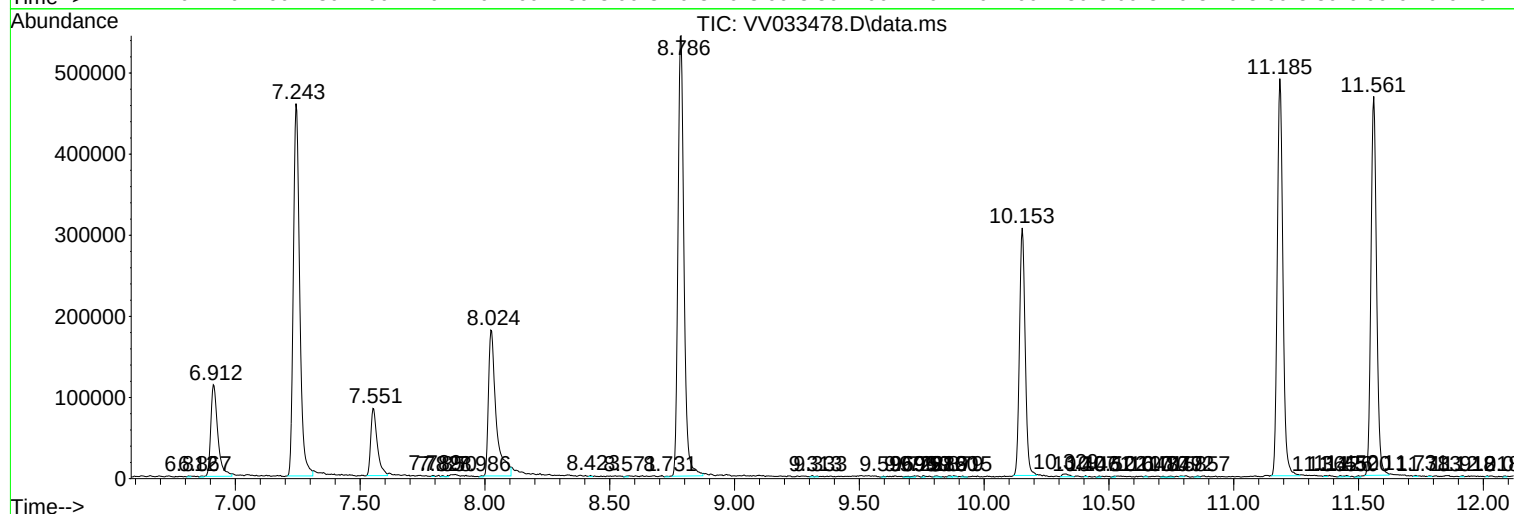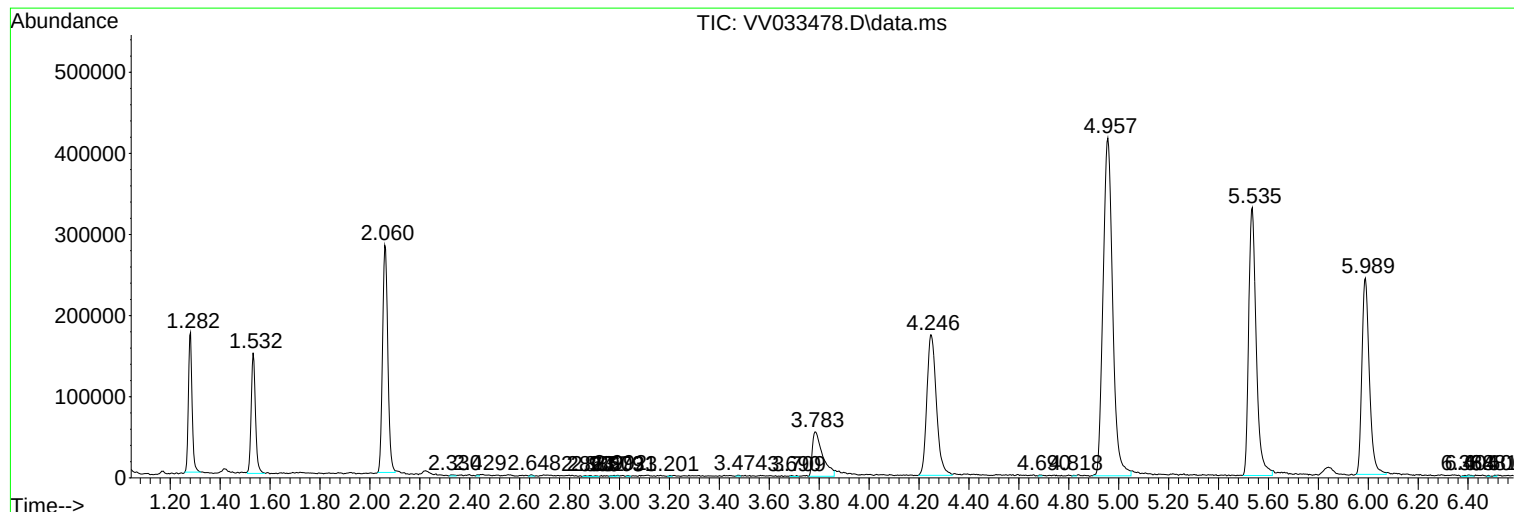

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033478.D
Acq On : 19 Dec 2023 15:22
Operator : SY/MD
Sample : 05912-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033478.D
Acq On : 19 Dec 2023 15:22
Operator : SY/MD
Sample : 05912-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------