

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033479.D
 Acq On : 19 Dec 2023 15:45
 Operator : SY/MD
 Sample : 05912-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VW033479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	163685	174326	16.35%	2.161%
2	1.532	146	153	168	rVB	143312	170712	16.01%	2.116%
3	2.060	308	317	343	rVB	273027	410270	38.47%	5.086%
4	2.275	382	384	386	rBV3	1343	909	0.09%	0.011%
5	2.394	418	421	423	rBV3	1146	622	0.06%	0.008%
6	2.426	428	431	435	rBV6	1317	1196	0.11%	0.015%
7	2.487	448	450	453	rVB2	1183	619	0.06%	0.008%
8	2.529	461	463	465	rBV4	944	493	0.05%	0.006%
9	2.545	465	468	469	rBV3	1803	856	0.08%	0.011%
10	2.703	513	517	518	rBV4	892	603	0.06%	0.007%
11	2.728	523	525	529	rBV3	1423	1137	0.11%	0.014%
12	2.796	542	546	547	rBV4	1585	988	0.09%	0.012%
13	2.863	564	567	570	rBV5	1092	935	0.09%	0.012%
14	3.050	622	625	628	rBV5	931	614	0.06%	0.008%
15	3.230	676	681	686	rBV7	1159	1360	0.13%	0.017%
16	3.355	715	720	724	rBV5	1092	914	0.09%	0.011%
17	3.384	724	729	732	rBV7	1115	1181	0.11%	0.015%
18	3.455	749	751	753	rVB2	1337	504	0.05%	0.006%
19	3.468	753	755	758	rBV3	804	580	0.05%	0.007%
20	3.513	766	769	771	rBV4	909	568	0.05%	0.007%
21	3.523	771	772	777	rVV6	856	736	0.07%	0.009%
22	3.783	844	853	875	rBV	58988	168316	15.78%	2.087%
23	4.249	985	998	1026	rVB	169163	433903	40.68%	5.379%
24	4.780	1161	1163	1165	rBV3	1105	661	0.06%	0.008%
25	4.857	1181	1187	1191	rBV8	1379	1639	0.15%	0.020%
26	4.957	1201	1218	1252	rBV2	395021	1066508	100.00%	13.222%
27	5.532	1385	1397	1419	rBV	323212	678857	63.65%	8.416%
28	5.834	1480	1491	1508	rBV	9827	27287	2.56%	0.338%
29	5.924	1517	1519	1521	rBV2	1154	717	0.07%	0.009%
30	5.989	1526	1539	1568	rVV	233307	492381	46.17%	6.104%
31	6.436	1675	1678	1681	rBV3	1424	1035	0.10%	0.013%
32	6.516	1701	1703	1707	rVB4	1318	608	0.06%	0.008%
33	6.699	1758	1760	1764	rBV5	1021	717	0.07%	0.009%
34	6.748	1772	1775	1780	rBV6	1245	1234	0.12%	0.015%
35	6.815	1793	1796	1797	rBV2	1475	915	0.09%	0.011%
36	6.844	1804	1805	1808	rBV2	983	511	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033479.D
 Acq On : 19 Dec 2023 15:45
 Operator : SY/MD
 Sample : 05912-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.915	1817	1827	1846	rBV	108384	205016	19.22%	2.542%
38	7.243	1918	1929	1952	rBV	434528	771318	72.32%	9.562%
39	7.555	2016	2026	2043	rBV	81226	145002	13.60%	1.798%
40	7.944	2143	2147	2149	rBV4	1164	953	0.09%	0.012%
41	8.024	2164	2172	2210	rBV	185212	398508	37.37%	4.940%
42	8.632	2359	2361	2362	rBV2	1289	517	0.05%	0.006%
43	8.786	2398	2409	2440	rBV	529615	898299	84.23%	11.136%
44	9.185	2531	2533	2535	rBV3	1124	588	0.06%	0.007%
45	9.342	2581	2582	2587	rBV5	993	549	0.05%	0.007%
46	9.403	2599	2601	2604	rBV4	1676	847	0.08%	0.011%
47	9.500	2629	2631	2634	rVB3	1158	696	0.07%	0.009%
48	9.567	2650	2652	2656	rBV5	962	694	0.07%	0.009%
49	9.699	2690	2693	2695	rBV4	689	534	0.05%	0.007%
50	9.712	2695	2697	2699	rVB4	1173	490	0.05%	0.006%
51	9.821	2727	2731	2736	rVB7	754	626	0.06%	0.008%
52	9.937	2764	2767	2768	rBV2	1101	572	0.05%	0.007%
53	9.979	2778	2780	2784	rVB5	1328	609	0.06%	0.008%
54	10.153	2823	2834	2855	rVV	294126	477719	44.79%	5.922%
55	10.381	2903	2905	2908	rBV4	902	595	0.06%	0.007%
56	10.487	2936	2938	2942	rBV4	981	727	0.07%	0.009%
57	10.535	2951	2953	2958	rVB4	1085	874	0.08%	0.011%
58	10.644	2985	2987	2989	rBV3	812	513	0.05%	0.006%
59	10.667	2992	2994	2998	rVB4	1014	538	0.05%	0.007%
60	10.989	3093	3094	3099	rVV4	843	492	0.05%	0.006%
61	11.104	3127	3130	3133	rBV4	848	517	0.05%	0.006%
62	11.130	3133	3138	3140	rBV6	2508	1954	0.18%	0.024%
63	11.185	3145	3155	3180	rVB	488175	764124	71.65%	9.473%
64	11.410	3219	3225	3226	rBV3	1460	1532	0.14%	0.019%
65	11.461	3238	3241	3244	rBV4	886	637	0.06%	0.008%
66	11.506	3247	3255	3258	rBV7	3746	5136	0.48%	0.064%
67	11.561	3261	3272	3296	rVB	445524	711736	66.74%	8.824%
68	11.947	3388	3392	3394	rBV4	1600	1308	0.12%	0.016%
69	12.062	3425	3428	3430	rBV3	1729	1086	0.10%	0.013%
70	12.133	3447	3450	3453	rBV4	1380	625	0.06%	0.008%
71	12.255	3485	3488	3489	rBV2	956	520	0.05%	0.006%
72	12.291	3495	3499	3503	rVB4	1489	1275	0.12%	0.016%
73	12.313	3503	3506	3508	rBV3	1107	598	0.06%	0.007%
74	12.333	3508	3512	3513	rBV2	1189	763	0.07%	0.009%
75	12.506	3564	3566	3568	rBV3	1241	527	0.05%	0.007%
76	12.702	3625	3627	3632	rVB5	842	491	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033479.D
 Acq On : 19 Dec 2023 15:45
 Operator : SY/MD
 Sample : 05912-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.734	3634	3637	3639	rBV3	1112	673	0.06%	0.008%
78	12.860	3672	3676	3678	rBV5	1040	547	0.05%	0.007%
79	13.291	3803	3810	3816	rBV10	1684	2205	0.21%	0.027%
80	13.381	3835	3838	3841	rVB3	938	631	0.06%	0.008%
81	13.442	3853	3857	3858	rBV3	1652	1214	0.11%	0.015%
82	13.503	3874	3876	3879	rBV3	833	596	0.06%	0.007%
83	13.545	3883	3889	3892	rBV6	1384	1888	0.18%	0.023%
84	13.622	3911	3913	3916	rBV2	881	681	0.06%	0.008%
85	13.670	3925	3928	3931	rBV4	978	776	0.07%	0.010%
86	13.715	3939	3942	3944	rBV4	944	634	0.06%	0.008%
87	13.818	3973	3974	3978	rVB3	994	542	0.05%	0.007%
88	13.898	3997	3999	4001	rBV3	1051	568	0.05%	0.007%
89	13.982	4024	4025	4031	rBV5	972	590	0.06%	0.007%
90	14.078	4052	4055	4060	rVB5	1001	873	0.08%	0.011%
91	14.140	4072	4074	4077	rBV4	1070	615	0.06%	0.008%
92	14.168	4081	4083	4084	rBV2	1108	541	0.05%	0.007%
93	14.342	4133	4137	4139	rBV5	742	538	0.05%	0.007%
94	14.429	4162	4164	4167	rVB4	1456	673	0.06%	0.008%
95	14.718	4248	4254	4255	rBV5	1397	970	0.09%	0.012%
96	14.914	4312	4315	4320	rBV4	964	1069	0.10%	0.013%
97	15.165	4391	4393	4396	rBV3	1254	530	0.05%	0.007%
98	15.197	4401	4403	4406	rBV4	1110	650	0.06%	0.008%
99	15.297	4430	4434	4439	rBV6	1747	1819	0.17%	0.023%
100	15.413	4467	4470	4472	rBV2	1193	932	0.09%	0.012%




Sum of corrected areas: 8066272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033479.D
Acq On : 19 Dec 2023 15:45
Operator : SY/MD
Sample : 05912-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

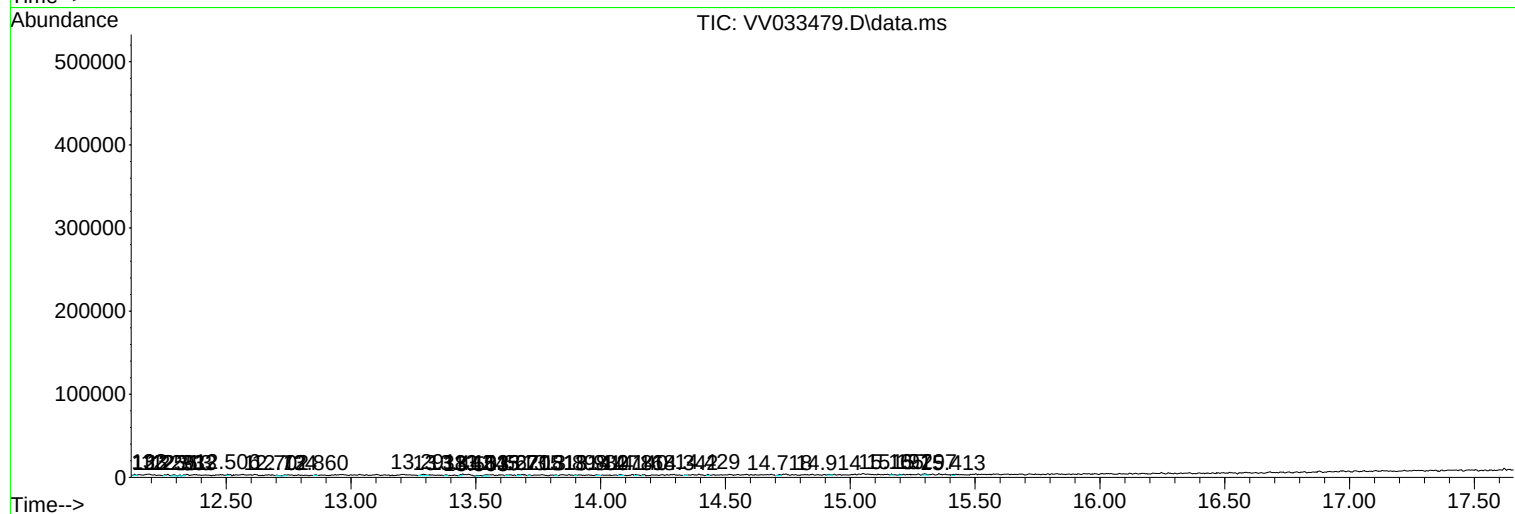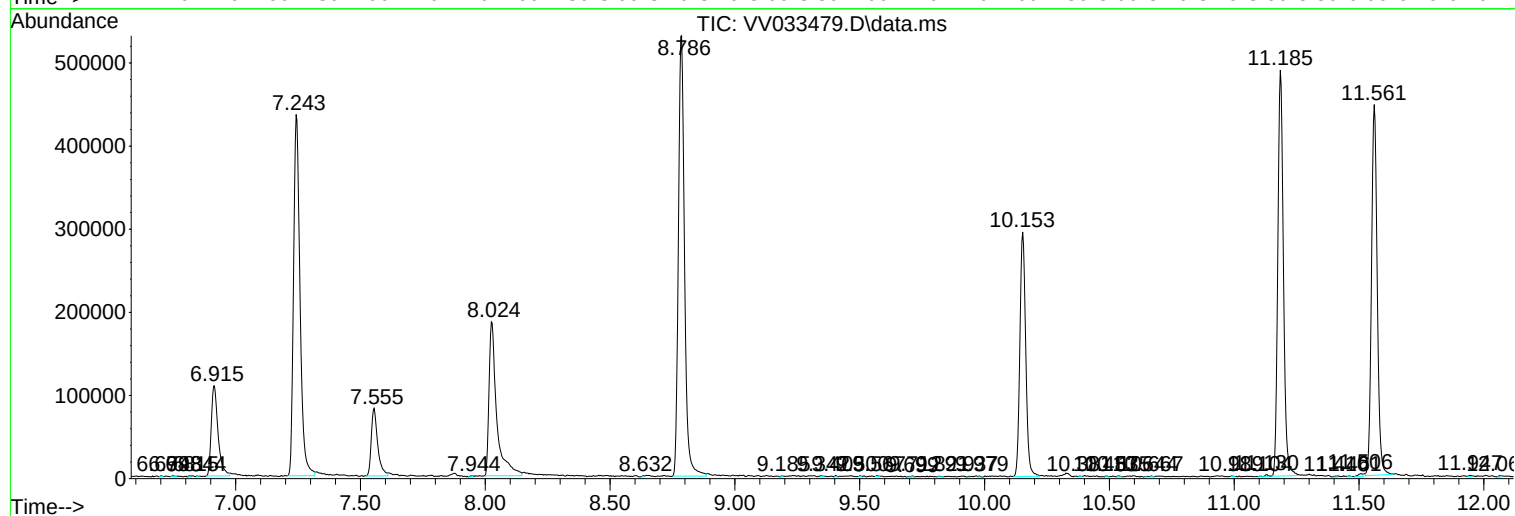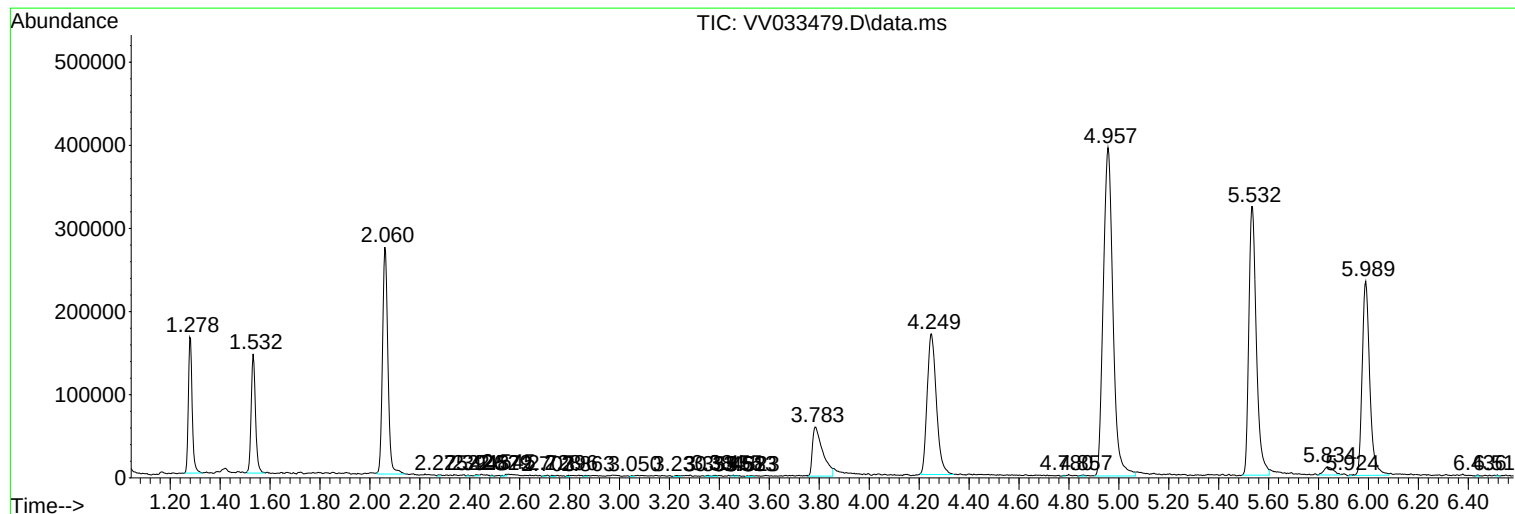

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033479.D
Acq On : 19 Dec 2023 15:45
Operator : SY/MD
Sample : 05912-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033479.D
Acq On : 19 Dec 2023 15:45
Operator : SY/MD
Sample : 05912-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc