

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033481.D
 Acq On : 19 Dec 2023 16:31
 Operator : SY/MD
 Sample : 05912-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	48	rBV	7599	9455	0.90%	0.121%
2	1.282	68	75	92	rBV	160886	170398	16.21%	2.186%
3	1.532	147	153	167	rVB	142350	164341	15.63%	2.109%
4	2.060	309	317	333	rVB	263320	380455	36.18%	4.882%
5	2.680	506	510	513	rBV6	895	830	0.08%	0.011%
6	2.835	556	558	562	rVB5	1069	628	0.06%	0.008%
7	3.076	631	633	638	rBV4	1341	973	0.09%	0.012%
8	3.134	650	651	653	rBV2	1076	401	0.04%	0.005%
9	3.236	681	683	688	rBV3	1388	1015	0.10%	0.013%
10	3.275	692	695	696	rBV3	1067	559	0.05%	0.007%
11	3.333	710	713	716	rBV5	1706	1128	0.11%	0.014%
12	3.388	728	730	734	rVB3	1255	702	0.07%	0.009%
13	3.420	738	740	741	rVV	959	419	0.04%	0.005%
14	3.439	744	746	748	rVB3	1284	484	0.05%	0.006%
15	3.494	761	763	766	rBV4	921	534	0.05%	0.007%
16	3.526	769	773	774	rBV3	1171	704	0.07%	0.009%
17	3.638	806	808	810	rBV2	756	441	0.04%	0.006%
18	3.757	842	845	846	rBV2	921	599	0.06%	0.008%
19	3.786	846	854	876	rBV	48884	134424	12.78%	1.725%
20	4.249	984	998	1026	rVB	167333	433455	41.22%	5.562%
21	4.625	1110	1115	1116	rBV3	989	739	0.07%	0.009%
22	4.847	1182	1184	1185	rBV2	975	386	0.04%	0.005%
23	4.957	1202	1218	1251	rBV3	390189	1051460	100.00%	13.492%
24	5.494	1380	1385	1386	rBV4	1559	1211	0.12%	0.016%
25	5.535	1386	1398	1422	rVV	310218	654142	62.21%	8.394%
26	5.822	1480	1487	1489	rBV7	3730	3868	0.37%	0.050%
27	5.941	1520	1524	1525	rBV4	1310	930	0.09%	0.012%
28	5.989	1527	1539	1562	rVV	230216	483140	45.95%	6.199%
29	6.439	1677	1679	1682	rBV3	1369	815	0.08%	0.010%
30	6.548	1711	1713	1714	rBV3	982	462	0.04%	0.006%
31	6.677	1751	1753	1755	rBV3	731	486	0.05%	0.006%
32	6.812	1794	1795	1799	rVB3	1182	574	0.05%	0.007%
33	6.915	1817	1827	1844	rBV	107349	200581	19.08%	2.574%
34	7.243	1918	1929	1953	rBV	429898	772666	73.49%	9.914%
35	7.555	2017	2026	2044	rBV2	77557	141442	13.45%	1.815%
36	7.838	2111	2114	2116	rBV3	1323	918	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033481.D
 Acq On : 19 Dec 2023 16:31
 Operator : SY/MD
 Sample : 05912-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.024	2164	2172	2210	rBV2	163227	365994	34.81%	4.696%
38	8.783	2397	2408	2439	rBV	518429	877066	83.41%	11.254%
39	9.149	2519	2522	2523	rBV2	1292	573	0.05%	0.007%
40	9.284	2562	2564	2568	rVB3	1515	744	0.07%	0.010%
41	9.313	2568	2573	2574	rBV5	1530	1428	0.14%	0.018%
42	9.358	2582	2587	2590	rBV6	1271	1297	0.12%	0.017%
43	9.445	2611	2614	2616	rBV4	880	711	0.07%	0.009%
44	9.629	2668	2671	2673	rVV4	858	561	0.05%	0.007%
45	9.648	2676	2677	2680	rVB2	807	371	0.04%	0.005%
46	9.677	2684	2686	2690	rVV4	1000	580	0.06%	0.007%
47	9.747	2706	2708	2712	rBV4	915	600	0.06%	0.008%
48	9.792	2720	2722	2725	rBV3	1158	666	0.06%	0.009%
49	9.895	2751	2754	2761	rVB9	1671	1701	0.16%	0.022%
50	9.953	2771	2772	2775	rBV3	744	462	0.04%	0.006%
51	10.018	2789	2792	2793	rBV3	1520	736	0.07%	0.009%
52	10.027	2793	2795	2796	rBV2	920	366	0.03%	0.005%
53	10.072	2806	2809	2811	rBV4	1439	797	0.08%	0.010%
54	10.153	2824	2834	2851	rBV	288839	455686	43.34%	5.847%
55	10.384	2903	2906	2907	rBV3	1096	546	0.05%	0.007%
56	10.468	2928	2932	2936	rBV6	1127	1107	0.11%	0.014%
57	10.571	2962	2964	2967	rVB2	1385	742	0.07%	0.010%
58	10.815	3038	3040	3042	rBV3	1025	586	0.06%	0.008%
59	10.860	3050	3054	3056	rBV4	772	570	0.05%	0.007%
60	11.050	3110	3113	3116	rBV5	1088	862	0.08%	0.011%
61	11.104	3128	3130	3131	rBV2	1308	439	0.04%	0.006%
62	11.185	3144	3155	3173	rBV	464734	736327	70.03%	9.448%
63	11.500	3251	3253	3254	rBV2	954	424	0.04%	0.005%
64	11.561	3262	3272	3293	rVB	444951	696438	66.24%	8.936%
65	11.828	3353	3355	3357	rBV3	1209	669	0.06%	0.009%
66	11.982	3401	3403	3405	rBV3	1205	628	0.06%	0.008%
67	12.220	3474	3477	3479	rBV3	957	537	0.05%	0.007%
68	12.233	3479	3481	3484	rVB4	1051	501	0.05%	0.006%
69	12.252	3484	3487	3490	rBV4	1086	634	0.06%	0.008%
70	12.275	3491	3494	3495	rBV3	1178	581	0.06%	0.007%
71	12.435	3538	3544	3545	rBV6	838	789	0.08%	0.010%
72	12.545	3572	3578	3579	rBV6	1151	1162	0.11%	0.015%
73	12.609	3596	3598	3601	rVB3	1224	716	0.07%	0.009%
74	12.725	3631	3634	3638	rBV5	1058	1115	0.11%	0.014%
75	12.786	3651	3653	3655	rVB3	1062	401	0.04%	0.005%
76	12.963	3706	3708	3710	rVB2	1338	543	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VV033481.D
 Acq On : 19 Dec 2023 16:31
 Operator : SY/MD
 Sample : 05912-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.014	3721	3724	3728	rBV4	1825	1603	0.15%	0.021%
78	13.085	3744	3746	3748	rBV3	915	586	0.06%	0.008%
79	13.149	3764	3766	3770	rVB5	1400	702	0.07%	0.009%
80	13.172	3771	3773	3777	rVB3	1042	487	0.05%	0.006%
81	13.204	3777	3783	3785	rBV6	1457	1471	0.14%	0.019%
82	13.271	3801	3804	3811	rBV6	1511	1798	0.17%	0.023%
83	13.368	3832	3834	3835	rBV2	1164	472	0.04%	0.006%
84	13.419	3848	3850	3851	rBV2	1056	450	0.04%	0.006%
85	13.554	3888	3892	3896	rBV7	1274	1045	0.10%	0.013%
86	13.574	3896	3898	3900	rBV3	956	550	0.05%	0.007%
87	13.632	3912	3916	3919	rBV6	1026	1015	0.10%	0.013%
88	13.677	3927	3930	3933	rBV4	742	576	0.05%	0.007%
89	13.706	3937	3939	3942	rVV4	1091	573	0.05%	0.007%
90	14.169	4081	4083	4086	rVB4	1181	603	0.06%	0.008%
91	14.197	4086	4092	4093	rBV5	1063	935	0.09%	0.012%
92	14.214	4095	4097	4102	rVB4	1161	803	0.08%	0.010%
93	14.291	4118	4121	4124	rBV5	923	609	0.06%	0.008%
94	14.487	4180	4182	4183	rBV2	1681	593	0.06%	0.008%
95	14.570	4206	4208	4210	rBV3	1014	408	0.04%	0.005%
96	14.779	4270	4273	4279	rBV6	1323	1470	0.14%	0.019%
97	14.863	4295	4299	4304	rBV8	1278	1538	0.15%	0.020%
98	15.349	4448	4450	4451	rBV2	1297	580	0.06%	0.007%
99	15.641	4539	4541	4542	rBV2	1256	487	0.05%	0.006%
100	15.705	4558	4561	4567	rVB3	1522	1561	0.15%	0.020%


Sum of corrected areas: 7793336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033481.D
Acq On : 19 Dec 2023 16:31
Operator : SY/MD
Sample : 05912-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

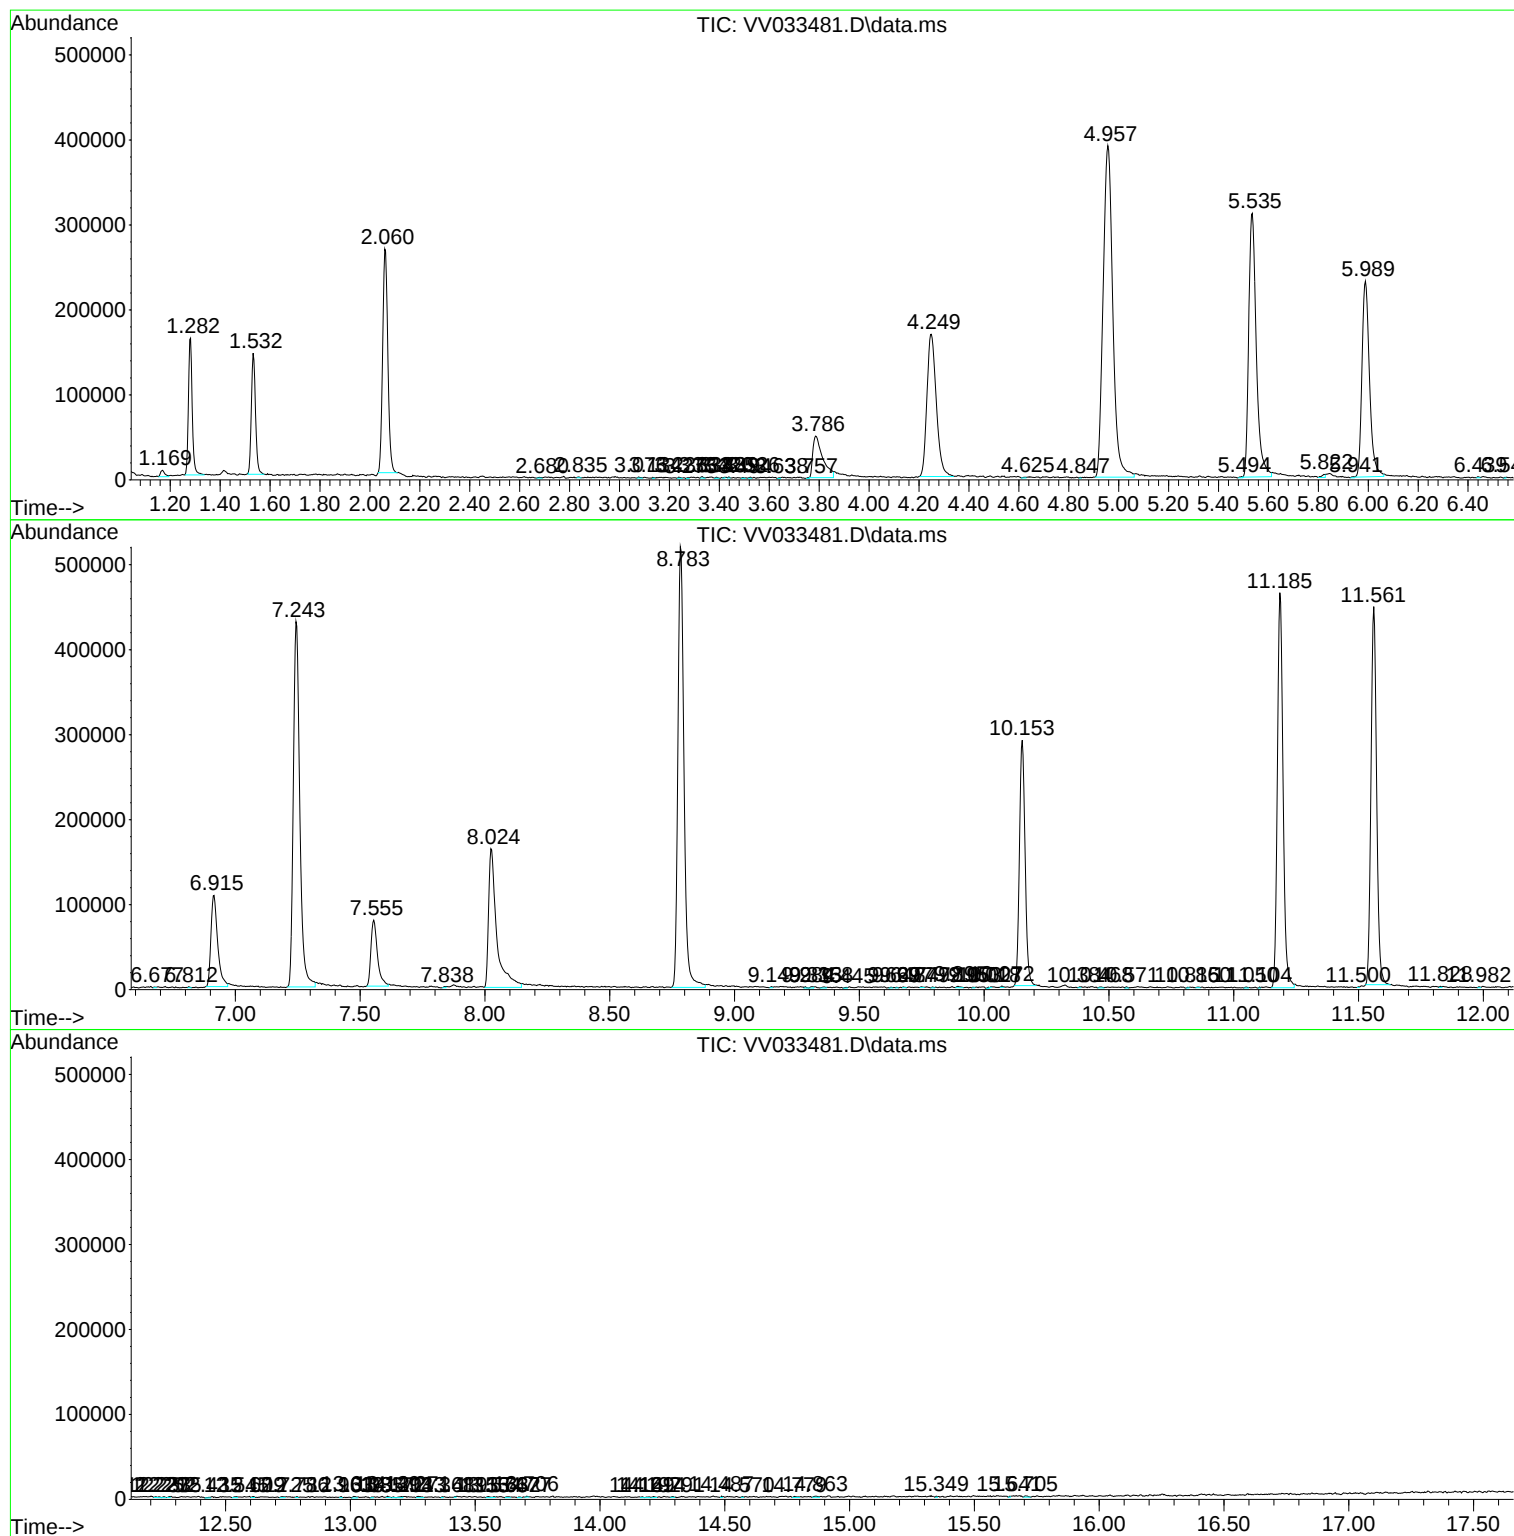

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033481.D
Acq On : 19 Dec 2023 16:31
Operator : SY/MD
Sample : 05912-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033481.D
Acq On : 19 Dec 2023 16:31
Operator : SY/MD
Sample : 05912-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc