

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033483.D
 Acq On : 19 Dec 2023 17:17
 Operator : SY/MD
 Sample : 05912-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	160938	171775	15.93%	2.159%
2	1.532	146	153	166	rVB	138922	166440	15.44%	2.092%
3	2.063	308	318	331	rBV	267300	396115	36.74%	4.979%
4	2.371	413	414	416	rBV2	1036	575	0.05%	0.007%
5	2.404	421	424	426	rBV3	1325	809	0.08%	0.010%
6	2.526	460	462	464	rBV3	1189	782	0.07%	0.010%
7	2.577	475	478	479	rBV2	1240	804	0.07%	0.010%
8	2.786	540	543	545	rBV2	957	492	0.05%	0.006%
9	2.809	545	550	554	rVV6	1322	1304	0.12%	0.016%
10	2.918	581	584	586	rBV3	896	634	0.06%	0.008%
11	2.973	599	601	606	rVB4	2388	1242	0.12%	0.016%
12	2.998	606	609	610	rBV2	1228	564	0.05%	0.007%
13	3.043	620	623	627	rBV6	751	731	0.07%	0.009%
14	3.063	627	629	632	rBV4	849	581	0.05%	0.007%
15	3.098	638	640	643	rBV4	1168	620	0.06%	0.008%
16	3.127	647	649	651	rBV3	1172	504	0.05%	0.006%
17	3.143	651	654	656	rBV4	1144	684	0.06%	0.009%
18	3.368	718	724	726	rBV5	1199	1248	0.12%	0.016%
19	3.404	733	735	737	rBV3	1107	627	0.06%	0.008%
20	3.638	805	808	809	rBV4	921	471	0.04%	0.006%
21	3.725	834	835	839	rVB4	936	404	0.04%	0.005%
22	3.783	839	853	878	rBV	50279	149670	13.88%	1.881%
23	4.249	985	998	1025	rVB	170940	439081	40.73%	5.520%
24	4.542	1087	1089	1092	rBV4	1180	739	0.07%	0.009%
25	4.635	1116	1118	1120	rBV3	970	461	0.04%	0.006%
26	4.783	1162	1164	1167	rBV4	1011	587	0.05%	0.007%
27	4.847	1182	1184	1188	rVB6	1124	507	0.05%	0.006%
28	4.879	1191	1194	1195	rBV2	1083	513	0.05%	0.006%
29	4.957	1202	1218	1258	rBV2	401271	1078055	100.00%	13.552%
30	5.535	1386	1398	1427	rBV	312874	658357	61.07%	8.276%
31	5.989	1527	1539	1567	rBV	235525	494303	45.85%	6.214%
32	6.304	1634	1637	1638	rBV3	1565	837	0.08%	0.011%
33	6.407	1665	1669	1671	rBV4	895	712	0.07%	0.009%
34	6.436	1676	1678	1682	rVB3	1146	486	0.05%	0.006%
35	6.654	1744	1746	1749	rVB3	822	387	0.04%	0.005%
36	6.699	1757	1760	1761	rBV3	1163	523	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033483.D
 Acq On : 19 Dec 2023 17:17
 Operator : SY/MD
 Sample : 05912-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.719	1764	1766	1768	rBV3	873	489	0.05%	0.006%
38	6.821	1796	1798	1801	rVB3	1149	601	0.06%	0.008%
39	6.847	1801	1806	1808	rBV4	1321	1173	0.11%	0.015%
40	6.912	1817	1826	1847	rBV	108483	209703	19.45%	2.636%
41	7.243	1918	1929	1950	rBV	440798	786676	72.97%	9.889%
42	7.555	2015	2026	2051	rBV	82499	158162	14.67%	1.988%
43	7.828	2109	2111	2118	rVB7	1596	1458	0.14%	0.018%
44	8.024	2164	2172	2206	rBV	169539	367014	34.04%	4.614%
45	8.500	2317	2320	2323	rBV4	1469	906	0.08%	0.011%
46	8.654	2366	2368	2373	rVB5	1797	1031	0.10%	0.013%
47	8.786	2396	2409	2435	rBV	514865	876092	81.27%	11.013%
48	9.339	2580	2581	2583	rBV2	923	483	0.04%	0.006%
49	9.352	2583	2585	2588	rVB3	1411	907	0.08%	0.011%
50	9.403	2599	2601	2603	rVB2	997	462	0.04%	0.006%
51	9.416	2603	2605	2606	rBV2	1534	601	0.06%	0.008%
52	9.590	2656	2659	2662	rBV6	1011	831	0.08%	0.010%
53	9.635	2671	2673	2678	rBV5	1139	732	0.07%	0.009%
54	9.763	2709	2713	2715	rBV3	1191	763	0.07%	0.010%
55	9.873	2744	2747	2749	rBV4	956	644	0.06%	0.008%
56	9.924	2760	2763	2768	rBV6	1672	1571	0.15%	0.020%
57	9.989	2778	2783	2784	rBV4	1428	1060	0.10%	0.013%
58	10.034	2795	2797	2799	rBV3	842	436	0.04%	0.005%
59	10.153	2823	2834	2853	rBV	301226	470992	43.69%	5.921%
60	10.368	2898	2901	2902	rBV3	795	412	0.04%	0.005%
61	10.715	3008	3009	3013	rVV4	1028	608	0.06%	0.008%
62	10.751	3016	3020	3021	rBV4	1522	878	0.08%	0.011%
63	10.760	3021	3023	3026	rVB4	2006	842	0.08%	0.011%
64	10.789	3029	3032	3034	rBV3	1255	634	0.06%	0.008%
65	10.831	3041	3045	3048	rBV5	1298	1283	0.12%	0.016%
66	10.979	3087	3091	3092	rBV3	949	537	0.05%	0.007%
67	11.185	3144	3155	3177	rBV	473851	740185	68.66%	9.305%
68	11.561	3255	3272	3293	rBV	459976	731916	67.89%	9.201%
69	11.808	3347	3349	3352	rBV2	1103	726	0.07%	0.009%
70	12.005	3408	3410	3411	rBV2	928	425	0.04%	0.005%
71	12.246	3482	3485	3488	rBV4	1267	987	0.09%	0.012%
72	12.432	3540	3543	3545	rBV3	1091	718	0.07%	0.009%
73	12.480	3555	3558	3563	rBV5	1407	1235	0.11%	0.016%
74	12.599	3593	3595	3597	rBV3	887	396	0.04%	0.005%
75	12.651	3609	3611	3615	rVB4	1468	783	0.07%	0.010%
76	12.744	3638	3640	3644	rVB5	1583	817	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033483.D
 Acq On : 19 Dec 2023 17:17
 Operator : SY/MD
 Sample : 05912-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.818	3660	3663	3665	rBV	1234	781	0.07%	0.010%
78	12.853	3670	3674	3675	rBV3	670	439	0.04%	0.006%
79	12.902	3687	3689	3692	rBV3	801	388	0.04%	0.005%
80	12.921	3692	3695	3697	rVV4	1166	527	0.05%	0.007%
81	13.062	3734	3739	3743	rBV8	1420	1498	0.14%	0.019%
82	13.101	3748	3751	3753	rBV5	1098	683	0.06%	0.009%
83	13.172	3770	3773	3775	rBV4	1122	583	0.05%	0.007%
84	13.259	3798	3800	3805	rVB6	1217	644	0.06%	0.008%
85	13.287	3807	3809	3812	rBV4	879	477	0.04%	0.006%
86	13.384	3836	3839	3841	rBV4	1268	825	0.08%	0.010%
87	13.413	3845	3848	3851	rBV3	1106	563	0.05%	0.007%
88	13.484	3867	3870	3873	rBV3	777	601	0.06%	0.008%
89	13.686	3931	3933	3934	rBV2	994	405	0.04%	0.005%
90	13.750	3951	3953	3954	rBV2	1343	584	0.05%	0.007%
91	13.844	3980	3982	3987	rBV6	1331	1035	0.10%	0.013%
92	13.953	4014	4016	4019	rBV3	1015	603	0.06%	0.008%
93	13.969	4019	4021	4024	rBV4	660	462	0.04%	0.006%
94	14.056	4046	4048	4051	rVB4	979	515	0.05%	0.006%
95	14.082	4051	4056	4058	rBV6	1465	1284	0.12%	0.016%
96	14.120	4066	4068	4071	rVB4	1281	576	0.05%	0.007%
97	14.445	4166	4169	4170	rBV3	961	506	0.05%	0.006%
98	14.805	4277	4281	4282	rBV3	1446	929	0.09%	0.012%
99	14.844	4291	4293	4296	rBV3	924	550	0.05%	0.007%
100	15.024	4347	4349	4354	rVB6	1056	773	0.07%	0.010%


Sum of corrected areas: 7955024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033483.D
Acq On : 19 Dec 2023 17:17
Operator : SY/MD
Sample : 05912-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

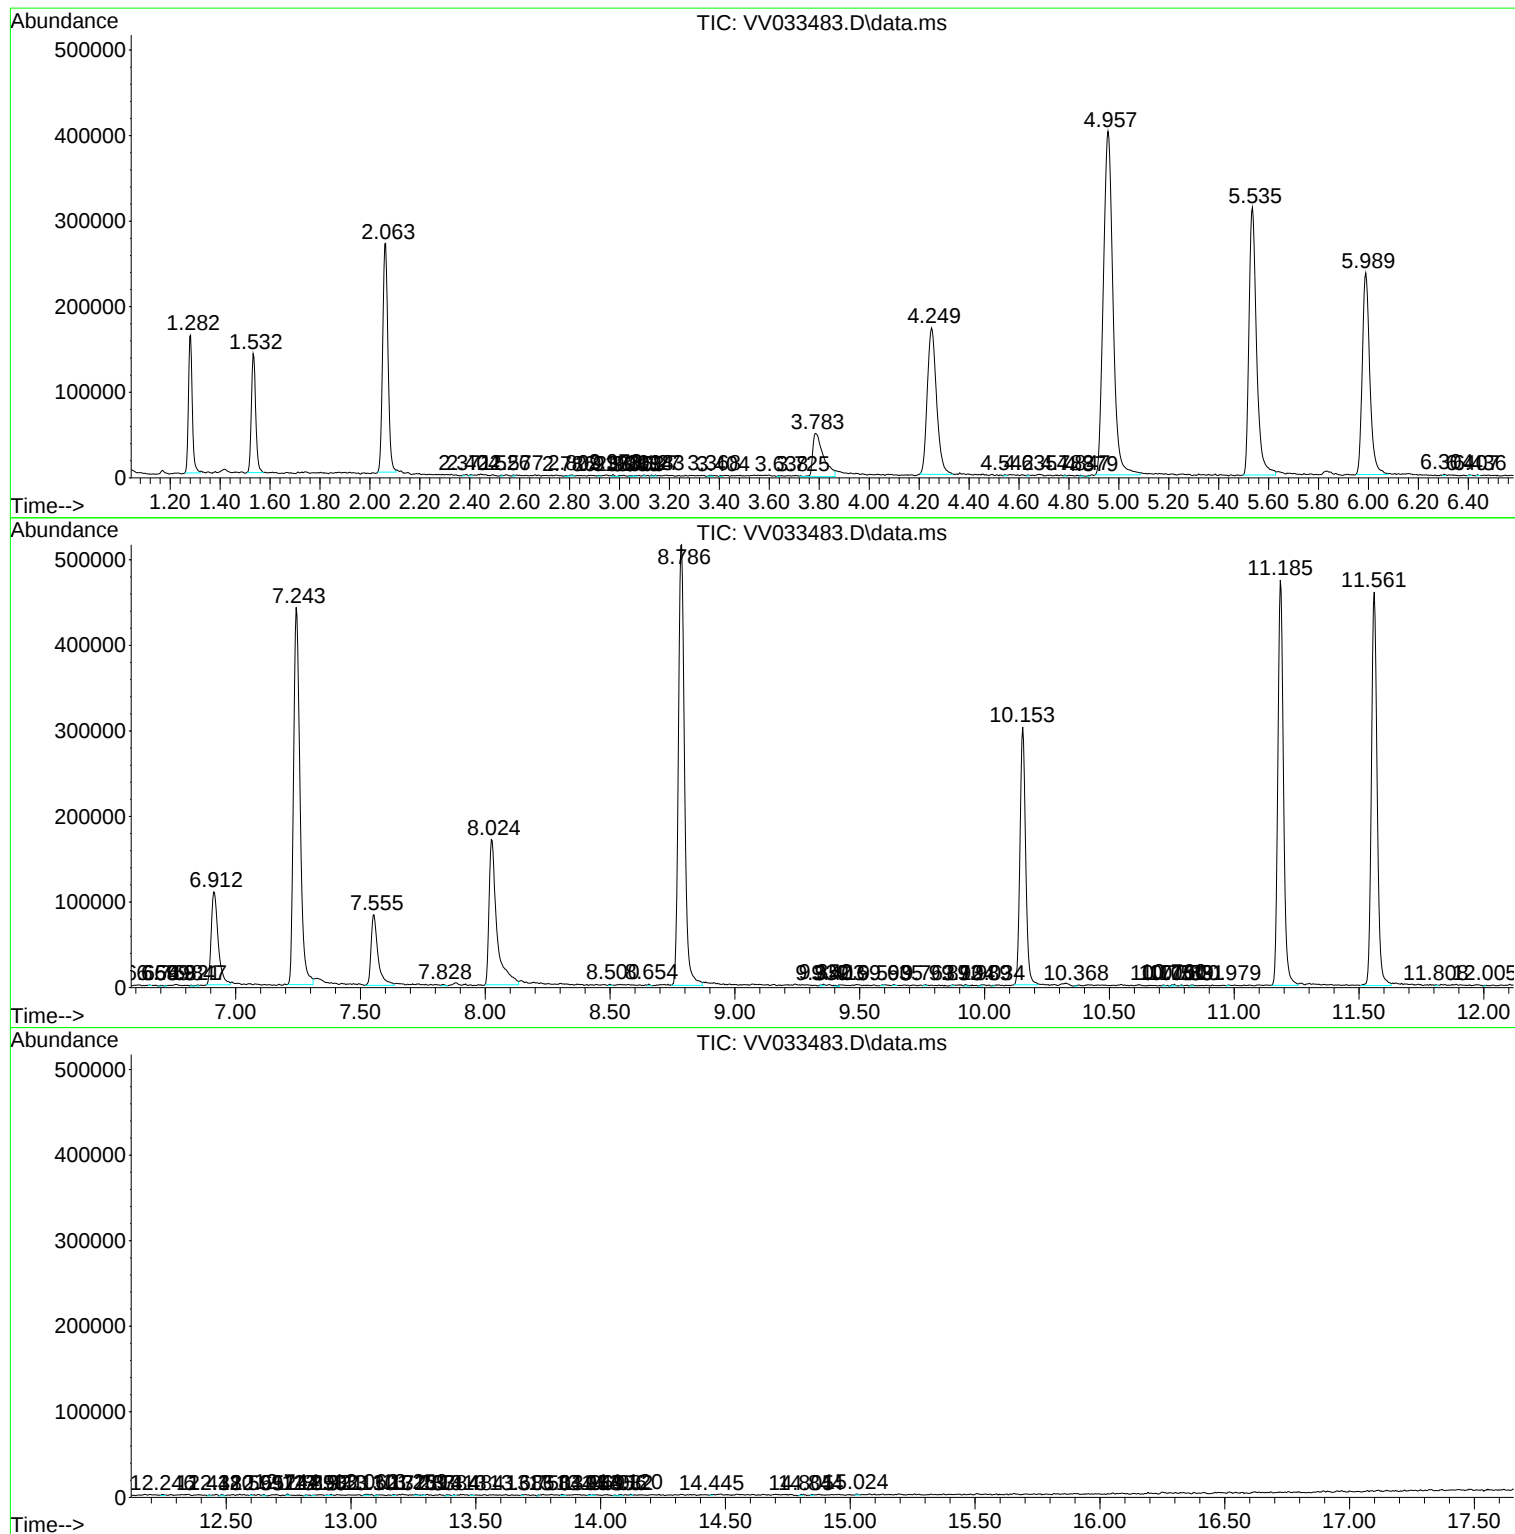

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033483.D
Acq On : 19 Dec 2023 17:17
Operator : SY/MD
Sample : 05912-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033483.D
Acq On : 19 Dec 2023 17:17
Operator : SY/MD
Sample : 05912-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc