

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033484.D
 Acq On : 19 Dec 2023 17:41
 Operator : SY/MD
 Sample : 05912-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	84	rBV	160808	169765	16.01%	2.114%
2	1.532	146	153	165	rBV	142654	166023	15.66%	2.067%
3	2.059	308	317	338	rVB	270517	403231	38.02%	5.021%
4	2.555	466	471	473	rBV7	1623	1197	0.11%	0.015%
5	2.596	482	484	487	rVB3	1319	789	0.07%	0.010%
6	2.613	487	489	492	rBV4	963	716	0.07%	0.009%
7	2.690	511	513	518	rBV6	921	636	0.06%	0.008%
8	2.850	559	563	566	rBV5	1272	1048	0.10%	0.013%
9	3.027	614	618	619	rBV2	748	538	0.05%	0.007%
10	3.043	622	623	626	rBV4	1040	590	0.06%	0.007%
11	3.082	633	635	638	rBV4	1740	963	0.09%	0.012%
12	3.101	638	641	642	rBV2	836	474	0.04%	0.006%
13	3.294	697	701	702	rBV3	1081	796	0.08%	0.010%
14	3.330	710	712	715	rVB2	1035	532	0.05%	0.007%
15	3.349	715	718	722	rVB6	1211	883	0.08%	0.011%
16	3.368	722	724	725	rBV2	925	382	0.04%	0.005%
17	3.449	747	749	750	rBV2	1246	567	0.05%	0.007%
18	3.532	773	775	778	rBV3	732	486	0.05%	0.006%
19	3.584	789	791	794	rVB3	979	477	0.04%	0.006%
20	3.613	798	800	802	rBV4	1530	765	0.07%	0.010%
21	3.741	834	840	841	rBV6	1157	1243	0.12%	0.015%
22	3.786	846	854	876	rBV2	52719	140512	13.25%	1.750%
23	4.249	985	998	1023	rVB	171326	435407	41.06%	5.422%
24	4.821	1175	1176	1178	rBV2	1056	419	0.04%	0.005%
25	4.957	1203	1218	1246	rBV2	396517	1060453	100.00%	13.205%
26	5.535	1387	1398	1421	rBV	321620	675932	63.74%	8.417%
27	5.937	1519	1523	1525	rBV6	1393	1291	0.12%	0.016%
28	5.989	1528	1539	1564	rVV	240046	497173	46.88%	6.191%
29	6.358	1652	1654	1656	rBV3	1197	640	0.06%	0.008%
30	6.468	1685	1688	1689	rBV3	926	401	0.04%	0.005%
31	6.590	1723	1726	1728	rBV3	1477	635	0.06%	0.008%
32	6.715	1763	1765	1767	rBV3	973	410	0.04%	0.005%
33	6.744	1771	1774	1777	rBV5	934	714	0.07%	0.009%
34	6.789	1785	1788	1792	rBV4	1168	858	0.08%	0.011%
35	6.915	1816	1827	1844	rBV	111507	212382	20.03%	2.645%
36	7.243	1918	1929	1950	rBV	441557	791590	74.65%	9.857%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033484.D
 Acq On : 19 Dec 2023 17:41
 Operator : SY/MD
 Sample : 05912-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.554	2017	2026	2045	rBV	81581	146270	13.79%	1.821%
38	7.953	2148	2150	2153	rBV4	836	477	0.04%	0.006%
39	8.024	2163	2172	2198	rBV	173159	369242	34.82%	4.598%
40	8.455	2302	2306	2307	rBV3	1193	806	0.08%	0.010%
41	8.783	2397	2408	2437	rBV	540735	911714	85.97%	11.353%
42	9.275	2557	2561	2563	rBV5	1415	1249	0.12%	0.016%
43	9.477	2621	2624	2626	rBV4	1116	710	0.07%	0.009%
44	9.654	2674	2679	2680	rBV3	1087	841	0.08%	0.010%
45	9.680	2685	2687	2690	rVB3	1232	574	0.05%	0.007%
46	9.744	2705	2707	2709	rBV3	895	423	0.04%	0.005%
47	9.915	2758	2760	2766	rVB6	1195	972	0.09%	0.012%
48	9.956	2769	2773	2774	rBV3	1091	687	0.06%	0.009%
49	10.008	2786	2789	2791	rBV4	1077	568	0.05%	0.007%
50	10.046	2798	2801	2805	rBV6	1088	1017	0.10%	0.013%
51	10.104	2813	2819	2820	rBV5	1433	1283	0.12%	0.016%
52	10.152	2820	2834	2859	rVV	304081	487165	45.94%	6.066%
53	10.423	2916	2918	2921	rBV4	976	652	0.06%	0.008%
54	10.464	2928	2931	2934	rBV5	865	530	0.05%	0.007%
55	10.484	2934	2937	2938	rBV3	1211	564	0.05%	0.007%
56	10.522	2946	2949	2950	rBV	913	452	0.04%	0.006%
57	10.541	2953	2955	2961	rVB4	1234	1099	0.10%	0.014%
58	10.580	2965	2967	2969	rBV2	1046	550	0.05%	0.007%
59	10.664	2989	2993	2995	rBV4	1574	1218	0.11%	0.015%
60	10.722	3007	3011	3015	rBV5	1510	1111	0.10%	0.014%
61	10.876	3055	3059	3061	rBV4	899	767	0.07%	0.010%
62	11.004	3096	3099	3103	rBV4	1395	1430	0.13%	0.018%
63	11.040	3108	3110	3112	rBV3	991	614	0.06%	0.008%
64	11.053	3112	3114	3117	rVB4	1144	561	0.05%	0.007%
65	11.066	3117	3118	3122	rVB3	735	452	0.04%	0.006%
66	11.098	3125	3128	3130	rBV4	1179	657	0.06%	0.008%
67	11.127	3135	3137	3144	rVB7	1429	1041	0.10%	0.013%
68	11.185	3144	3155	3175	rBV	491824	774973	73.08%	9.650%
69	11.439	3230	3234	3241	rVB7	1397	1420	0.13%	0.018%
70	11.467	3241	3243	3244	rBV2	963	403	0.04%	0.005%
71	11.503	3252	3254	3255	rBV	1044	435	0.04%	0.005%
72	11.561	3261	3272	3290	rBV	456345	723886	68.26%	9.014%
73	11.998	3405	3408	3411	rBV4	1225	996	0.09%	0.012%
74	12.037	3418	3420	3421	rBV2	880	403	0.04%	0.005%
75	12.181	3462	3465	3466	rBV3	1478	632	0.06%	0.008%
76	12.226	3477	3479	3482	rVB4	1363	662	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033484.D
 Acq On : 19 Dec 2023 17:41
 Operator : SY/MD
 Sample : 05912-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.384	3527	3528	3532	rBV3	1098	782	0.07%	0.010%
78	12.516	3567	3569	3572	rBV3	897	485	0.05%	0.006%
79	12.580	3584	3589	3592	rBV6	1247	1283	0.12%	0.016%
80	12.667	3614	3616	3618	rBV3	1205	535	0.05%	0.007%
81	12.802	3654	3658	3661	rBV6	1219	1045	0.10%	0.013%
82	12.937	3698	3700	3701	rBV	1183	546	0.05%	0.007%
83	13.217	3784	3787	3794	rBV8	1624	1683	0.16%	0.021%
84	13.274	3802	3805	3808	rBV4	1711	1192	0.11%	0.015%
85	13.310	3812	3816	3817	rBV4	818	500	0.05%	0.006%
86	13.358	3829	3831	3833	rBV2	936	538	0.05%	0.007%
87	13.490	3871	3872	3873	rBV	1102	360	0.03%	0.004%
88	13.554	3886	3892	3894	rBV7	2012	1792	0.17%	0.022%
89	13.709	3939	3940	3941	rBV	1111	391	0.04%	0.005%
90	13.779	3959	3962	3965	rBV5	1182	909	0.09%	0.011%
91	13.940	4010	4012	4015	rBV5	952	623	0.06%	0.008%
92	13.985	4024	4026	4028	rBV2	1297	799	0.08%	0.010%
93	14.078	4051	4055	4058	rBV4	1720	1083	0.10%	0.013%
94	14.255	4108	4110	4112	rVB3	1121	362	0.03%	0.005%
95	14.332	4131	4134	4138	rBV6	1018	1054	0.10%	0.013%
96	14.384	4148	4150	4152	rBV3	1128	539	0.05%	0.007%
97	14.410	4156	4158	4159	rBV2	1128	499	0.05%	0.006%
98	14.670	4236	4239	4241	rBV4	1421	714	0.07%	0.009%
99	14.744	4260	4262	4266	rBV5	1595	1463	0.14%	0.018%
100	15.091	4367	4370	4373	rBV4	1353	978	0.09%	0.012%




Sum of corrected areas: 8030579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033484.D
Acq On : 19 Dec 2023 17:41
Operator : SY/MD
Sample : 05912-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

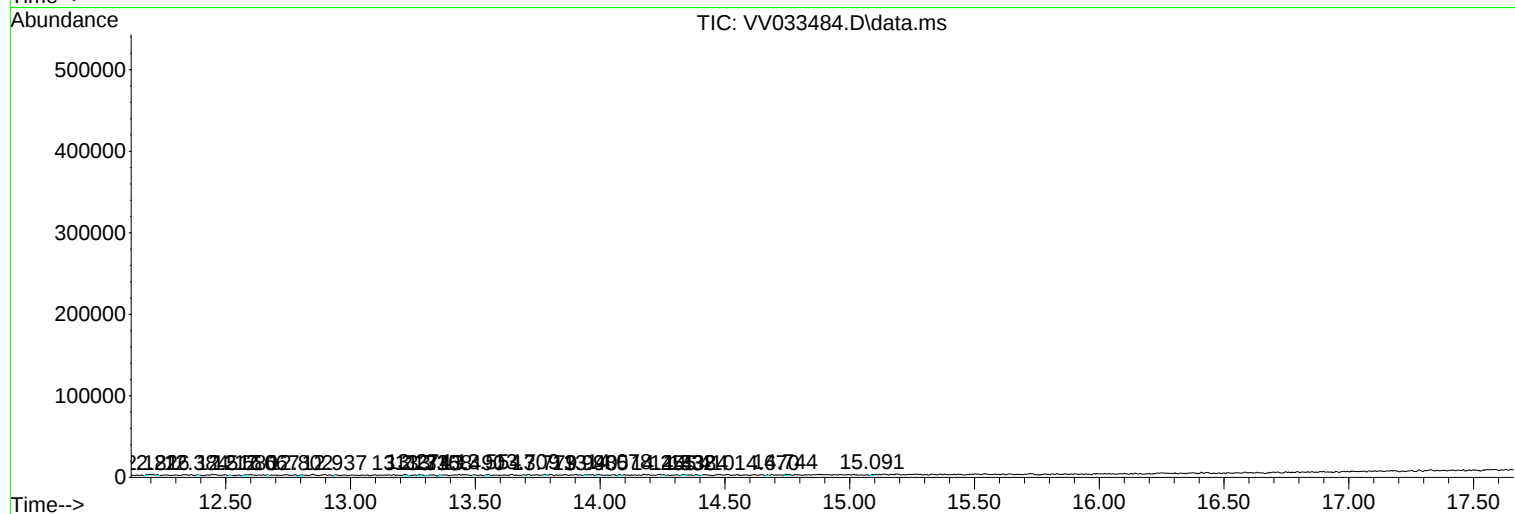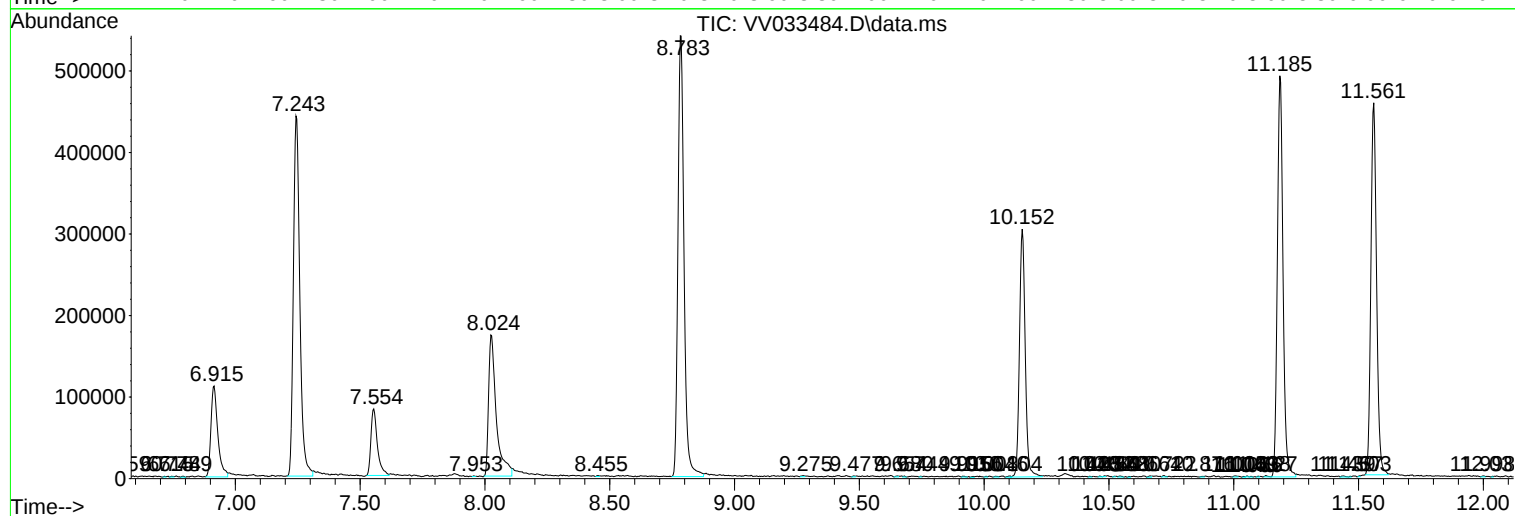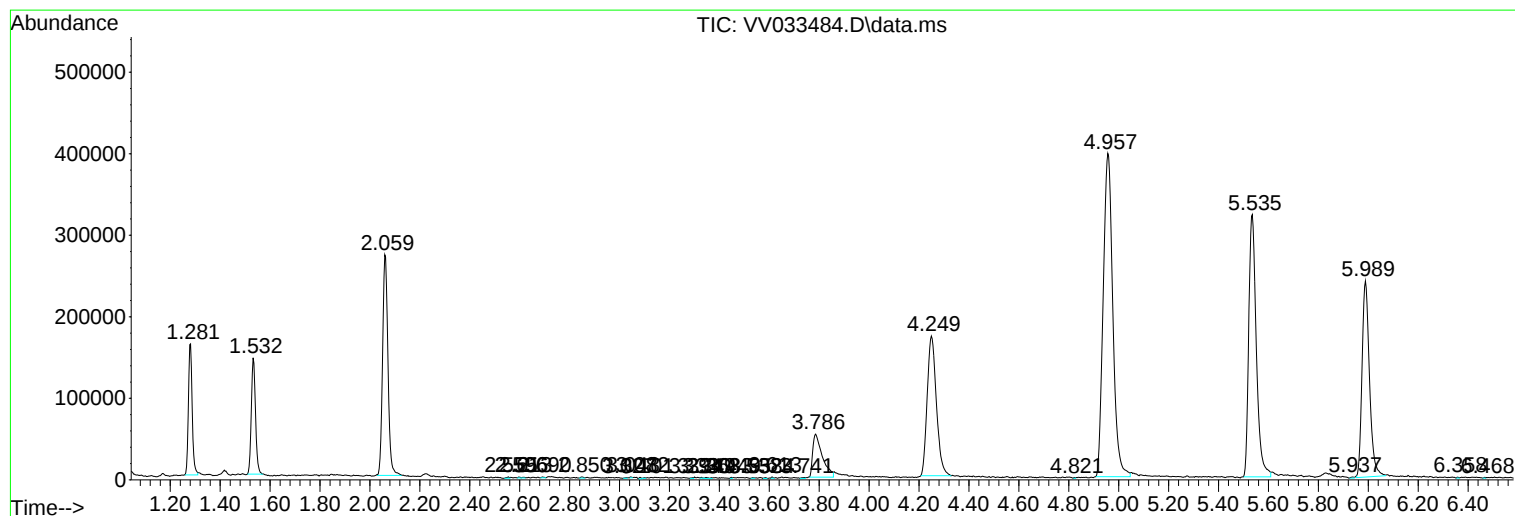

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033484.D
Acq On : 19 Dec 2023 17:41
Operator : SY/MD
Sample : 05912-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033484.D
Acq On : 19 Dec 2023 17:41
Operator : SY/MD
Sample : 05912-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------