

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033485.D
 Acq On : 19 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05912-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rVB	166507	174848	16.39%	2.201%
2	1.532	146	153	169	rVB	140271	166254	15.58%	2.093%
3	2.063	308	318	334	rBV	266062	393630	36.89%	4.955%
4	2.587	479	481	484	rBV3	861	596	0.06%	0.008%
5	2.670	503	507	508	rBV4	868	609	0.06%	0.008%
6	2.738	522	528	530	rBV4	1572	1343	0.13%	0.017%
7	2.815	549	552	554	rBV2	991	819	0.08%	0.010%
8	2.883	570	573	575	rBV4	1841	992	0.09%	0.012%
9	2.960	595	597	600	rBV2	1341	868	0.08%	0.011%
10	3.217	673	677	679	rBV4	973	700	0.07%	0.009%
11	3.262	688	691	694	rBV5	1102	766	0.07%	0.010%
12	3.281	694	697	698	rVV2	1133	623	0.06%	0.008%
13	3.426	736	742	743	rBV6	1068	864	0.08%	0.011%
14	3.529	771	774	776	rBV3	884	726	0.07%	0.009%
15	3.645	805	810	813	rBV5	1299	1081	0.10%	0.014%
16	3.786	844	854	882	rBV	49460	146813	13.76%	1.848%
17	4.249	983	998	1031	rBV2	168844	438546	41.10%	5.520%
18	4.538	1087	1088	1092	rBV4	899	568	0.05%	0.007%
19	4.725	1143	1146	1149	rVB3	1084	819	0.08%	0.010%
20	4.747	1149	1153	1156	rBV5	1293	1124	0.11%	0.014%
21	4.956	1202	1218	1248	rBV2	395277	1066991	100.00%	13.431%
22	5.342	1336	1338	1340	rBV3	1667	844	0.08%	0.011%
23	5.535	1386	1398	1423	rBV	317940	672989	63.07%	8.471%
24	5.989	1527	1539	1564	rBV2	233257	489403	45.87%	6.160%
25	6.349	1647	1651	1653	rBV6	1122	910	0.09%	0.011%
26	6.571	1717	1720	1722	rVB3	1053	620	0.06%	0.008%
27	6.583	1722	1724	1726	rBV3	1577	875	0.08%	0.011%
28	6.609	1729	1732	1734	rVV4	1209	575	0.05%	0.007%
29	6.645	1741	1743	1746	rVB3	1069	646	0.06%	0.008%
30	6.802	1790	1792	1798	rVB5	1404	1066	0.10%	0.013%
31	6.837	1798	1803	1806	rVB5	1104	1063	0.10%	0.013%
32	6.857	1806	1809	1811	rBV4	1341	898	0.08%	0.011%
33	6.915	1817	1827	1853	rBV	109656	214121	20.07%	2.695%
34	7.201	1912	1916	1918	rBV5	857	722	0.07%	0.009%
35	7.243	1918	1929	1948	rBV	435460	777075	72.83%	9.781%
36	7.554	2016	2026	2044	rBV	80456	145093	13.60%	1.826%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033485.D
 Acq On : 19 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05912-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.837	2112	2114	2116	rBV3	1326	932	0.09%	0.012%
38	8.027	2163	2173	2202	rBV	168049	368174	34.51%	4.634%
39	8.497	2317	2319	2322	rVB4	1455	878	0.08%	0.011%
40	8.577	2340	2344	2346	rBV4	1316	1001	0.09%	0.013%
41	8.628	2357	2360	2361	rBV2	1147	676	0.06%	0.009%
42	8.783	2397	2408	2427	rBV	526819	875449	82.05%	11.020%
43	9.287	2561	2565	2568	rVV3	1326	1172	0.11%	0.015%
44	9.320	2572	2575	2580	rVV6	1379	1242	0.12%	0.016%
45	9.345	2581	2583	2587	rVB5	988	586	0.05%	0.007%
46	9.403	2598	2601	2602	rBV2	1074	631	0.06%	0.008%
47	9.435	2607	2611	2615	rBV5	973	1063	0.10%	0.013%
48	9.564	2648	2651	2654	rBV4	1655	780	0.07%	0.010%
49	9.593	2658	2660	2663	rVB2	1236	574	0.05%	0.007%
50	9.718	2694	2699	2701	rBV5	999	875	0.08%	0.011%
51	9.844	2735	2738	2741	rVB4	1133	640	0.06%	0.008%
52	9.902	2753	2756	2757	rBV3	1212	794	0.07%	0.010%
53	9.953	2769	2772	2775	rBV3	1466	1210	0.11%	0.015%
54	9.982	2778	2781	2783	rVV3	818	571	0.05%	0.007%
55	10.005	2785	2788	2792	rVB5	1141	713	0.07%	0.009%
56	10.152	2823	2834	2854	rBV	300328	474955	44.51%	5.978%
57	10.377	2902	2904	2907	rBV4	1098	666	0.06%	0.008%
58	10.750	3017	3020	3023	rBV3	1357	985	0.09%	0.012%
59	10.789	3029	3032	3034	rBV3	1209	937	0.09%	0.012%
60	10.934	3070	3077	3079	rVB8	1409	1478	0.14%	0.019%
61	10.947	3079	3081	3083	rBV3	927	567	0.05%	0.007%
62	11.127	3135	3137	3140	rBV3	1320	898	0.08%	0.011%
63	11.185	3145	3155	3180	rVV	483256	754332	70.70%	9.495%
64	11.374	3212	3214	3218	rVB3	1091	563	0.05%	0.007%
65	11.406	3221	3224	3228	rVB5	1018	675	0.06%	0.008%
66	11.448	3234	3237	3242	rBV7	1245	1257	0.12%	0.016%
67	11.561	3261	3272	3291	rBV	456805	713778	66.90%	8.985%
68	11.918	3382	3383	3386	rBV3	1084	680	0.06%	0.009%
69	11.956	3393	3395	3397	rBV3	857	561	0.05%	0.007%
70	12.094	3436	3438	3443	rVB4	1274	1053	0.10%	0.013%
71	12.127	3443	3448	3449	rBV5	923	740	0.07%	0.009%
72	12.435	3542	3544	3547	rBV3	868	557	0.05%	0.007%
73	12.464	3551	3553	3556	rVB3	1489	765	0.07%	0.010%
74	12.487	3556	3560	3563	rBV5	802	769	0.07%	0.010%
75	12.612	3595	3599	3602	rBV5	1508	1071	0.10%	0.013%
76	12.628	3602	3604	3607	rVV4	1183	752	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033485.D
 Acq On : 19 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05912-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.738	3636	3638	3640	rBV3	1180	621	0.06%	0.008%
78	12.815	3657	3662	3666	rBV6	1519	1339	0.13%	0.017%
79	12.856	3672	3675	3677	rBV3	1139	563	0.05%	0.007%
80	13.030	3725	3729	3733	rBV6	1188	1188	0.11%	0.015%
81	13.242	3793	3795	3799	rVB4	1002	614	0.06%	0.008%
82	13.358	3829	3831	3834	rBV3	1734	1045	0.10%	0.013%
83	13.393	3839	3842	3850	rBV6	1077	1042	0.10%	0.013%
84	13.432	3850	3854	3856	rBV4	768	628	0.06%	0.008%
85	13.458	3859	3862	3863	rBV3	1146	684	0.06%	0.009%
86	13.525	3879	3883	3884	rBV3	1101	834	0.08%	0.010%
87	13.586	3901	3902	3906	rBV4	1022	690	0.06%	0.009%
88	13.673	3925	3929	3931	rBV4	1226	893	0.08%	0.011%
89	13.725	3942	3945	3949	rBV5	1064	780	0.07%	0.010%
90	13.930	4006	4009	4012	rBV5	1262	837	0.08%	0.011%
91	14.262	4109	4112	4113	rBV3	1017	572	0.05%	0.007%
92	14.352	4138	4140	4141	rBV2	1497	637	0.06%	0.008%
93	14.387	4147	4151	4153	rVB4	1484	1024	0.10%	0.013%
94	14.406	4155	4157	4161	rBV4	837	628	0.06%	0.008%
95	14.548	4199	4201	4205	rBV5	901	686	0.06%	0.009%
96	14.734	4253	4259	4263	rBV7	2022	2201	0.21%	0.028%
97	14.754	4263	4265	4268	rBV3	954	668	0.06%	0.008%
98	14.905	4309	4312	4316	rBV5	1349	1150	0.11%	0.014%
99	14.943	4322	4324	4329	rBV5	1615	1280	0.12%	0.016%
100	15.641	4538	4541	4544	rBV5	1384	1400	0.13%	0.018%




Sum of corrected areas: 7944484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033485.D
Acq On : 19 Dec 2023 18:04
Operator : SY/MD
Sample : 05912-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

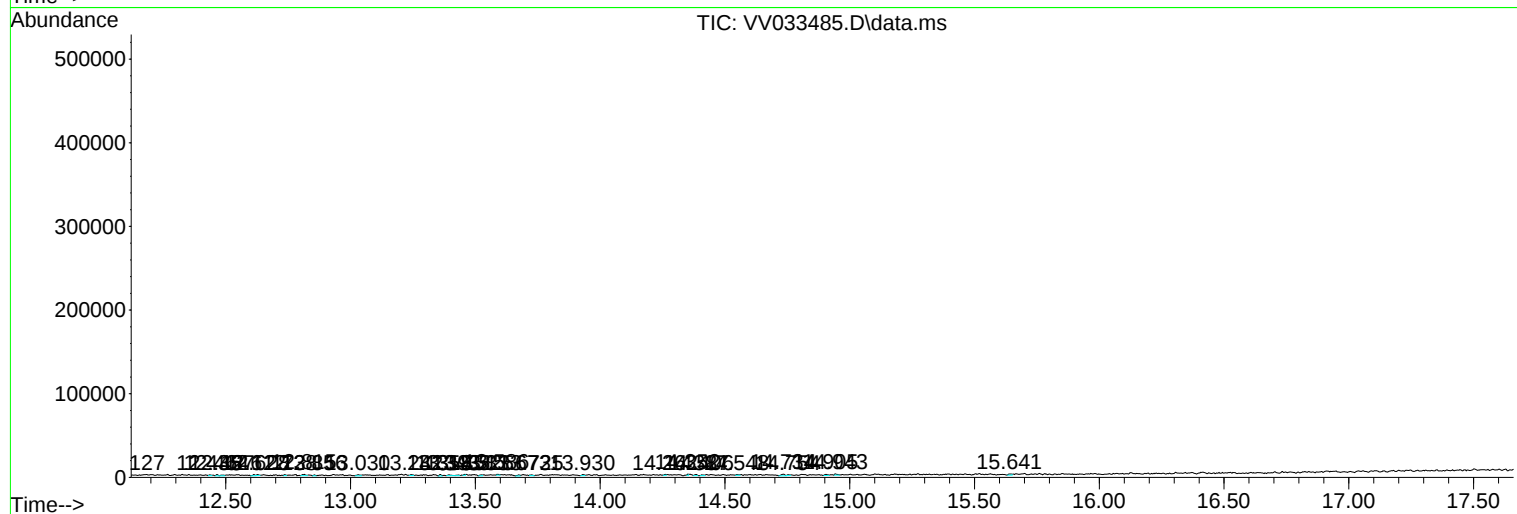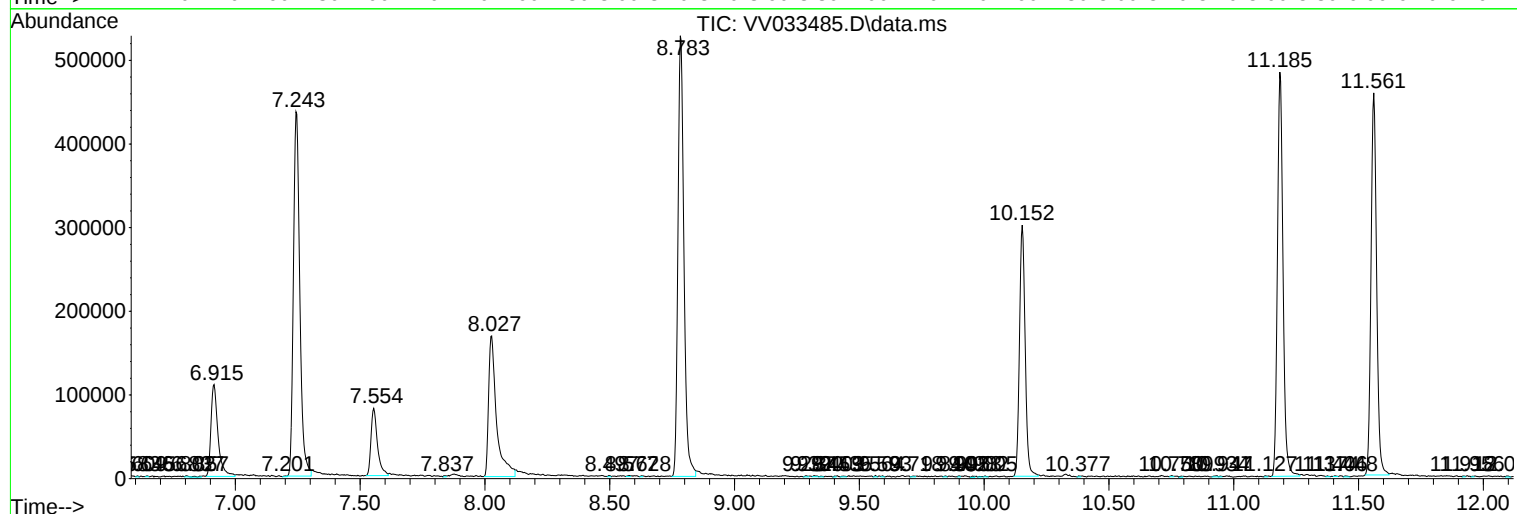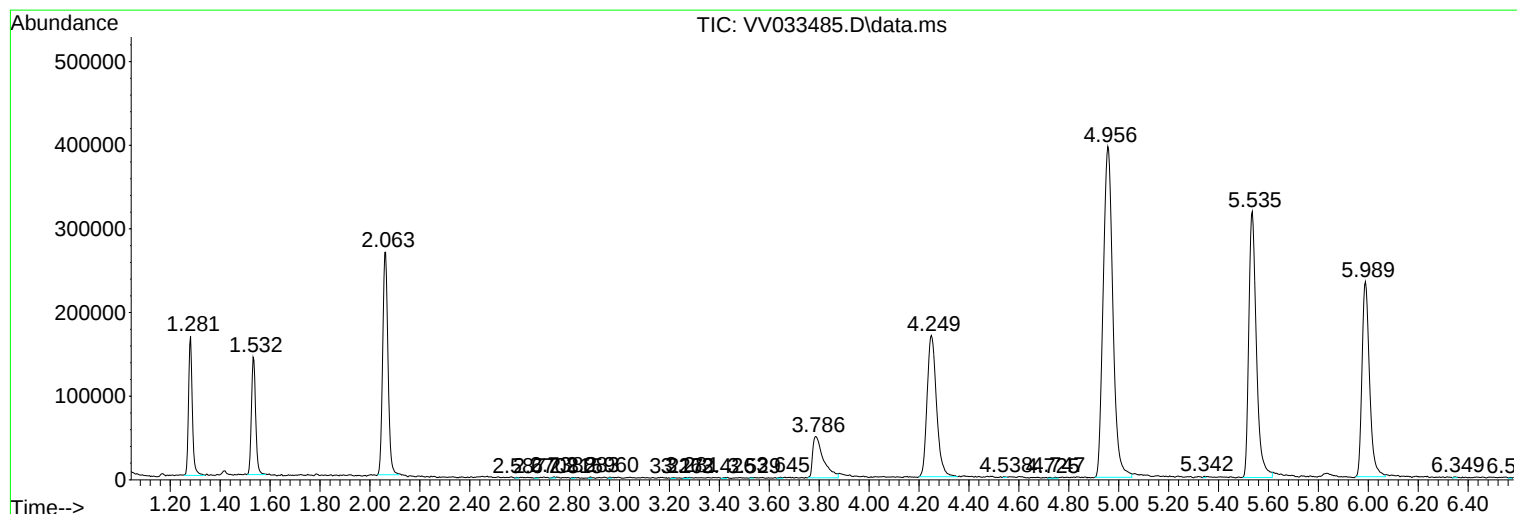

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033485.D
Acq On : 19 Dec 2023 18:04
Operator : SY/MD
Sample : 05912-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033485.D
Acq On : 19 Dec 2023 18:04
Operator : SY/MD
Sample : 05912-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------