

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033486.D
 Acq On : 19 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05912-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV	167780	171900	15.86%	2.136%
2	1.532	146	153	166	rBV	142241	168170	15.52%	2.090%
3	2.063	308	318	337	rBV	272391	399530	36.87%	4.965%
4	2.301	390	392	395	rBV3	961	645	0.06%	0.008%
5	2.381	413	417	420	rBV6	1378	1287	0.12%	0.016%
6	2.500	451	454	456	rBV4	1175	749	0.07%	0.009%
7	2.725	521	524	531	rBV7	1251	1095	0.10%	0.014%
8	2.780	538	541	543	rBV4	1383	735	0.07%	0.009%
9	2.921	582	585	589	rBV6	911	734	0.07%	0.009%
10	3.076	632	633	637	rVB2	1060	744	0.07%	0.009%
11	3.169	657	662	663	rBV4	879	620	0.06%	0.008%
12	3.233	675	682	683	rBV6	865	828	0.08%	0.010%
13	3.262	687	691	695	rVB4	1029	881	0.08%	0.011%
14	3.294	697	701	705	rBV6	1021	997	0.09%	0.012%
15	3.439	743	746	749	rBV5	1369	1166	0.11%	0.014%
16	3.548	774	780	784	rVB7	1070	998	0.09%	0.012%
17	3.574	784	788	792	rBV6	1352	1101	0.10%	0.014%
18	3.593	792	794	798	rBV4	956	622	0.06%	0.008%
19	3.616	798	801	804	rVB5	1275	655	0.06%	0.008%
20	3.645	807	810	812	rVB3	1151	628	0.06%	0.008%
21	3.786	846	854	879	rBV	53186	144513	13.34%	1.796%
22	4.140	960	964	969	rVB8	1728	1586	0.15%	0.020%
23	4.249	985	998	1023	rVB2	171413	435886	40.23%	5.417%
24	4.609	1105	1110	1112	rBV5	807	762	0.07%	0.009%
25	4.638	1117	1119	1126	rBV7	1437	1429	0.13%	0.018%
26	4.761	1155	1157	1161	rBV4	915	804	0.07%	0.010%
27	4.957	1202	1218	1251	rVV2	404628	1083596	100.00%	13.465%
28	5.474	1376	1379	1381	rBV3	888	717	0.07%	0.009%
29	5.535	1386	1398	1422	rBV	324293	676926	62.47%	8.412%
30	5.989	1528	1539	1560	rBV	238752	489238	45.15%	6.080%
31	6.317	1639	1641	1647	rBV5	1481	1420	0.13%	0.018%
32	6.375	1656	1659	1664	rBV6	1474	1400	0.13%	0.017%
33	6.452	1678	1683	1684	rBV5	835	801	0.07%	0.010%
34	6.506	1698	1700	1705	rBV6	1401	993	0.09%	0.012%
35	6.603	1728	1730	1735	rBV5	1159	862	0.08%	0.011%
36	6.822	1795	1798	1799	rBV3	1167	785	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033486.D
 Acq On : 19 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05912-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.912	1816	1826	1844	rBV	109519	211295	19.50%	2.626%
38	7.243	1918	1929	1953	rBV	441977	792380	73.13%	9.847%
39	7.555	2017	2026	2038	rBV	79282	142468	13.15%	1.770%
40	7.805	2101	2104	2108	rBV5	1426	888	0.08%	0.011%
41	7.873	2119	2125	2127	rBV6	2227	2392	0.22%	0.030%
42	8.024	2164	2172	2206	rVV	173866	379778	35.05%	4.719%
43	8.420	2293	2295	2301	rBV6	1347	1076	0.10%	0.013%
44	8.561	2338	2339	2350	rVB9	1165	1488	0.14%	0.018%
45	8.667	2369	2372	2374	rBV4	1300	897	0.08%	0.011%
46	8.709	2381	2385	2387	rBV5	1151	738	0.07%	0.009%
47	8.783	2397	2408	2428	rBV	534951	893997	82.50%	11.109%
48	9.117	2509	2512	2513	rBV2	1112	718	0.07%	0.009%
49	9.191	2531	2535	2537	rBV5	1242	1107	0.10%	0.014%
50	9.320	2571	2575	2581	rBV8	1298	1224	0.11%	0.015%
51	9.413	2601	2604	2605	rBV3	1154	634	0.06%	0.008%
52	9.693	2689	2691	2696	rVB6	1050	648	0.06%	0.008%
53	9.744	2704	2707	2711	rBV6	600	581	0.05%	0.007%
54	9.764	2711	2713	2721	rVB7	1089	1246	0.11%	0.015%
55	9.809	2724	2727	2730	rBV5	1174	646	0.06%	0.008%
56	9.863	2741	2744	2747	rBV3	921	705	0.07%	0.009%
57	9.895	2752	2754	2765	rVB10	1220	1367	0.13%	0.017%
58	9.963	2772	2775	2778	rVB5	1064	685	0.06%	0.009%
59	10.024	2792	2794	2799	rVB6	1409	1032	0.10%	0.013%
60	10.072	2805	2809	2811	rBV4	1222	1163	0.11%	0.014%
61	10.153	2820	2834	2850	rBV	299973	480366	44.33%	5.969%
62	10.323	2882	2887	2888	rBV5	2794	2043	0.19%	0.025%
63	10.529	2947	2951	2952	rBV5	1280	867	0.08%	0.011%
64	10.567	2957	2963	2969	rBV8	1115	1139	0.11%	0.014%
65	10.632	2981	2983	2986	rVB4	1817	877	0.08%	0.011%
66	10.651	2986	2989	2992	rBV5	1132	828	0.08%	0.010%
67	10.747	3014	3019	3020	rBV4	1245	909	0.08%	0.011%
68	10.789	3027	3032	3034	rBV4	1450	1489	0.14%	0.019%
69	10.870	3054	3057	3059	rBV4	1267	713	0.07%	0.009%
70	10.902	3064	3067	3073	rVV7	946	923	0.09%	0.011%
71	11.059	3112	3116	3119	rBV5	1235	1332	0.12%	0.017%
72	11.114	3129	3133	3135	rBV5	1283	761	0.07%	0.009%
73	11.185	3145	3155	3180	rBV	489084	761143	70.24%	9.458%
74	11.561	3261	3272	3299	rVB	461679	734371	67.77%	9.126%
75	11.741	3325	3328	3333	rVB7	1712	1193	0.11%	0.015%
76	11.789	3341	3343	3347	rBV5	1410	788	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033486.D
 Acq On : 19 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05912-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	11.828	3353	3355	3357	rVB3	1901	804	0.07%	0.010%
78	11.850	3357	3362	3367	rBV6	1790	2071	0.19%	0.026%
79	12.262	3487	3490	3491	rBV3	1204	730	0.07%	0.009%
80	12.300	3499	3502	3503	rBV3	1231	650	0.06%	0.008%
81	12.464	3549	3553	3556	rBV4	908	764	0.07%	0.009%
82	12.526	3570	3572	3576	rBV4	1022	850	0.08%	0.011%
83	12.696	3623	3625	3628	rVB2	1201	589	0.05%	0.007%
84	13.120	3754	3757	3761	rBV7	1099	1039	0.10%	0.013%
85	13.181	3773	3776	3778	rBV2	1377	786	0.07%	0.010%
86	13.278	3802	3806	3808	rBV4	1203	812	0.07%	0.010%
87	13.355	3826	3830	3832	rVV4	1369	1046	0.10%	0.013%
88	13.500	3872	3875	3878	rVB4	1066	704	0.06%	0.009%
89	13.519	3878	3881	3888	rBV7	1565	1956	0.18%	0.024%
90	13.889	3994	3996	3999	rBV3	1121	597	0.06%	0.007%
91	13.989	4025	4027	4031	rVB3	1166	897	0.08%	0.011%
92	14.043	4042	4044	4050	rBV6	1303	1518	0.14%	0.019%
93	14.207	4093	4095	4099	rVB5	1569	906	0.08%	0.011%
94	14.230	4099	4102	4105	rVB4	1241	607	0.06%	0.008%
95	14.538	4196	4198	4201	rVB3	1408	633	0.06%	0.008%
96	14.754	4263	4265	4267	rBV3	1149	618	0.06%	0.008%
97	15.259	4420	4422	4424	rBV3	1266	654	0.06%	0.008%
98	15.506	4495	4499	4502	rBV5	1254	1178	0.11%	0.015%
99	15.548	4510	4512	4517	rBV6	1882	1258	0.12%	0.016%
100	15.918	4625	4627	4629	rBV3	1468	909	0.08%	0.011%




Sum of corrected areas: 8047274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033486.D
Acq On : 19 Dec 2023 18:27
Operator : SY/MD
Sample : 05912-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

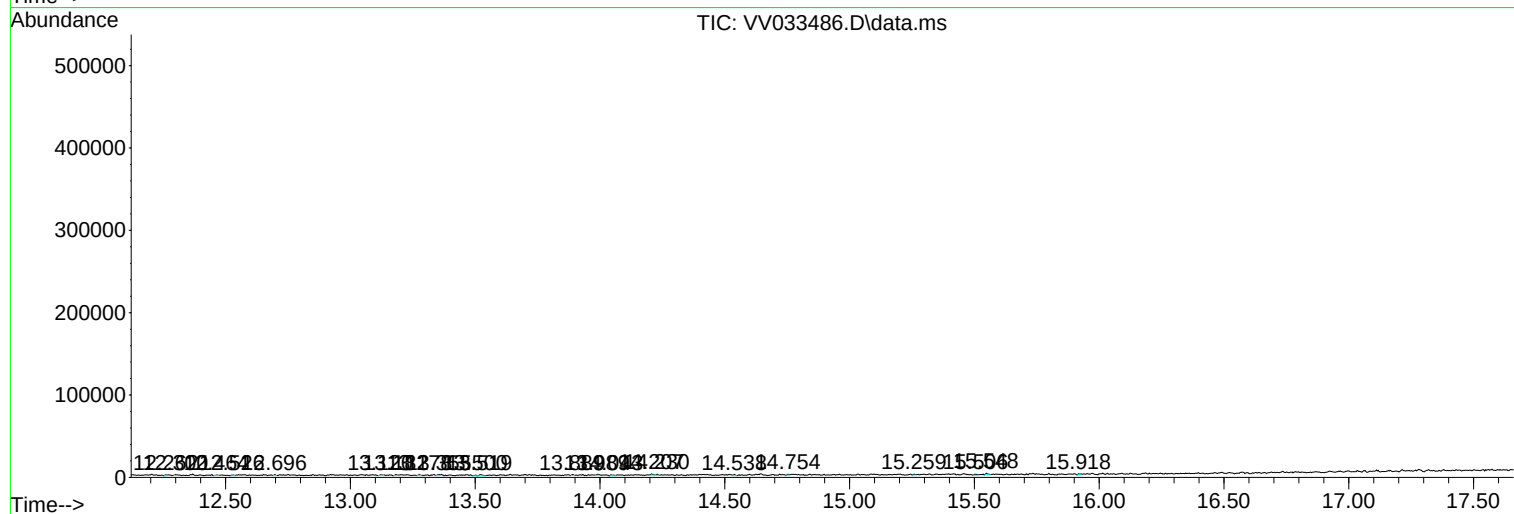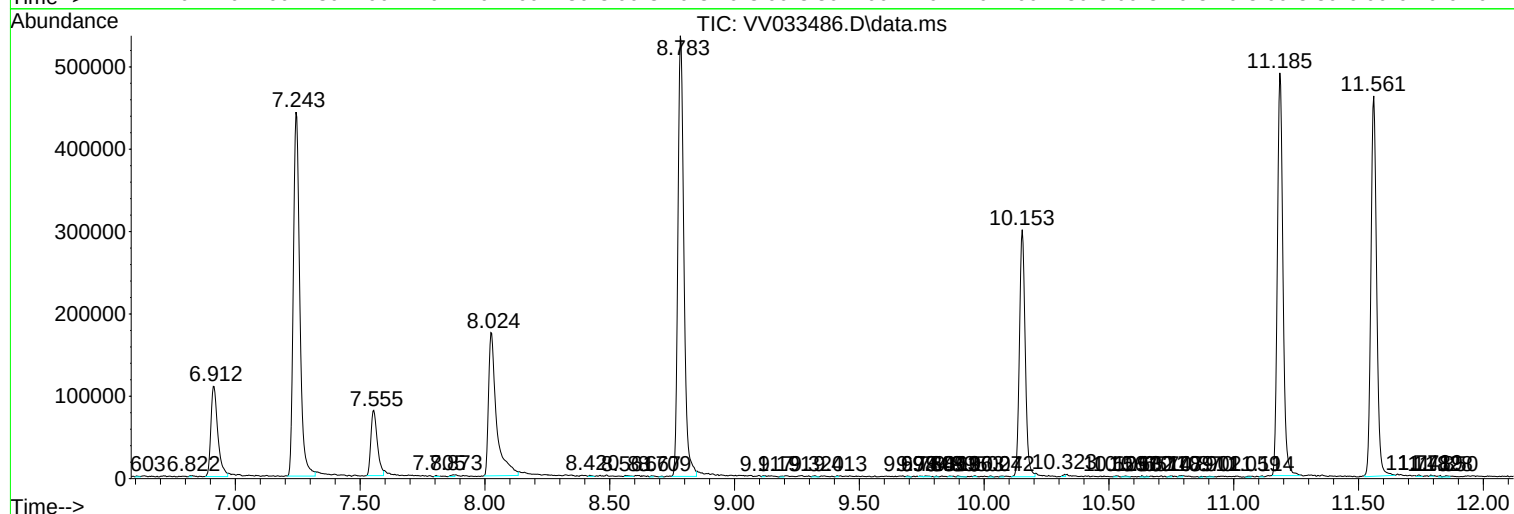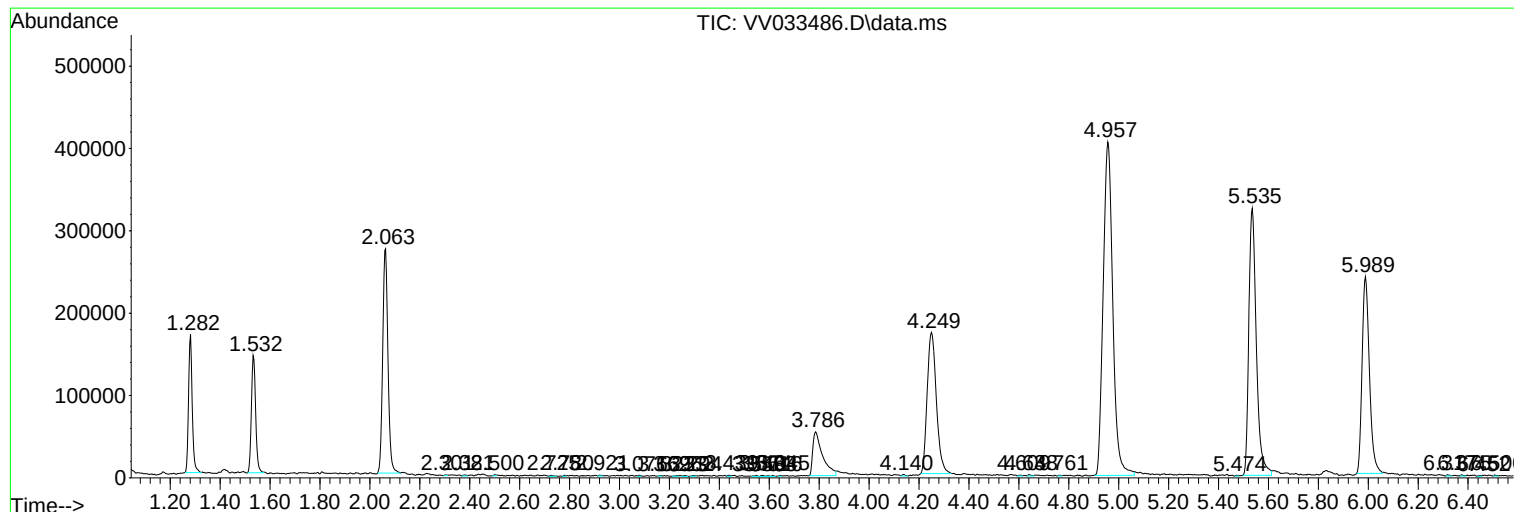

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033486.D
Acq On : 19 Dec 2023 18:27
Operator : SY/MD
Sample : 05912-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033486.D
Acq On : 19 Dec 2023 18:27
Operator : SY/MD
Sample : 05912-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------