

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033487.D
 Acq On : 19 Dec 2023 18:50
 Operator : SY/MD
 Sample : 05912-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3D6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rBV	161205	167171	16.06%	2.149%
2	1.532	147	153	170	rVB	136845	165200	15.87%	2.124%
3	2.060	308	317	329	rBV	262303	381786	36.68%	4.908%
4	2.600	482	485	487	rBV3	1698	1085	0.10%	0.014%
5	2.638	493	497	500	rBV6	1303	824	0.08%	0.011%
6	2.764	532	536	537	rBV4	898	576	0.06%	0.007%
7	2.799	545	547	550	rVB4	1078	525	0.05%	0.007%
8	2.841	558	560	562	rBV3	1319	775	0.07%	0.010%
9	2.883	571	573	576	rVB4	1018	536	0.05%	0.007%
10	2.896	576	577	579	rBV2	664	249	0.02%	0.003%
11	3.053	624	626	628	rBV3	1082	758	0.07%	0.010%
12	3.130	648	650	651	rBV2	661	242	0.02%	0.003%
13	3.140	651	653	657	rVB5	1094	811	0.08%	0.010%
14	3.201	669	672	675	rVB4	930	610	0.06%	0.008%
15	3.265	689	692	695	rVB4	1072	672	0.06%	0.009%
16	3.285	695	698	699	rBV3	965	357	0.03%	0.005%
17	3.307	703	705	708	rBV4	871	476	0.05%	0.006%
18	3.349	715	718	721	rBV5	852	461	0.04%	0.006%
19	3.375	724	726	728	rBV3	718	305	0.03%	0.004%
20	3.410	734	737	738	rBV3	1021	461	0.04%	0.006%
21	3.455	750	751	757	rVB5	861	538	0.05%	0.007%
22	3.551	778	781	787	rVV6	906	944	0.09%	0.012%
23	3.609	795	799	800	rBV3	1515	871	0.08%	0.011%
24	3.632	804	806	809	rVV2	1169	604	0.06%	0.008%
25	3.645	809	810	813	rVV2	677	285	0.03%	0.004%
26	3.738	837	839	841	rBV3	747	415	0.04%	0.005%
27	3.786	845	854	883	rBV	49366	144268	13.86%	1.855%
28	4.178	974	976	980	rBV5	833	625	0.06%	0.008%
29	4.249	984	998	1024	rVV	167396	435299	41.82%	5.596%
30	4.542	1087	1089	1094	rVB5	1416	921	0.09%	0.012%
31	4.638	1114	1119	1120	rBV4	1195	996	0.10%	0.013%
32	4.661	1124	1126	1128	rBV3	1244	482	0.05%	0.006%
33	4.715	1141	1143	1145	rBV3	1124	401	0.04%	0.005%
34	4.879	1192	1194	1195	rBV2	1017	307	0.03%	0.004%
35	4.957	1202	1218	1248	rBV2	386091	1040992	100.00%	13.383%
36	5.535	1386	1398	1425	rBV	310822	656061	63.02%	8.434%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033487.D
 Acq On : 19 Dec 2023 18:50
 Operator : SY/MD
 Sample : 05912-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3D6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	5.989	1527	1539	1566	rBV	233316	483673	46.46%	6.218%
38	6.625	1735	1737	1740	rBV3	1034	600	0.06%	0.008%
39	6.661	1745	1748	1749	rBV2	949	401	0.04%	0.005%
40	6.744	1771	1774	1778	rBV4	995	874	0.08%	0.011%
41	6.863	1808	1811	1815	rBV6	1099	867	0.08%	0.011%
42	6.915	1817	1827	1844	rBV	107283	203646	19.56%	2.618%
43	7.243	1918	1929	1951	rBV	425228	768517	73.83%	9.880%
44	7.555	2017	2026	2048	rBV	77000	141710	13.61%	1.822%
45	7.776	2091	2095	2096	rBV3	966	718	0.07%	0.009%
46	7.982	2157	2159	2160	rBV	1261	510	0.05%	0.007%
47	8.027	2164	2173	2204	rBV	164504	372813	35.81%	4.793%
48	8.497	2316	2319	2320	rBV3	1725	918	0.09%	0.012%
49	8.622	2356	2358	2361	rBV3	726	447	0.04%	0.006%
50	8.638	2361	2363	2366	rBV4	976	721	0.07%	0.009%
51	8.728	2389	2391	2395	rBV4	1455	880	0.08%	0.011%
52	8.783	2398	2408	2433	rVV	514115	864233	83.02%	11.110%
53	9.349	2579	2584	2590	rBV7	1481	1912	0.18%	0.025%
54	9.535	2640	2642	2646	rVB3	935	580	0.06%	0.007%
55	9.558	2646	2649	2651	rBV4	814	542	0.05%	0.007%
56	9.612	2664	2666	2667	rBV2	713	278	0.03%	0.004%
57	9.882	2748	2750	2754	rBV4	983	896	0.09%	0.012%
58	9.992	2781	2784	2787	rBV4	1509	1361	0.13%	0.017%
59	10.104	2815	2819	2821	rBV4	1411	1016	0.10%	0.013%
60	10.153	2823	2834	2852	rVV	286975	457162	43.92%	5.877%
61	10.413	2911	2915	2918	rBV6	1488	1137	0.11%	0.015%
62	10.429	2918	2920	2922	rVV3	915	439	0.04%	0.006%
63	10.538	2952	2954	2957	rVB4	1004	587	0.06%	0.008%
64	10.577	2964	2966	2968	rBV3	784	461	0.04%	0.006%
65	11.185	3145	3155	3178	rBV	478144	738799	70.97%	9.498%
66	11.487	3247	3249	3251	rBV3	1112	635	0.06%	0.008%
67	11.561	3262	3272	3296	rVB	439531	701978	67.43%	9.024%
68	12.230	3478	3480	3483	rBV5	804	555	0.05%	0.007%
69	12.297	3495	3501	3502	rBV5	1517	1432	0.14%	0.018%
70	12.413	3534	3537	3540	rBV3	947	677	0.07%	0.009%
71	12.429	3540	3542	3545	rBV3	1279	725	0.07%	0.009%
72	12.548	3575	3579	3581	rBV4	1095	793	0.08%	0.010%
73	12.612	3591	3599	3600	rBV7	1233	1665	0.16%	0.021%
74	12.660	3612	3614	3617	rVB3	892	331	0.03%	0.004%
75	12.677	3617	3619	3621	rBV3	936	476	0.05%	0.006%
76	12.705	3626	3628	3630	rBV3	608	243	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033487.D
 Acq On : 19 Dec 2023 18:50
 Operator : SY/MD
 Sample : 05912-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3D6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.728	3633	3635	3637	rBV3	747	402	0.04%	0.005%
78	12.921	3693	3695	3696	rBV2	693	238	0.02%	0.003%
79	12.953	3704	3705	3710	rVB4	925	460	0.04%	0.006%
80	12.982	3711	3714	3715	rBV3	825	382	0.04%	0.005%
81	13.082	3743	3745	3747	rBV2	677	227	0.02%	0.003%
82	13.136	3760	3762	3766	rVB3	1389	657	0.06%	0.008%
83	13.291	3807	3810	3811	rBV3	1038	471	0.05%	0.006%
84	13.329	3819	3822	3825	rBV4	1673	1111	0.11%	0.014%
85	13.361	3830	3832	3835	rVV3	721	459	0.04%	0.006%
86	13.377	3835	3837	3840	rVB3	909	403	0.04%	0.005%
87	13.445	3854	3858	3860	rBV4	1051	779	0.07%	0.010%
88	13.496	3872	3874	3877	rBV4	1076	483	0.05%	0.006%
89	13.532	3883	3885	3886	rBV	689	259	0.02%	0.003%
90	13.599	3904	3906	3909	rBV4	869	434	0.04%	0.006%
91	13.641	3916	3919	3920	rBV3	582	343	0.03%	0.004%
92	13.651	3920	3922	3926	rVV4	1064	638	0.06%	0.008%
93	13.718	3939	3943	3944	rBV4	1034	712	0.07%	0.009%
94	13.792	3964	3966	3968	rBV3	712	339	0.03%	0.004%
95	13.927	4006	4008	4013	rVB6	1639	979	0.09%	0.013%
96	14.053	4045	4047	4050	rBV3	750	498	0.05%	0.006%
97	14.188	4085	4089	4090	rBV4	1504	958	0.09%	0.012%
98	14.529	4192	4195	4200	rBV7	2128	2037	0.20%	0.026%
99	14.766	4267	4269	4270	rBV2	1032	294	0.03%	0.004%
100	15.557	4513	4515	4519	rBV4	1543	1023	0.10%	0.013%


Sum of corrected areas: 7778683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033487.D
Acq On : 19 Dec 2023 18:50
Operator : SY/MD
Sample : 05912-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3D6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

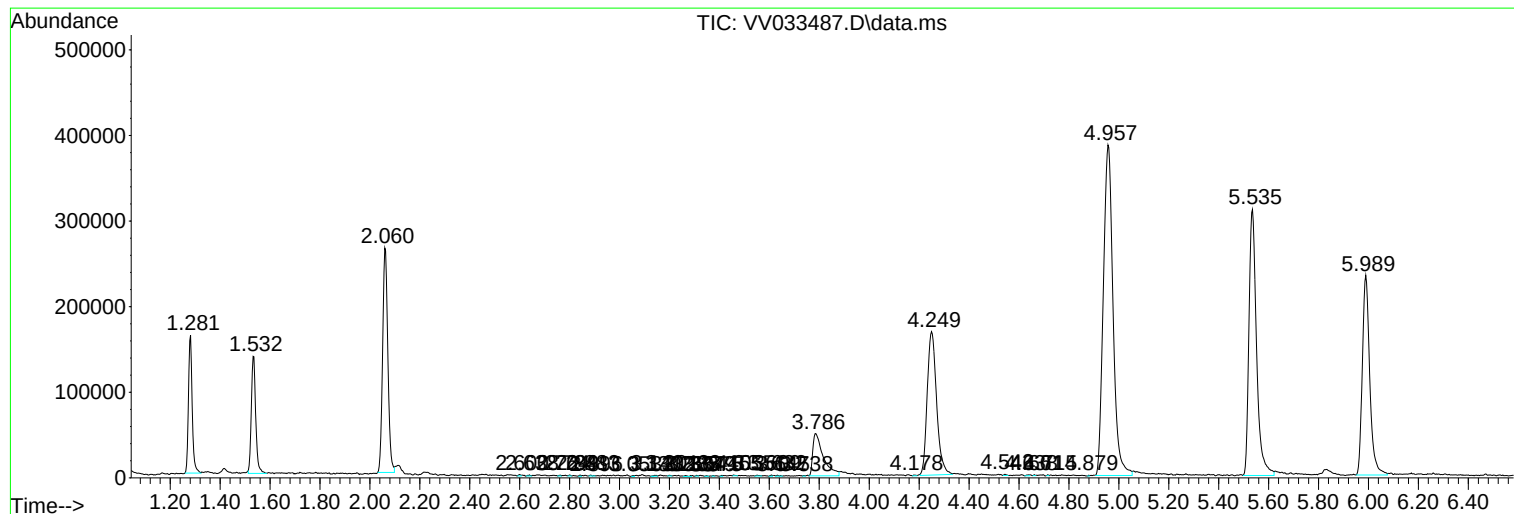

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033487.D
Acq On : 19 Dec 2023 18:50
Operator : SY/MD
Sample : 05912-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3D6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033487.D
Acq On : 19 Dec 2023 18:50
Operator : SY/MD
Sample : 05912-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3D6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------