

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033488.D
 Acq On : 19 Dec 2023 19:13
 Operator : SY/MD
 Sample : 05912-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	161401	167272	15.79%	2.119%
2	1.532	146	153	165	rVB	136582	162407	15.33%	2.057%
3	2.060	308	317	332	rVB	262321	382171	36.08%	4.841%
4	2.603	481	486	489	rBV5	846	976	0.09%	0.012%
5	2.700	514	516	520	rBV5	1089	530	0.05%	0.007%
6	2.767	535	537	540	rBV3	951	721	0.07%	0.009%
7	2.851	557	563	565	rBV3	816	628	0.06%	0.008%
8	3.082	631	635	637	rBV5	1463	853	0.08%	0.011%
9	3.114	643	645	649	rBV4	1468	852	0.08%	0.011%
10	3.285	696	698	702	rVB4	1522	768	0.07%	0.010%
11	3.307	702	705	708	rBV5	1125	806	0.08%	0.010%
12	3.339	713	715	718	rVB3	1247	730	0.07%	0.009%
13	3.368	723	724	726	rBV2	1208	482	0.05%	0.006%
14	3.426	738	742	744	rBV3	1002	870	0.08%	0.011%
15	3.462	749	753	757	rVV4	804	814	0.08%	0.010%
16	3.484	757	760	762	rVB3	1415	835	0.08%	0.011%
17	3.616	794	801	803	rBV7	1313	1168	0.11%	0.015%
18	3.645	808	810	814	rVB4	1020	686	0.06%	0.009%
19	3.683	819	822	824	rVB4	815	548	0.05%	0.007%
20	3.706	827	829	833	rVB4	1471	1000	0.09%	0.013%
21	3.732	833	837	838	rBV4	881	579	0.05%	0.007%
22	3.783	845	853	876	rBV	51575	144577	13.65%	1.831%
23	4.162	968	971	974	rBV5	1603	1220	0.12%	0.015%
24	4.249	983	998	1021	rBV	167746	430747	40.66%	5.456%
25	4.580	1098	1101	1107	rBV7	1523	1735	0.16%	0.022%
26	4.722	1141	1145	1148	rBV5	1153	1179	0.11%	0.015%
27	4.802	1168	1170	1172	rVV3	1277	575	0.05%	0.007%
28	4.957	1199	1218	1246	rBV2	391238	1059279	100.00%	13.418%
29	5.410	1357	1359	1361	rBV3	1144	579	0.05%	0.007%
30	5.535	1386	1398	1421	rBV	320826	673760	63.61%	8.535%
31	5.989	1527	1539	1567	rBV	236773	484164	45.71%	6.133%
32	6.346	1648	1650	1655	rVB6	1303	702	0.07%	0.009%
33	6.384	1660	1662	1667	rVB5	1065	725	0.07%	0.009%
34	6.432	1675	1677	1678	rBV	1532	735	0.07%	0.009%
35	6.632	1737	1739	1743	rBV5	980	755	0.07%	0.010%
36	6.709	1758	1763	1766	rBV6	1160	903	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033488.D
 Acq On : 19 Dec 2023 19:13
 Operator : SY/MD
 Sample : 05912-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.802	1788	1792	1794	rBV4	874	483	0.05%	0.006%
38	6.831	1798	1801	1803	rBV5	1334	731	0.07%	0.009%
39	6.912	1816	1826	1846	rBV	106708	203395	19.20%	2.576%
40	7.130	1892	1894	1895	rBV2	1296	514	0.05%	0.007%
41	7.243	1918	1929	1953	rBV	427585	770453	72.73%	9.759%
42	7.555	2017	2026	2050	rBV2	77621	148825	14.05%	1.885%
43	7.857	2118	2120	2122	rBV3	1742	858	0.08%	0.011%
44	8.024	2162	2172	2200	rBV	172346	369766	34.91%	4.684%
45	8.661	2368	2370	2372	rBV3	1248	478	0.05%	0.006%
46	8.677	2372	2375	2380	rVB6	1103	886	0.08%	0.011%
47	8.722	2385	2389	2391	rBV5	2011	1215	0.11%	0.015%
48	8.783	2397	2408	2429	rBV	534324	890731	84.09%	11.283%
49	9.346	2580	2583	2586	rBV5	918	824	0.08%	0.010%
50	9.461	2617	2619	2623	rBV5	1065	869	0.08%	0.011%
51	9.529	2637	2640	2643	rBV5	1068	646	0.06%	0.008%
52	9.577	2653	2655	2658	rVB3	1350	808	0.08%	0.010%
53	9.657	2675	2680	2683	rBV6	1113	1191	0.11%	0.015%
54	9.831	2733	2734	2738	rVB4	1129	514	0.05%	0.007%
55	10.024	2790	2794	2798	rVB7	1741	1451	0.14%	0.018%
56	10.153	2823	2834	2855	rBV	293908	466255	44.02%	5.906%
57	10.255	2865	2866	2873	rVB6	1517	1207	0.11%	0.015%
58	10.323	2883	2887	2895	rBV9	3094	3951	0.37%	0.050%
59	10.374	2901	2903	2906	rVB4	1438	623	0.06%	0.008%
60	10.403	2910	2912	2916	rVB5	965	580	0.05%	0.007%
61	10.535	2950	2953	2954	rBV3	1052	513	0.05%	0.006%
62	10.619	2976	2979	2980	rBV3	1249	530	0.05%	0.007%
63	10.735	3013	3015	3020	rBV5	705	650	0.06%	0.008%
64	10.841	3046	3048	3052	rVB4	877	466	0.04%	0.006%
65	11.098	3124	3128	3131	rBV4	1190	995	0.09%	0.013%
66	11.130	3136	3138	3140	rBV2	1196	623	0.06%	0.008%
67	11.185	3144	3155	3175	rBV	487411	764414	72.16%	9.683%
68	11.561	3261	3272	3293	rBV	450661	705834	66.63%	8.941%
69	11.911	3378	3381	3385	rBV3	1351	1031	0.10%	0.013%
70	11.927	3385	3386	3389	rVB3	1353	476	0.04%	0.006%
71	11.947	3389	3392	3393	rBV3	1433	847	0.08%	0.011%
72	11.985	3400	3404	3406	rVB3	1544	1113	0.11%	0.014%
73	12.005	3406	3410	3413	rBV5	1069	978	0.09%	0.012%
74	12.316	3502	3507	3512	rVB7	1860	1999	0.19%	0.025%
75	12.403	3531	3534	3535	rBV3	1247	613	0.06%	0.008%
76	12.458	3548	3551	3552	rBV3	1239	506	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033488.D
 Acq On : 19 Dec 2023 19:13
 Operator : SY/MD
 Sample : 05912-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.577	3586	3588	3591	rBV4	1385	676	0.06%	0.009%
78	12.709	3626	3629	3634	rVB5	944	836	0.08%	0.011%
79	12.738	3634	3638	3639	rBV4	998	674	0.06%	0.009%
80	12.773	3647	3649	3651	rBV3	1008	538	0.05%	0.007%
81	12.831	3664	3667	3669	rBV4	1735	919	0.09%	0.012%
82	13.059	3735	3738	3741	rBV4	1141	824	0.08%	0.010%
83	13.079	3742	3744	3747	rVV3	1117	596	0.06%	0.008%
84	13.111	3750	3754	3756	rVV5	705	530	0.05%	0.007%
85	13.387	3836	3840	3841	rBV2	1332	757	0.07%	0.010%
86	13.500	3873	3875	3880	rVB5	802	597	0.06%	0.008%
87	13.522	3880	3882	3885	rBV4	1625	888	0.08%	0.011%
88	13.622	3908	3913	3917	rBV6	1200	1292	0.12%	0.016%
89	13.664	3923	3926	3929	rBV3	1059	845	0.08%	0.011%
90	13.834	3976	3979	3984	rVB5	1507	1110	0.10%	0.014%
91	13.866	3987	3989	3992	rBV3	920	678	0.06%	0.009%
92	13.892	3992	3997	4001	rBV7	919	862	0.08%	0.011%
93	14.078	4053	4055	4057	rBV3	1032	699	0.07%	0.009%
94	14.114	4063	4066	4069	rBV3	922	528	0.05%	0.007%
95	14.484	4179	4181	4185	rBV5	1383	992	0.09%	0.013%
96	14.564	4203	4206	4208	rBV3	1095	802	0.08%	0.010%
97	14.757	4265	4266	4268	rBV2	953	485	0.05%	0.006%
98	14.995	4338	4340	4342	rBV3	1252	641	0.06%	0.008%
99	15.387	4459	4462	4463	rBV2	1408	769	0.07%	0.010%
100	15.603	4526	4529	4532	rBV4	1231	713	0.07%	0.009%




Sum of corrected areas: 7894424

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033488.D
Acq On : 19 Dec 2023 19:13
Operator : SY/MD
Sample : 05912-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

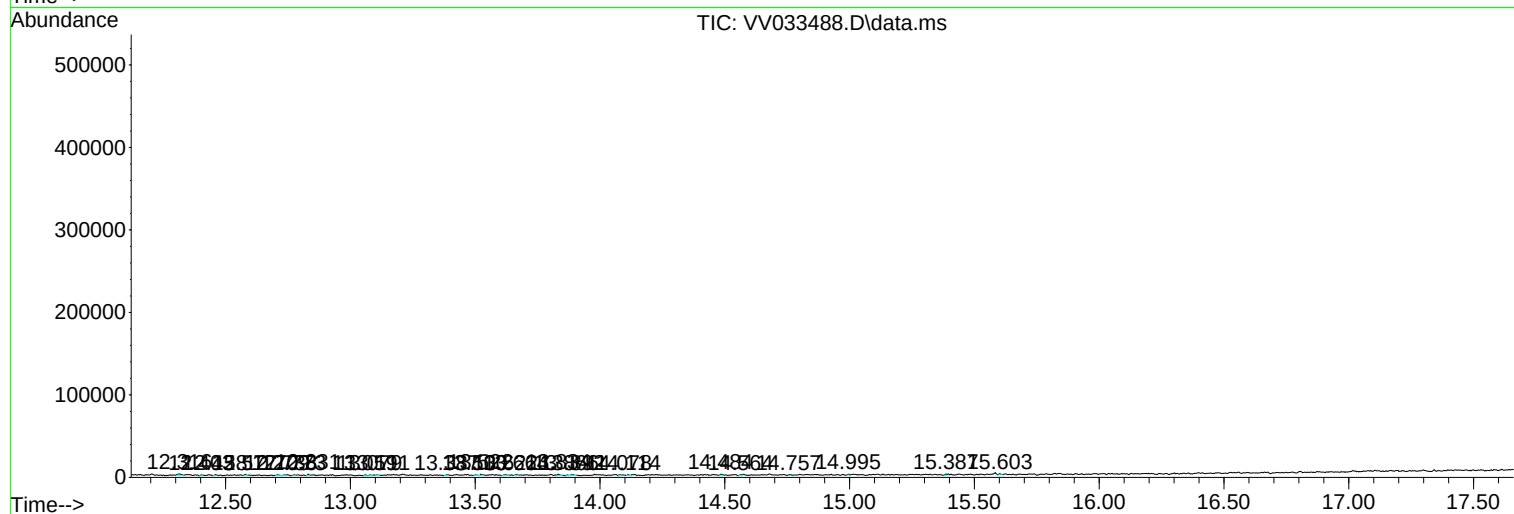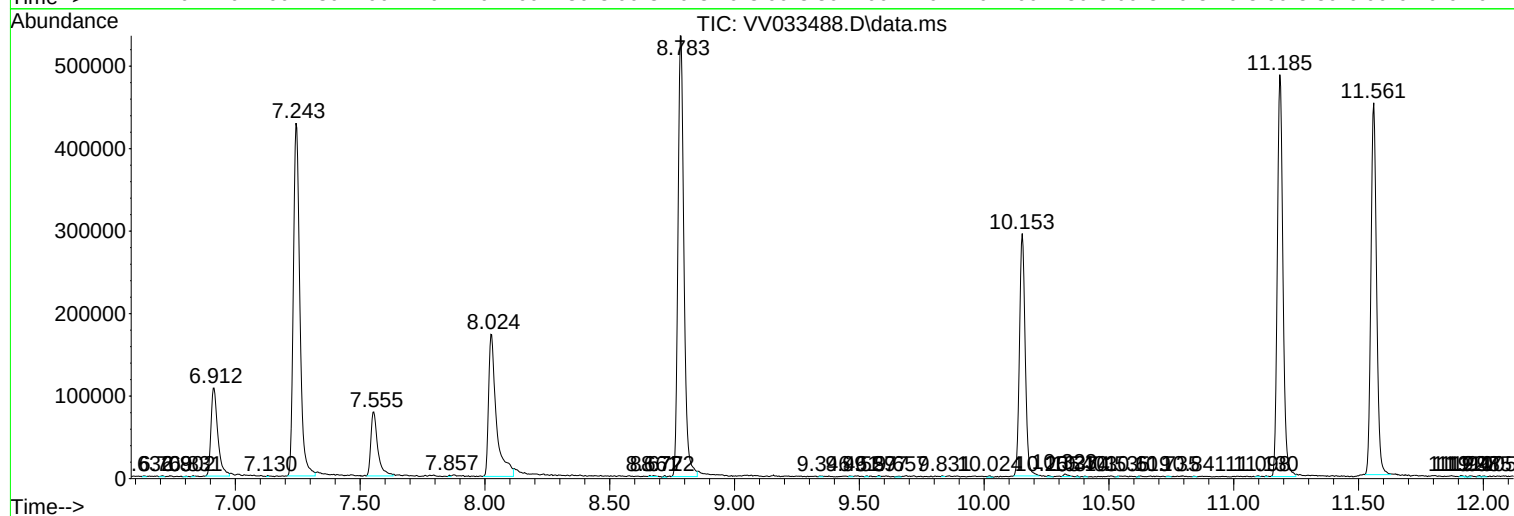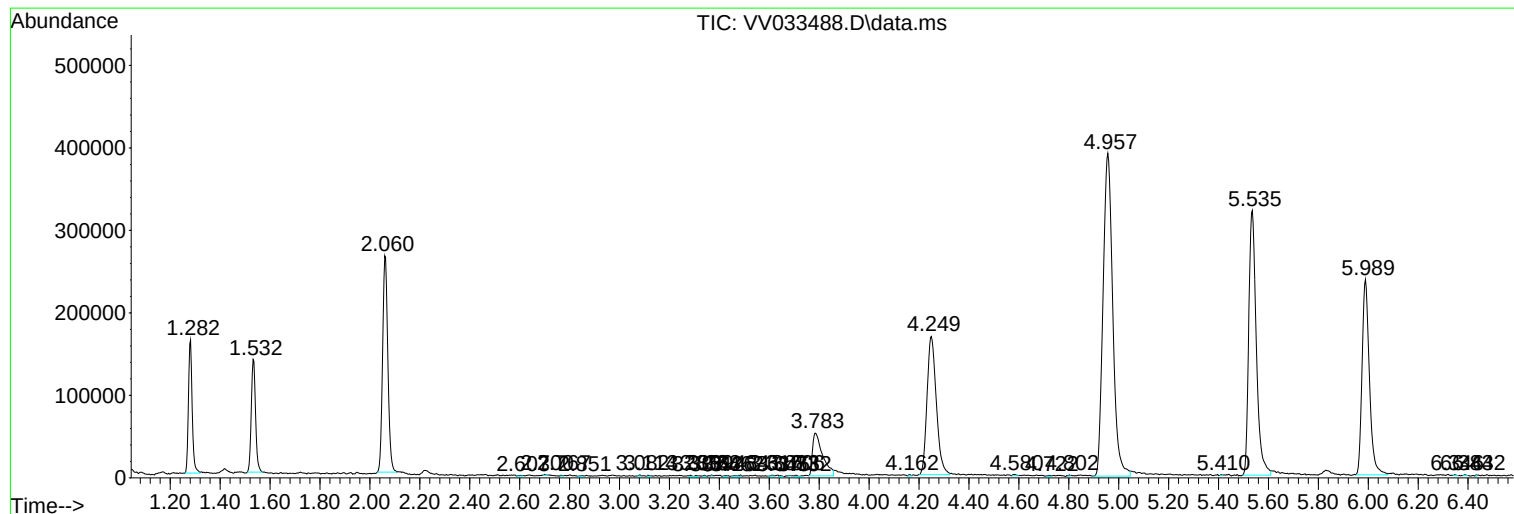

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033488.D
Acq On : 19 Dec 2023 19:13
Operator : SY/MD
Sample : 05912-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033488.D
Acq On : 19 Dec 2023 19:13
Operator : SY/MD
Sample : 05912-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc