

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033489.D
 Acq On : 19 Dec 2023 19:36
 Operator : SY/MD
 Sample : 05912-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rBV	161050	169713	16.10%	2.106%
2	1.532	146	153	169	rVB	140443	166445	15.79%	2.066%
3	2.060	308	317	335	rBV	263882	393312	37.32%	4.881%
4	2.426	427	431	436	rBV4	1499	1873	0.18%	0.023%
5	2.561	471	473	476	rVB3	1272	711	0.07%	0.009%
6	2.580	476	479	480	rBV2	1323	716	0.07%	0.009%
7	2.632	492	495	497	rBV3	793	507	0.05%	0.006%
8	2.770	534	538	540	rBV5	1233	732	0.07%	0.009%
9	2.986	602	605	607	rBV3	1150	814	0.08%	0.010%
10	2.998	607	609	610	rVV2	1179	468	0.04%	0.006%
11	3.008	610	612	614	rVB2	1008	502	0.05%	0.006%
12	3.101	639	641	643	rBV3	1176	529	0.05%	0.007%
13	3.179	662	665	669	rBV4	830	520	0.05%	0.006%
14	3.211	672	675	676	rBV2	1046	641	0.06%	0.008%
15	3.310	705	706	713	rVB7	1312	718	0.07%	0.009%
16	3.352	715	719	720	rBV2	1165	720	0.07%	0.009%
17	3.378	723	727	731	rVB5	1154	840	0.08%	0.010%
18	3.404	731	735	737	rBV3	1155	883	0.08%	0.011%
19	3.455	747	751	753	rVB3	932	567	0.05%	0.007%
20	3.478	756	758	762	rBV3	915	504	0.05%	0.006%
21	3.506	764	767	771	rVV6	930	699	0.07%	0.009%
22	3.523	771	772	775	rVB3	1282	466	0.04%	0.006%
23	3.539	775	777	783	rBV6	1053	864	0.08%	0.011%
24	3.571	783	787	789	rBV3	1125	802	0.08%	0.010%
25	3.783	845	853	882	rBV	53350	152268	14.45%	1.890%
26	4.249	985	998	1022	rVB	167250	429147	40.72%	5.326%
27	4.818	1173	1175	1178	rVB3	1060	570	0.05%	0.007%
28	4.886	1193	1196	1197	rBV2	927	528	0.05%	0.007%
29	4.957	1203	1218	1243	rBV2	397878	1053949	100.00%	13.079%
30	5.535	1386	1398	1434	rBV	323820	694247	65.87%	8.616%
31	5.989	1526	1539	1564	rBV2	236849	499305	47.37%	6.196%
32	6.503	1697	1699	1701	rBV2	1059	590	0.06%	0.007%
33	6.545	1710	1712	1714	rBV3	967	488	0.05%	0.006%
34	6.567	1717	1719	1722	rVB4	1090	490	0.05%	0.006%
35	6.728	1767	1769	1773	rVB5	1455	1014	0.10%	0.013%
36	6.754	1773	1777	1778	rBV4	1125	627	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033489.D
 Acq On : 19 Dec 2023 19:36
 Operator : SY/MD
 Sample : 05912-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.818	1793	1797	1798	rBV4	1306	660	0.06%	0.008%
38	6.866	1807	1812	1817	rBV8	1124	1388	0.13%	0.017%
39	6.915	1817	1827	1847	rBV	111038	214619	20.36%	2.663%
40	7.153	1898	1901	1904	rBV5	1212	1018	0.10%	0.013%
41	7.243	1918	1929	1957	rBV	441673	789756	74.93%	9.801%
42	7.555	2017	2026	2049	rBV	79864	146997	13.95%	1.824%
43	7.828	2109	2111	2114	rBV4	1276	680	0.06%	0.008%
44	7.976	2155	2157	2160	rBV3	810	466	0.04%	0.006%
45	8.024	2163	2172	2216	rVV	174431	393639	37.35%	4.885%
46	8.554	2334	2337	2340	rBV5	1208	686	0.07%	0.009%
47	8.683	2375	2377	2379	rBV2	1118	672	0.06%	0.008%
48	8.709	2383	2385	2390	rBV5	978	953	0.09%	0.012%
49	8.783	2398	2408	2431	rBV	547133	907389	86.09%	11.261%
50	9.294	2564	2567	2570	rBV5	1717	1320	0.13%	0.016%
51	9.400	2596	2600	2603	rBV4	1288	1212	0.11%	0.015%
52	9.490	2624	2628	2631	rVB6	2108	1604	0.15%	0.020%
53	9.513	2631	2635	2637	rBV4	1256	885	0.08%	0.011%
54	9.667	2680	2683	2684	rBV2	960	574	0.05%	0.007%
55	9.873	2745	2747	2749	rVB3	1499	531	0.05%	0.007%
56	9.937	2765	2767	2770	rBV4	1134	697	0.07%	0.009%
57	10.024	2790	2794	2796	rBV3	942	892	0.08%	0.011%
58	10.062	2804	2806	2810	rVB5	1486	1091	0.10%	0.014%
59	10.085	2810	2813	2816	rBV4	1250	995	0.09%	0.012%
60	10.153	2822	2834	2852	rBV	299779	477137	45.27%	5.921%
61	10.294	2872	2878	2880	rVB5	1263	1299	0.12%	0.016%
62	10.374	2899	2903	2905	rVB4	1348	1056	0.10%	0.013%
63	10.423	2914	2918	2921	rBV5	1177	1168	0.11%	0.014%
64	10.458	2927	2929	2931	rBV3	1310	732	0.07%	0.009%
65	10.516	2945	2947	2950	rVB4	1355	773	0.07%	0.010%
66	10.603	2971	2974	2975	rBV3	956	546	0.05%	0.007%
67	10.654	2988	2990	2994	rBV4	1228	548	0.05%	0.007%
68	11.185	3144	3155	3180	rBV	496413	779153	73.93%	9.669%
69	11.365	3208	3211	3215	rBV5	1456	1304	0.12%	0.016%
70	11.455	3235	3239	3242	rBV5	1313	1033	0.10%	0.013%
71	11.561	3261	3272	3290	rBV	457917	721392	68.45%	8.952%
72	11.869	3365	3368	3371	rBV4	724	552	0.05%	0.007%
73	12.056	3423	3426	3427	rBV3	1005	499	0.05%	0.006%
74	12.114	3440	3444	3445	rBV3	1292	1018	0.10%	0.013%
75	12.535	3572	3575	3577	rBV3	1236	767	0.07%	0.010%
76	12.570	3583	3586	3588	rBV3	1399	680	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033489.D
 Acq On : 19 Dec 2023 19:36
 Operator : SY/MD
 Sample : 05912-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.648	3608	3610	3614	rVB3	857	483	0.05%	0.006%
78	12.789	3650	3654	3655	rBV3	879	469	0.04%	0.006%
79	12.918	3690	3694	3696	rBV4	917	782	0.07%	0.010%
80	13.046	3731	3734	3738	rBV4	945	612	0.06%	0.008%
81	13.075	3740	3743	3745	rBV4	1278	646	0.06%	0.008%
82	13.091	3745	3748	3752	rVB4	959	764	0.07%	0.009%
83	13.175	3769	3774	3777	rBV5	1819	1763	0.17%	0.022%
84	13.230	3789	3791	3794	rBV4	762	483	0.05%	0.006%
85	13.316	3814	3818	3821	rVB6	1293	961	0.09%	0.012%
86	13.332	3821	3823	3825	rBV3	1069	663	0.06%	0.008%
87	13.368	3831	3834	3835	rBV3	1045	552	0.05%	0.007%
88	13.786	3961	3964	3965	rBV2	1364	718	0.07%	0.009%
89	14.043	4041	4044	4046	rBV4	876	625	0.06%	0.008%
90	14.104	4061	4063	4068	rBV6	844	743	0.07%	0.009%
91	14.252	4104	4109	4113	rBV7	1528	1840	0.17%	0.023%
92	14.358	4137	4142	4147	rBV6	1662	1679	0.16%	0.021%
93	14.381	4147	4149	4153	rVB4	1163	903	0.09%	0.011%
94	14.905	4309	4312	4313	rBV2	1229	637	0.06%	0.008%
95	15.001	4339	4342	4345	rBV4	1692	1147	0.11%	0.014%
96	15.156	4388	4390	4392	rBV2	1123	557	0.05%	0.007%
97	15.586	4520	4524	4525	rBV3	1423	1150	0.11%	0.014%
98	15.911	4623	4625	4628	rBV3	1281	923	0.09%	0.011%
99	16.072	4673	4675	4679	rBV5	1561	868	0.08%	0.011%
100	16.393	4773	4775	4780	rBV6	2113	1971	0.19%	0.024%




Sum of corrected areas: 8058089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033489.D
Acq On : 19 Dec 2023 19:36
Operator : SY/MD
Sample : 05912-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

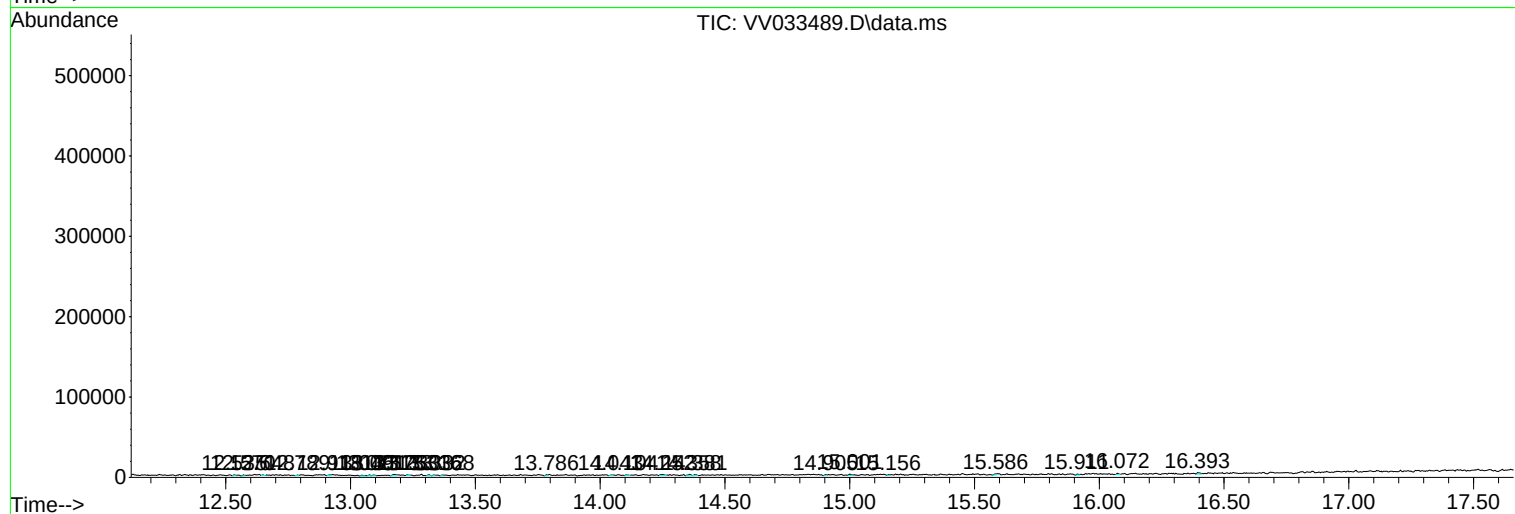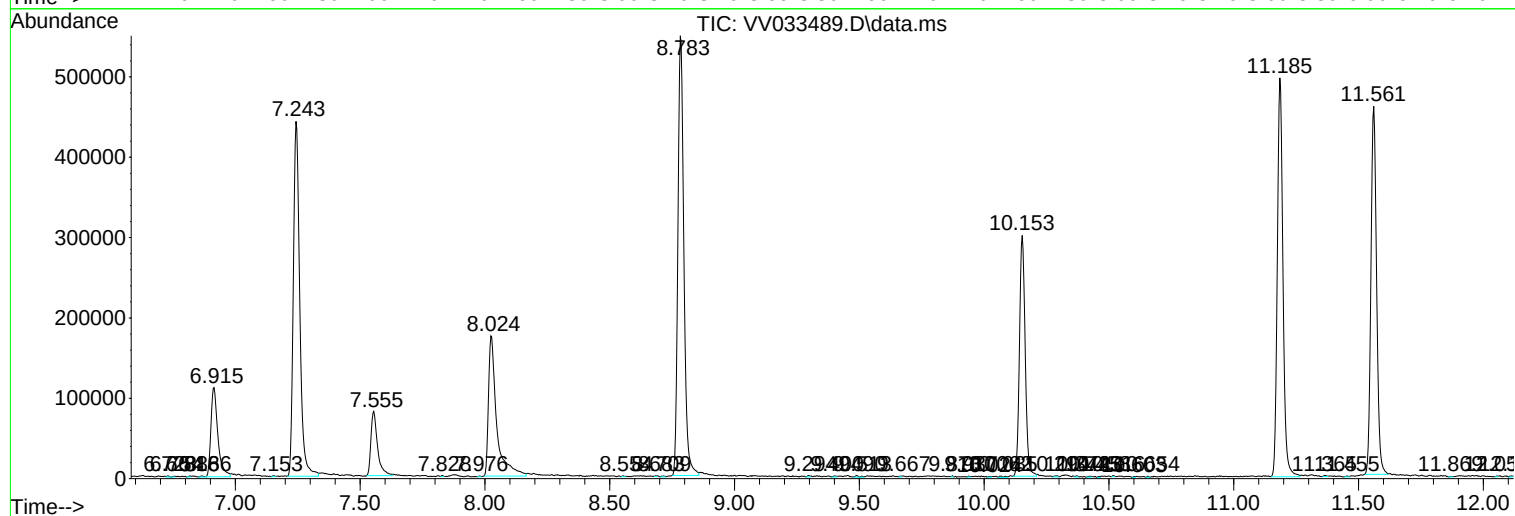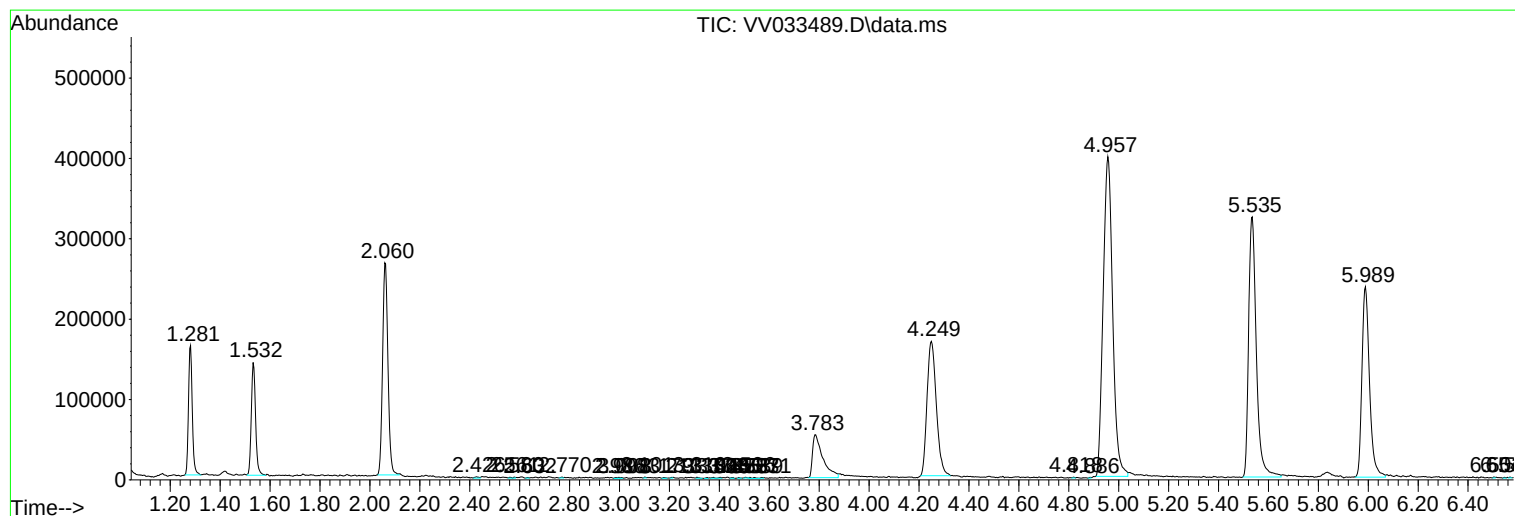

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033489.D
Acq On : 19 Dec 2023 19:36
Operator : SY/MD
Sample : 05912-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033489.D
Acq On : 19 Dec 2023 19:36
Operator : SY/MD
Sample : 05912-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc