

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033490.D
 Acq On : 19 Dec 2023 20:00
 Operator : SY/MD
 Sample : 05912-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rBV	160085	168921	15.69%	2.087%
2	1.532	147	153	166	rVB	138249	161050	14.96%	1.990%
3	2.063	308	318	333	rBV	258128	385886	35.84%	4.768%
4	2.439	431	435	436	rBV3	1614	1076	0.10%	0.013%
5	2.635	491	496	497	rBV4	1571	1299	0.12%	0.016%
6	2.683	508	511	513	rBV3	1799	1048	0.10%	0.013%
7	2.757	531	534	536	rBV4	1026	672	0.06%	0.008%
8	2.796	541	546	552	rBV8	1140	1063	0.10%	0.013%
9	2.831	553	557	559	rBV5	1429	1011	0.09%	0.012%
10	3.076	631	633	636	rBV3	985	563	0.05%	0.007%
11	3.108	639	643	644	rBV5	3627	2590	0.24%	0.032%
12	3.172	660	663	665	rBV4	1022	839	0.08%	0.010%
13	3.220	676	678	682	rVB4	1799	1032	0.10%	0.013%
14	3.307	703	705	709	rVB5	1289	714	0.07%	0.009%
15	3.445	746	748	751	rVB4	1050	613	0.06%	0.008%
16	3.461	751	753	757	rVB5	1006	687	0.06%	0.008%
17	3.519	767	771	772	rBV4	1046	760	0.07%	0.009%
18	3.574	784	788	790	rVV5	822	543	0.05%	0.007%
19	3.696	821	826	827	rBV4	1555	1197	0.11%	0.015%
20	3.786	845	854	885	rBV	52778	181973	16.90%	2.248%
21	4.249	985	998	1027	rVB	167101	425733	39.54%	5.260%
22	4.802	1168	1170	1172	rBV2	1112	672	0.06%	0.008%
23	4.844	1181	1183	1186	rVB4	1286	613	0.06%	0.008%
24	4.957	1201	1218	1252	rBV2	396556	1076719	100.00%	13.304%
25	5.535	1386	1398	1425	rVV	315378	667409	61.99%	8.246%
26	5.989	1528	1539	1565	rBV	231405	475864	44.20%	5.880%
27	6.545	1708	1712	1713	rBV4	938	601	0.06%	0.007%
28	6.754	1775	1777	1779	rVB3	1397	607	0.06%	0.007%
29	6.776	1779	1784	1787	rBV5	1178	798	0.07%	0.010%
30	6.841	1802	1804	1810	rBV6	913	809	0.08%	0.010%
31	6.911	1814	1826	1852	rBV	107619	213779	19.85%	2.641%
32	7.243	1918	1929	1961	rVV	438082	787378	73.13%	9.729%
33	7.555	2017	2026	2051	rBV	80112	150008	13.93%	1.853%
34	7.844	2113	2116	2119	rBV3	1370	1126	0.10%	0.014%
35	8.024	2162	2172	2199	rBV	172999	367534	34.13%	4.541%
36	8.593	2346	2349	2352	rBV5	1370	969	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033490.D
 Acq On : 19 Dec 2023 20:00
 Operator : SY/MD
 Sample : 05912-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.696	2378	2381	2383	rVB4	1001	565	0.05%	0.007%
38	8.786	2397	2409	2414	rBV	567292	938832	87.19%	11.600%
39	9.162	2523	2526	2533	rVB7	1562	1380	0.13%	0.017%
40	9.394	2596	2598	2602	rVB5	1223	775	0.07%	0.010%
41	9.429	2602	2609	2611	rBV8	1822	1808	0.17%	0.022%
42	9.490	2626	2628	2633	rBV4	934	752	0.07%	0.009%
43	9.583	2654	2657	2660	rBV5	1332	746	0.07%	0.009%
44	9.612	2663	2666	2668	rVB4	1479	705	0.07%	0.009%
45	9.641	2672	2675	2676	rBV2	1151	743	0.07%	0.009%
46	9.699	2689	2693	2694	rBV4	1258	936	0.09%	0.012%
47	9.815	2725	2729	2731	rBV4	897	741	0.07%	0.009%
48	9.969	2771	2777	2779	rBV4	1523	1076	0.10%	0.013%
49	10.034	2793	2797	2799	rBV5	878	776	0.07%	0.010%
50	10.079	2809	2811	2813	rBV2	1120	614	0.06%	0.008%
51	10.152	2819	2834	2851	rBV	291522	471898	43.83%	5.831%
52	10.297	2876	2879	2881	rBV4	741	588	0.05%	0.007%
53	10.358	2896	2898	2901	rVB4	1007	559	0.05%	0.007%
54	10.400	2908	2911	2917	rBV7	1309	1364	0.13%	0.017%
55	10.452	2924	2927	2929	rVB3	1373	732	0.07%	0.009%
56	10.474	2929	2934	2936	rBV6	1182	1065	0.10%	0.013%
57	10.686	2998	3000	3005	rVB5	1296	879	0.08%	0.011%
58	10.725	3009	3012	3015	rBV3	1076	750	0.07%	0.009%
59	10.744	3015	3018	3020	rBV4	1266	880	0.08%	0.011%
60	10.799	3033	3035	3037	rBV3	1286	843	0.08%	0.010%
61	10.863	3053	3055	3058	rBV3	1056	700	0.07%	0.009%
62	11.056	3113	3115	3118	rVB4	962	530	0.05%	0.007%
63	11.098	3125	3128	3130	rBV4	1597	1118	0.10%	0.014%
64	11.127	3130	3137	3145	rVV8	4162	6136	0.57%	0.076%
65	11.185	3145	3155	3181	rVV	494315	814343	75.63%	10.062%
66	11.468	3238	3243	3244	rBV4	1510	1184	0.11%	0.015%
67	11.561	3262	3272	3291	rBV	456083	725024	67.34%	8.958%
68	12.111	3440	3443	3445	rBV3	1015	693	0.06%	0.009%
69	12.159	3456	3458	3461	rBV3	1264	771	0.07%	0.010%
70	12.361	3519	3521	3523	rVB3	1366	576	0.05%	0.007%
71	12.487	3558	3560	3564	rVV6	1032	686	0.06%	0.008%
72	12.609	3595	3598	3601	rBV5	1255	798	0.07%	0.010%
73	12.799	3655	3657	3660	rBV4	1128	645	0.06%	0.008%
74	13.069	3737	3741	3742	rBV3	1344	711	0.07%	0.009%
75	13.242	3793	3795	3801	rBV7	1329	838	0.08%	0.010%
76	13.281	3804	3807	3812	rVB5	1250	858	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033490.D
 Acq On : 19 Dec 2023 20:00
 Operator : SY/MD
 Sample : 05912-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.342	3823	3826	3828	rBV4	1048	751	0.07%	0.009%
78	13.361	3828	3832	3834	rVB4	1162	838	0.08%	0.010%
79	13.445	3855	3858	3861	rBV4	1354	853	0.08%	0.011%
80	13.496	3870	3874	3877	rVB5	1099	733	0.07%	0.009%
81	13.516	3877	3880	3885	rBV6	1339	1023	0.10%	0.013%
82	13.574	3893	3898	3901	rBV5	1352	1169	0.11%	0.014%
83	14.075	4052	4054	4056	rBV3	1305	792	0.07%	0.010%
84	14.114	4062	4066	4069	rVB5	1434	1274	0.12%	0.016%
85	14.136	4069	4073	4075	rBV4	713	616	0.06%	0.008%
86	14.220	4097	4099	4106	rBV7	959	1275	0.12%	0.016%
87	14.326	4127	4132	4135	rBV7	1081	1223	0.11%	0.015%
88	14.371	4142	4146	4151	rBV9	1396	1739	0.16%	0.021%
89	14.416	4158	4160	4165	rBV6	872	674	0.06%	0.008%
90	14.477	4175	4179	4182	rBV5	1217	947	0.09%	0.012%
91	14.519	4189	4192	4195	rBV5	1243	914	0.08%	0.011%
92	14.741	4259	4261	4266	rBV6	1081	680	0.06%	0.008%
93	14.901	4307	4311	4315	rBV6	1561	1523	0.14%	0.019%
94	15.136	4382	4384	4388	rBV4	1068	929	0.09%	0.011%
95	15.162	4388	4392	4395	rBV5	1673	1170	0.11%	0.014%
96	15.316	4437	4440	4442	rBV3	1334	743	0.07%	0.009%
97	15.361	4450	4454	4455	rBV3	1493	1153	0.11%	0.014%
98	15.548	4511	4512	4517	rVB5	1280	639	0.06%	0.008%
99	15.876	4610	4614	4616	rBV4	1427	1192	0.11%	0.015%
100	16.419	4781	4783	4784	rBV2	1740	738	0.07%	0.009%




Sum of corrected areas: 8093362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033490.D
Acq On : 19 Dec 2023 20:00
Operator : SY/MD
Sample : 05912-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

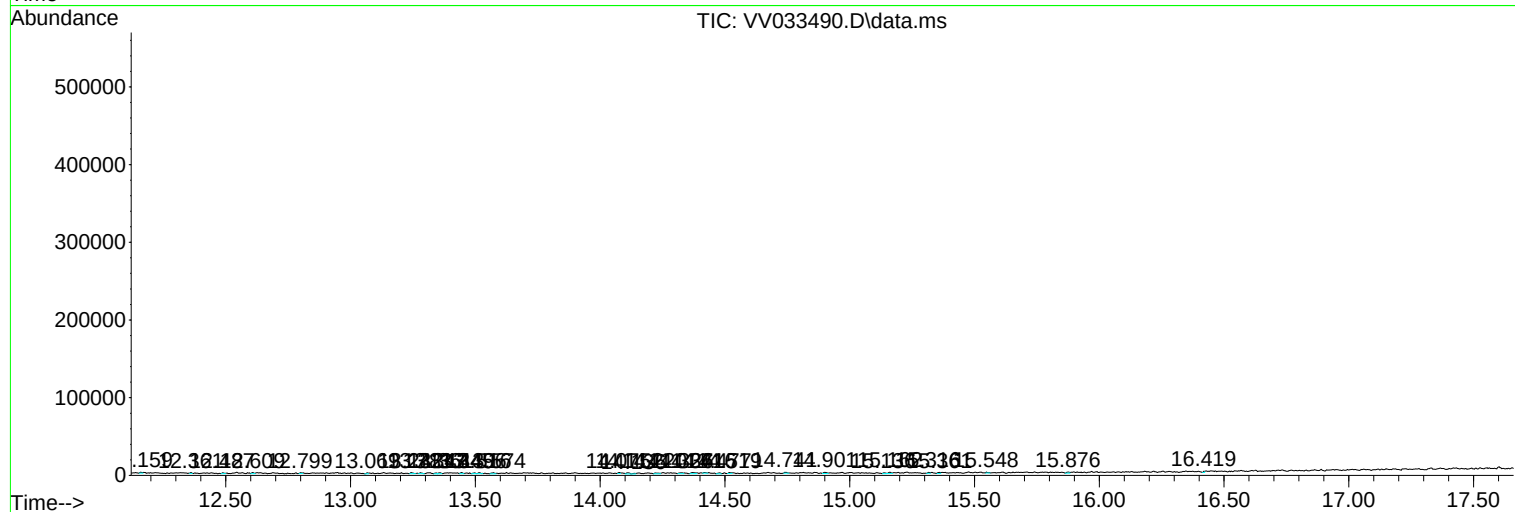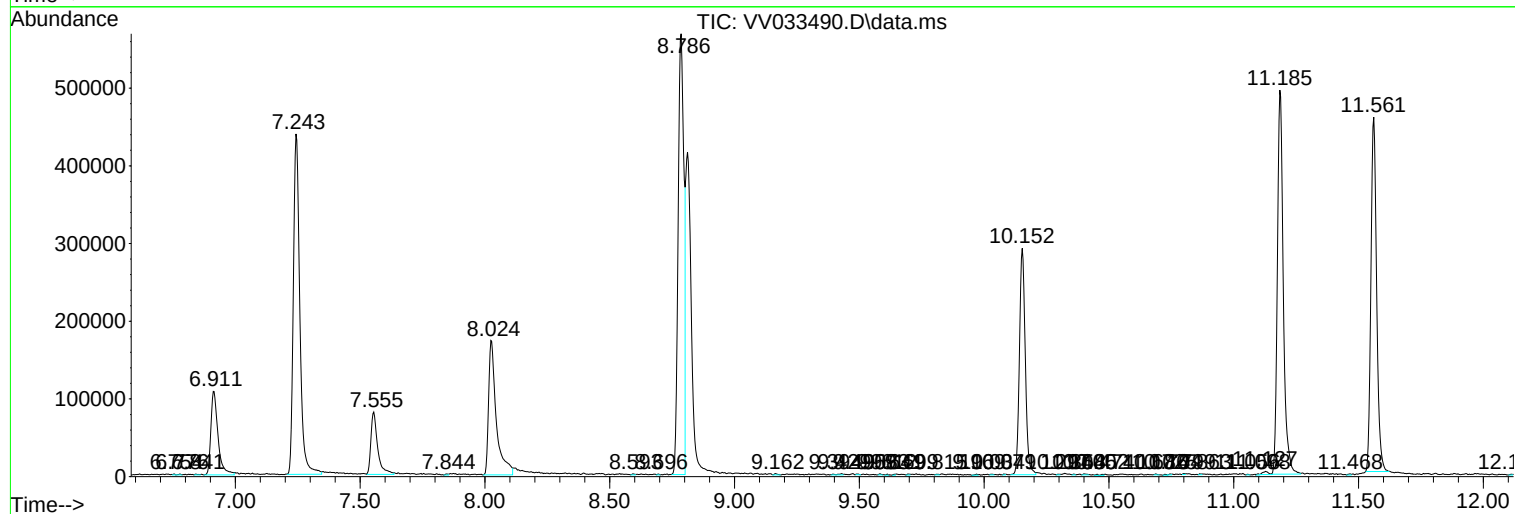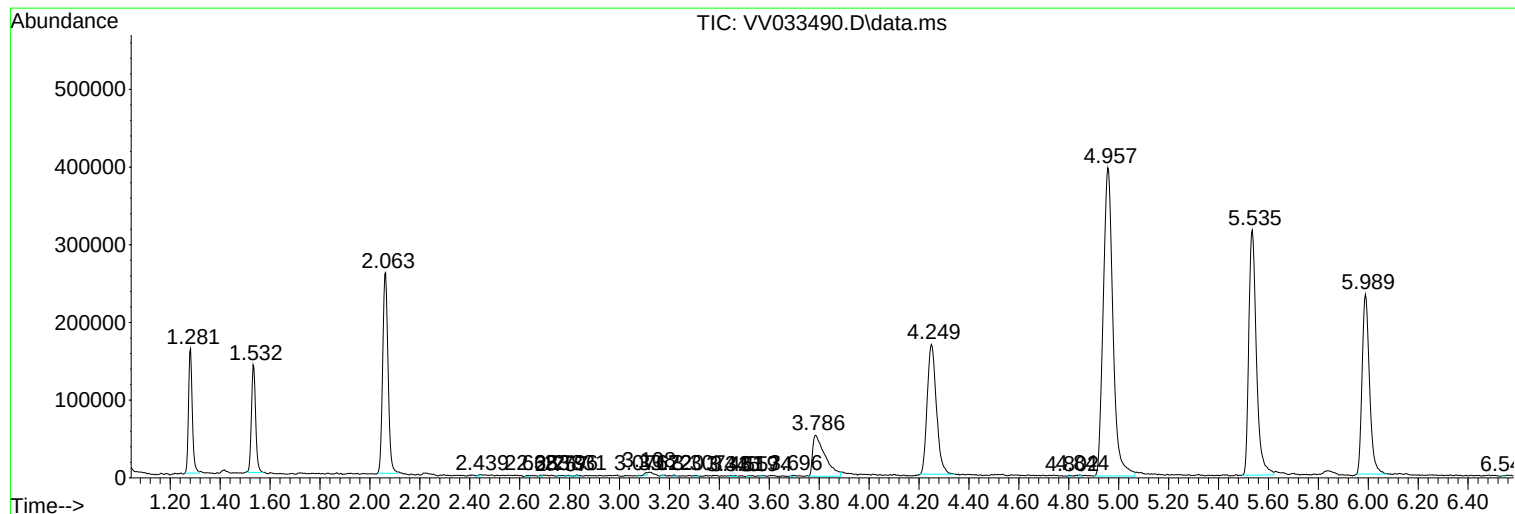

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033490.D
Acq On : 19 Dec 2023 20:00
Operator : SY/MD
Sample : 05912-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033490.D
Acq On : 19 Dec 2023 20:00
Operator : SY/MD
Sample : 05912-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------