

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033491.D
 Acq On : 19 Dec 2023 20:23
 Operator : SY/MD
 Sample : 05912-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV2	153602	168915	18.34%	2.407%
2	1.532	146	153	165	rVB	116835	138287	15.01%	1.970%
3	2.060	308	317	332	rBV	208352	309574	33.60%	4.411%
4	2.741	528	529	531	rBV2	1251	527	0.06%	0.008%
5	2.777	537	540	542	rBV4	1741	1015	0.11%	0.014%
6	2.883	571	573	575	rBV3	860	344	0.04%	0.005%
7	2.899	575	578	584	rVB7	1025	934	0.10%	0.013%
8	2.957	594	596	597	rBV2	802	282	0.03%	0.004%
9	2.986	600	605	606	rBV3	1345	1110	0.12%	0.016%
10	3.056	621	627	631	rBV7	1266	1432	0.16%	0.020%
11	3.114	632	645	656	rBV3	26198	57826	6.28%	0.824%
12	3.246	684	686	689	rBV4	1014	557	0.06%	0.008%
13	3.285	697	698	702	rBV3	1058	718	0.08%	0.010%
14	3.314	704	707	710	rVB4	1696	1211	0.13%	0.017%
15	3.355	718	720	725	rBV5	1457	1194	0.13%	0.017%
16	3.420	738	740	742	rBV3	1087	433	0.05%	0.006%
17	3.484	757	760	762	rBV4	1151	579	0.06%	0.008%
18	3.523	768	772	778	rVB9	1389	1640	0.18%	0.023%
19	3.555	778	782	783	rBV3	695	471	0.05%	0.007%
20	3.609	797	799	808	rVB8	1500	1860	0.20%	0.027%
21	3.648	808	811	812	rBV3	1636	858	0.09%	0.012%
22	3.732	835	837	839	rBV3	1435	702	0.08%	0.010%
23	3.812	846	862	879	rBV4	68169	255147	27.70%	3.636%
24	4.249	983	998	1020	rBV	143779	372938	40.48%	5.314%
25	4.841	1178	1182	1184	rVB4	1027	682	0.07%	0.010%
26	4.896	1194	1199	1201	rBV6	1076	963	0.10%	0.014%
27	4.957	1203	1218	1255	rVV2	334613	921252	100.00%	13.127%
28	5.368	1344	1346	1349	rBV4	1178	601	0.07%	0.009%
29	5.535	1386	1398	1418	rBV	260055	549045	59.60%	7.823%
30	5.989	1528	1539	1564	rBV	198718	409704	44.47%	5.838%
31	6.323	1640	1643	1645	rBV3	1128	856	0.09%	0.012%
32	6.391	1662	1664	1666	rBV3	883	238	0.03%	0.003%
33	6.494	1694	1696	1699	rBV3	804	470	0.05%	0.007%
34	6.535	1706	1709	1710	rBV3	1102	559	0.06%	0.008%
35	6.613	1729	1733	1734	rBV3	919	546	0.06%	0.008%
36	6.683	1752	1755	1759	rBV5	875	672	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033491.D
 Acq On : 19 Dec 2023 20:23
 Operator : SY/MD
 Sample : 05912-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.728	1766	1769	1770	rBV2	914	498	0.05%	0.007%
38	6.915	1817	1827	1845	rBV	91901	177648	19.28%	2.531%
39	7.243	1918	1929	1953	rBV	353962	642025	69.69%	9.148%
40	7.555	2018	2026	2043	rBV	67192	121576	13.20%	1.732%
41	7.799	2100	2102	2104	rBV3	855	526	0.06%	0.007%
42	7.937	2144	2145	2146	rBV	795	282	0.03%	0.004%
43	7.985	2158	2160	2162	rBV2	1029	583	0.06%	0.008%
44	8.024	2163	2172	2207	rVV	161799	357615	38.82%	5.096%
45	8.432	2297	2299	2300	rBV2	945	357	0.04%	0.005%
46	8.506	2320	2322	2324	rBV3	1450	804	0.09%	0.011%
47	8.545	2332	2334	2338	rBV4	836	419	0.05%	0.006%
48	8.606	2348	2353	2356	rBV6	1527	1425	0.15%	0.020%
49	8.702	2380	2383	2385	rBV2	1557	626	0.07%	0.009%
50	8.786	2398	2409	2413	rBV	479678	752199	81.65%	10.718%
51	9.149	2520	2522	2524	rBV3	1126	647	0.07%	0.009%
52	9.185	2530	2533	2534	rBV3	1230	752	0.08%	0.011%
53	9.436	2610	2611	2617	rVB6	1389	1058	0.11%	0.015%
54	9.497	2628	2630	2634	rBV4	1125	664	0.07%	0.009%
55	9.600	2659	2662	2665	rBV4	809	507	0.06%	0.007%
56	9.651	2673	2678	2681	rBV5	1241	1204	0.13%	0.017%
57	9.731	2701	2703	2705	rBV3	821	295	0.03%	0.004%
58	9.754	2709	2710	2712	rVB2	726	204	0.02%	0.003%
59	9.870	2744	2746	2749	rBV4	1607	1197	0.13%	0.017%
60	10.021	2791	2793	2796	rBV3	753	483	0.05%	0.007%
61	10.037	2796	2798	2799	rBV	872	405	0.04%	0.006%
62	10.085	2811	2813	2816	rBV4	1235	884	0.10%	0.013%
63	10.153	2820	2834	2848	rBV	275280	434662	47.18%	6.193%
64	10.307	2880	2882	2883	rBV2	1128	399	0.04%	0.006%
65	10.471	2930	2933	2934	rBV2	618	367	0.04%	0.005%
66	10.561	2959	2961	2963	rBV2	992	403	0.04%	0.006%
67	10.587	2967	2969	2972	rVB3	1065	620	0.07%	0.009%
68	10.853	3051	3052	3055	rBV2	659	295	0.03%	0.004%
69	10.992	3093	3095	3096	rBV2	854	351	0.04%	0.005%
70	11.075	3119	3121	3125	rVB5	1329	939	0.10%	0.013%
71	11.095	3125	3127	3128	rBV2	795	245	0.03%	0.003%
72	11.185	3145	3155	3179	rBV	398572	675685	73.34%	9.628%
73	11.503	3251	3254	3256	rBV2	1725	919	0.10%	0.013%
74	11.561	3262	3272	3290	rBV	383487	616718	66.94%	8.787%
75	11.773	3334	3338	3345	rBV8	1436	1270	0.14%	0.018%
76	11.857	3358	3364	3365	rBV6	1745	1512	0.16%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033491.D
 Acq On : 19 Dec 2023 20:23
 Operator : SY/MD
 Sample : 05912-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	11.963	3395	3397	3400	rBV4	1065	693	0.08%	0.010%
78	12.034	3416	3419	3421	rBV5	1188	939	0.10%	0.013%
79	12.046	3421	3423	3425	rBV3	1035	483	0.05%	0.007%
80	12.104	3439	3441	3442	rBV3	723	322	0.03%	0.005%
81	12.387	3526	3529	3531	rVB3	1050	451	0.05%	0.006%
82	12.400	3531	3533	3534	rBV2	917	419	0.05%	0.006%
83	12.622	3600	3602	3609	rBV6	948	821	0.09%	0.012%
84	13.140	3758	3763	3764	rBV3	882	746	0.08%	0.011%
85	13.233	3790	3792	3793	rBV2	960	337	0.04%	0.005%
86	13.310	3814	3816	3819	rBV3	1029	629	0.07%	0.009%
87	13.416	3847	3849	3850	rBV2	1157	496	0.05%	0.007%
88	13.500	3874	3875	3879	rVB3	1540	674	0.07%	0.010%
89	13.541	3886	3888	3890	rBV2	1199	656	0.07%	0.009%
90	13.673	3928	3929	3933	rVB4	663	263	0.03%	0.004%
91	13.696	3933	3936	3938	rBV4	1481	827	0.09%	0.012%
92	13.792	3962	3966	3968	rBV3	1225	837	0.09%	0.012%
93	13.918	4003	4005	4007	rVB	921	299	0.03%	0.004%
94	14.037	4040	4042	4045	rBV4	776	314	0.03%	0.004%
95	14.069	4050	4052	4054	rBV3	1420	657	0.07%	0.009%
96	14.217	4095	4098	4102	rBV5	1278	941	0.10%	0.013%
97	14.667	4235	4238	4239	rBV2	1149	480	0.05%	0.007%
98	14.821	4285	4286	4289	rBV2	1051	590	0.06%	0.008%
99	14.966	4327	4331	4334	rBV6	1517	1511	0.16%	0.022%
100	15.130	4380	4382	4384	rVB3	1016	356	0.04%	0.005%




Sum of corrected areas: 7018151

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033491.D
Acq On : 19 Dec 2023 20:23
Operator : SY/MD
Sample : 05912-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

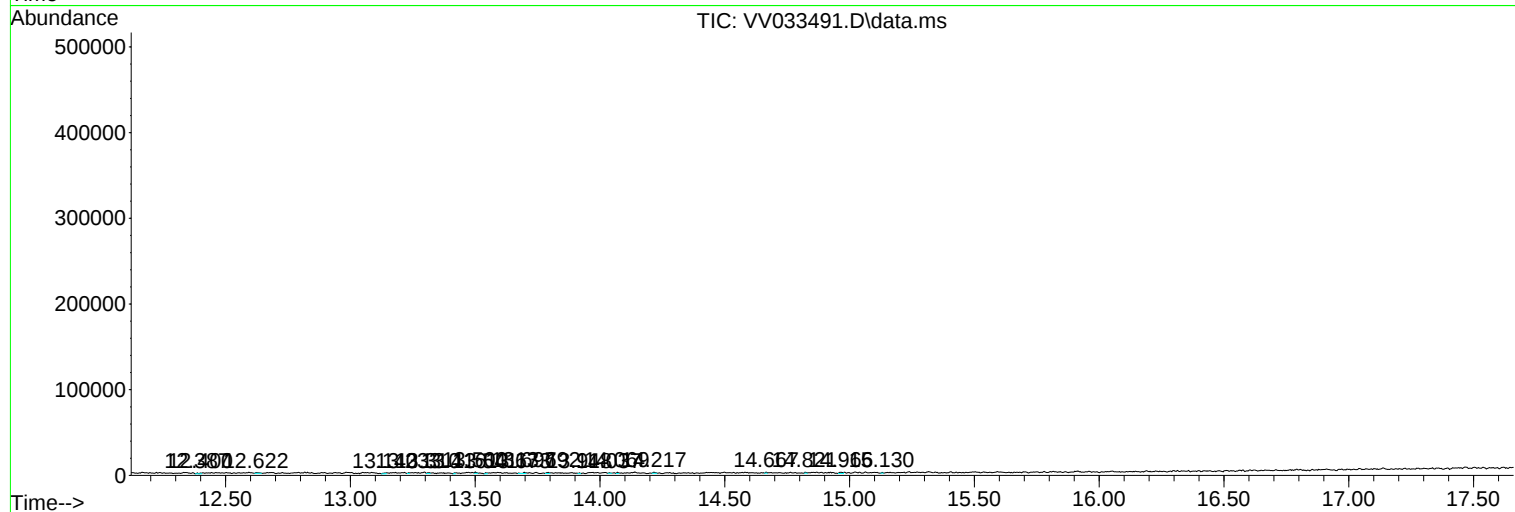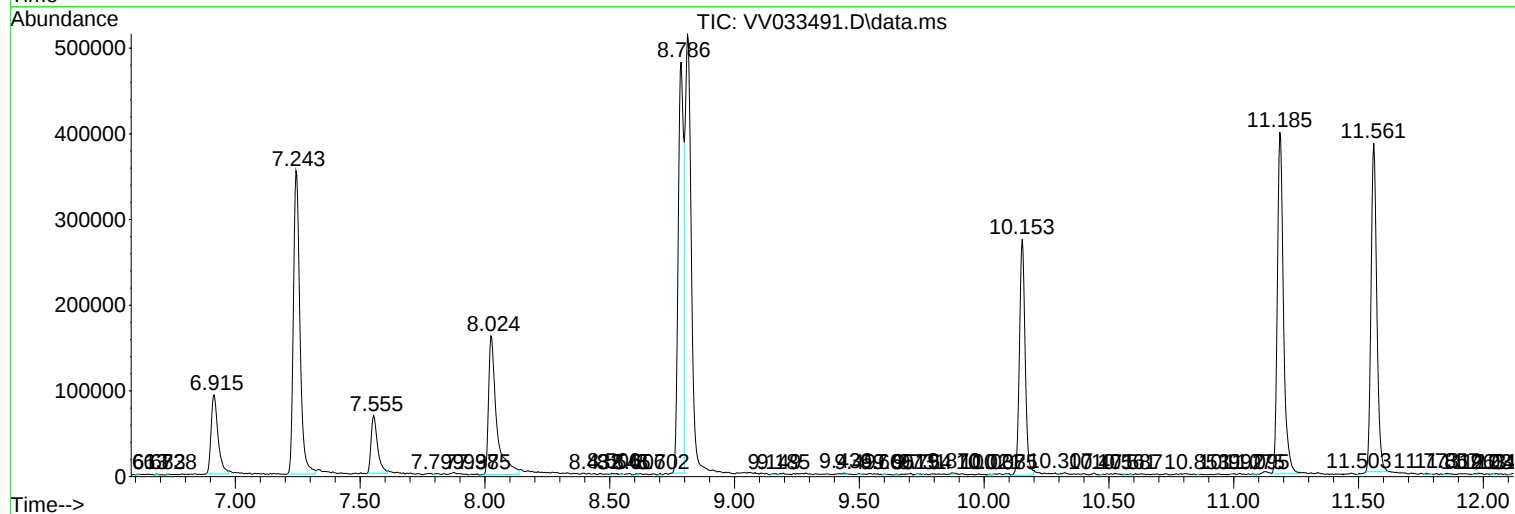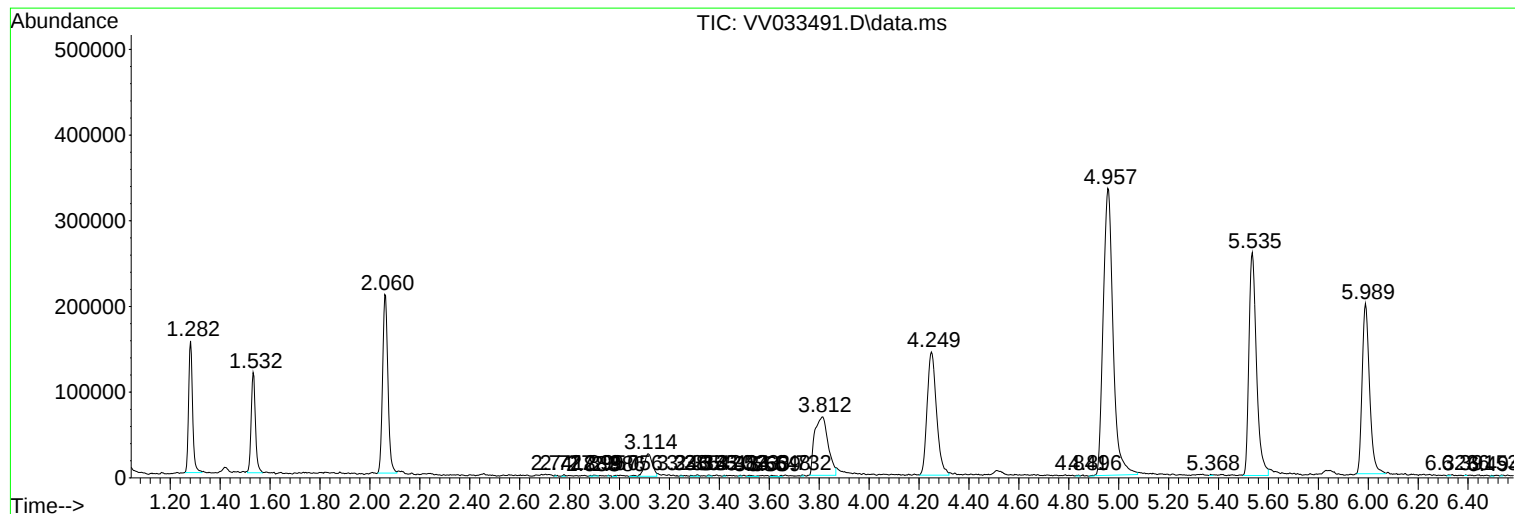

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033491.D
Acq On : 19 Dec 2023 20:23
Operator : SY/MD
Sample : 05912-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033491.D
Acq On : 19 Dec 2023 20:23
Operator : SY/MD
Sample : 05912-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------