

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033492.D
 Acq On : 19 Dec 2023 20:46
 Operator : SY/MD
 Sample : 05912-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VW033492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rBV	162473	165194	15.87%	2.070%
2	1.532	146	153	166	rVB	135109	157577	15.13%	1.975%
3	2.059	308	317	332	rBV	259761	382775	36.76%	4.797%
4	2.571	473	476	477	rBV3	1668	604	0.06%	0.008%
5	2.651	498	501	504	rVB5	948	525	0.05%	0.007%
6	2.670	504	507	512	rBV6	1223	1337	0.13%	0.017%
7	2.850	559	563	566	rVB5	1558	1338	0.13%	0.017%
8	2.879	568	572	576	rVB7	1468	1201	0.12%	0.015%
9	2.899	576	578	581	rBV4	821	598	0.06%	0.007%
10	2.944	589	592	594	rVB3	1041	563	0.05%	0.007%
11	3.002	606	610	615	rVB4	1558	1414	0.14%	0.018%
12	3.278	693	696	699	rVB4	1014	709	0.07%	0.009%
13	3.297	699	702	704	rBV3	818	502	0.05%	0.006%
14	3.397	730	733	735	rBV3	807	476	0.05%	0.006%
15	3.465	750	754	756	rBV3	1345	900	0.09%	0.011%
16	3.542	774	778	780	rBV3	1501	1031	0.10%	0.013%
17	3.722	832	834	838	rVB5	1271	635	0.06%	0.008%
18	3.748	840	842	845	rVB3	1178	566	0.05%	0.007%
19	3.786	845	854	880	rBV3	55033	206191	19.80%	2.584%
20	4.249	984	998	1023	rBV	166569	424343	40.75%	5.318%
21	4.606	1107	1109	1111	rVB2	1113	510	0.05%	0.006%
22	4.715	1138	1143	1145	rBV4	2037	1609	0.15%	0.020%
23	4.805	1169	1171	1174	rVB4	1344	697	0.07%	0.009%
24	4.828	1174	1178	1179	rBV3	1025	753	0.07%	0.009%
25	4.956	1202	1218	1246	rBV2	385373	1041224	100.00%	13.049%
26	5.535	1386	1398	1429	rBV	310242	656720	63.07%	8.230%
27	5.989	1526	1539	1558	rBV	229553	479612	46.06%	6.011%
28	6.268	1623	1626	1628	rBV4	993	776	0.07%	0.010%
29	6.436	1676	1678	1684	rBV5	1181	1272	0.12%	0.016%
30	6.535	1706	1709	1710	rBV2	1010	583	0.06%	0.007%
31	6.657	1740	1747	1750	rBV8	1103	1201	0.12%	0.015%
32	6.915	1816	1827	1850	rBV2	104682	206611	19.84%	2.589%
33	7.243	1917	1929	1951	rBV	422224	763434	73.32%	9.568%
34	7.554	2016	2026	2051	rBV	79154	148406	14.25%	1.860%
35	7.770	2091	2093	2096	rVB4	1821	1107	0.11%	0.014%
36	7.789	2096	2099	2101	rBV4	2024	1474	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121923\
 Data File : VW033492.D
 Acq On : 19 Dec 2023 20:46
 Operator : SY/MD
 Sample : 05912-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.857	2116	2120	2123	rBV6	1376	1204	0.12%	0.015%
38	8.024	2163	2172	2208	rBV	163336	368654	35.41%	4.620%
39	8.651	2365	2367	2369	rVV2	1103	471	0.05%	0.006%
40	8.699	2377	2382	2385	rVB6	1096	1006	0.10%	0.013%
41	8.786	2395	2409	2436	rBV	521665	979845	94.11%	12.280%
42	9.149	2520	2522	2525	rBV4	1497	724	0.07%	0.009%
43	9.432	2607	2610	2613	rBV4	1469	1249	0.12%	0.016%
44	9.464	2616	2620	2622	rBV4	1149	930	0.09%	0.012%
45	9.599	2655	2662	2664	rBV7	1656	1879	0.18%	0.024%
46	9.689	2687	2690	2693	rVB6	1167	791	0.08%	0.010%
47	9.705	2693	2695	2698	rBV4	1178	923	0.09%	0.012%
48	9.821	2728	2731	2733	rVB4	1158	604	0.06%	0.008%
49	9.924	2761	2763	2767	rVB5	685	479	0.05%	0.006%
50	10.050	2800	2802	2806	rVB4	1181	543	0.05%	0.007%
51	10.104	2816	2819	2821	rBV4	987	574	0.06%	0.007%
52	10.152	2823	2834	2852	rVV	286517	461270	44.30%	5.781%
53	10.365	2897	2900	2902	rBV4	1068	562	0.05%	0.007%
54	10.458	2927	2929	2931	rVB3	1256	508	0.05%	0.006%
55	10.570	2961	2964	2967	rBV4	686	498	0.05%	0.006%
56	10.651	2987	2989	2993	rVB5	1784	1079	0.10%	0.014%
57	10.680	2993	2998	3000	rBV5	1483	1442	0.14%	0.018%
58	10.882	3059	3061	3063	rVB3	1561	733	0.07%	0.009%
59	11.008	3098	3100	3102	rBV3	1099	619	0.06%	0.008%
60	11.085	3119	3124	3126	rBV5	701	583	0.06%	0.007%
61	11.127	3132	3137	3138	rBV4	1723	1318	0.13%	0.017%
62	11.185	3144	3155	3181	rBV	463511	747898	71.83%	9.373%
63	11.345	3202	3205	3209	rBV6	1691	1465	0.14%	0.018%
64	11.381	3214	3216	3221	rVB6	1571	949	0.09%	0.012%
65	11.419	3225	3228	3229	rBV3	1020	539	0.05%	0.007%
66	11.561	3262	3272	3292	rVB	452068	719533	69.10%	9.017%
67	11.815	3348	3351	3353	rBV4	1468	879	0.08%	0.011%
68	11.953	3391	3394	3396	rBV3	1195	856	0.08%	0.011%
69	12.123	3444	3447	3448	rBV3	1043	568	0.05%	0.007%
70	12.152	3454	3456	3457	rBV2	1298	612	0.06%	0.008%
71	12.233	3479	3481	3486	rBV5	1027	778	0.07%	0.010%
72	12.284	3495	3497	3502	rVB5	1119	698	0.07%	0.009%
73	12.307	3502	3504	3507	rBV3	1175	810	0.08%	0.010%
74	12.438	3540	3545	3546	rBV5	798	630	0.06%	0.008%
75	12.477	3554	3557	3559	rBV4	1549	866	0.08%	0.011%
76	12.606	3594	3597	3599	rBV4	1029	793	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
 Data File : VV033492.D
 Acq On : 19 Dec 2023 20:46
 Operator : SY/MD
 Sample : 05912-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.644	3604	3609	3613	rVB5	1408	1039	0.10%	0.013%
78	12.734	3633	3637	3643	rVB4	1121	1188	0.11%	0.015%
79	12.828	3663	3666	3668	rBV4	780	595	0.06%	0.007%
80	13.220	3786	3788	3790	rVB3	1169	517	0.05%	0.006%
81	13.313	3815	3817	3820	rBV2	1155	575	0.06%	0.007%
82	13.352	3827	3829	3831	rBV2	1813	857	0.08%	0.011%
83	13.406	3840	3846	3849	rBV7	797	818	0.08%	0.010%
84	13.606	3905	3908	3912	rBV6	1465	1056	0.10%	0.013%
85	13.628	3912	3915	3918	rBV3	799	582	0.06%	0.007%
86	13.721	3940	3944	3947	rBV5	1372	1131	0.11%	0.014%
87	13.873	3989	3991	3994	rBV3	1366	894	0.09%	0.011%
88	13.921	4002	4006	4009	rBV5	1297	1116	0.11%	0.014%
89	13.979	4020	4024	4026	rBV4	908	764	0.07%	0.010%
90	14.046	4042	4045	4047	rBV4	960	512	0.05%	0.006%
91	14.088	4056	4058	4062	rVB5	1092	598	0.06%	0.007%
92	14.130	4067	4071	4074	rBV6	940	919	0.09%	0.012%
93	14.200	4090	4093	4097	rVB5	1321	1030	0.10%	0.013%
94	14.345	4136	4138	4140	rBV3	997	512	0.05%	0.006%
95	14.419	4157	4161	4162	rBV3	835	585	0.06%	0.007%
96	14.471	4175	4177	4181	rBV4	953	818	0.08%	0.010%
97	14.509	4186	4189	4192	rBV4	1108	644	0.06%	0.008%
98	14.737	4257	4260	4263	rBV4	1077	604	0.06%	0.008%
99	14.811	4281	4283	4285	rBV3	948	619	0.06%	0.008%
100	15.220	4408	4410	4412	rBV2	1188	588	0.06%	0.007%




Sum of corrected areas: 7979391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033492.D
Acq On : 19 Dec 2023 20:46
Operator : SY/MD
Sample : 05912-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

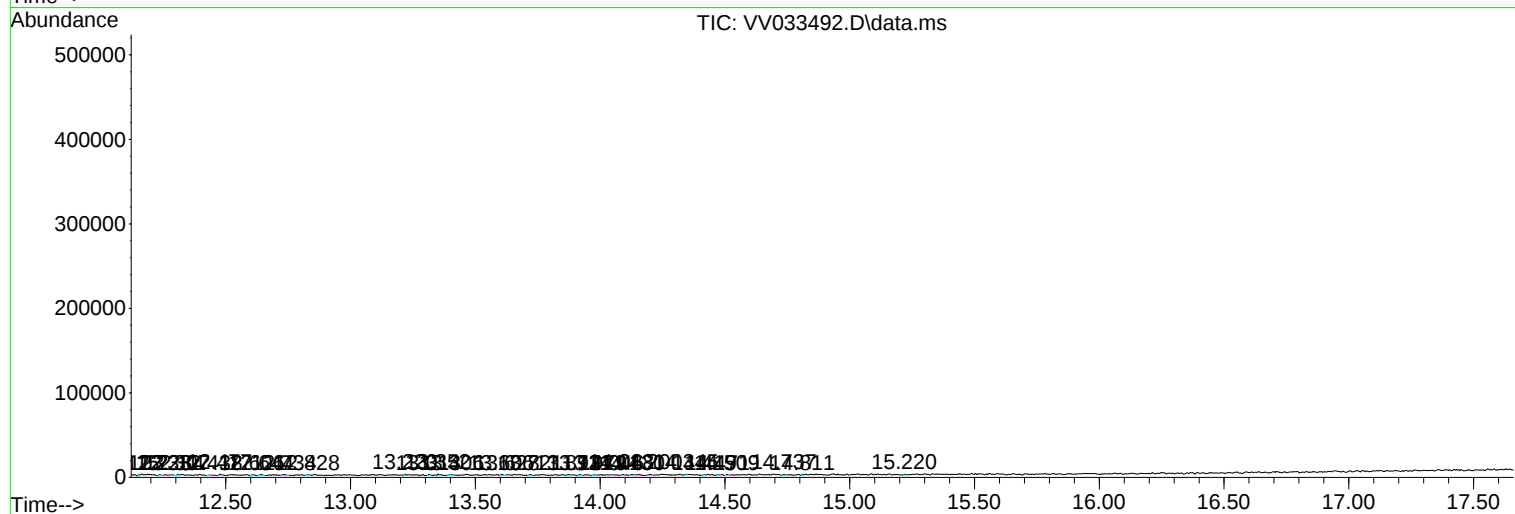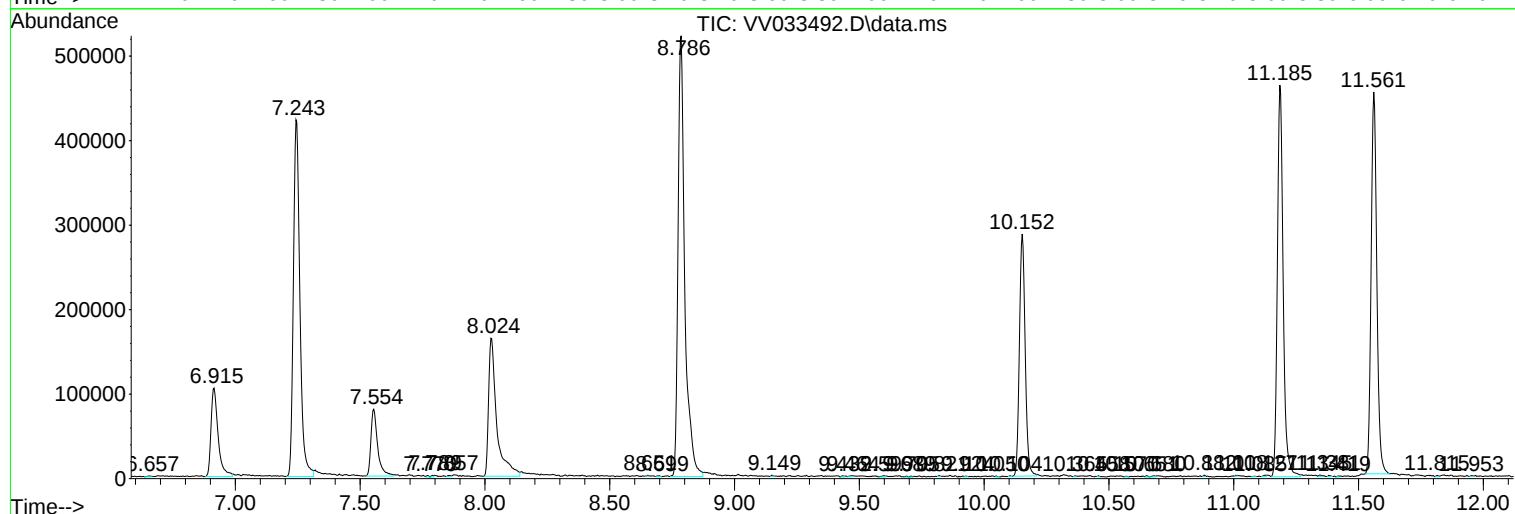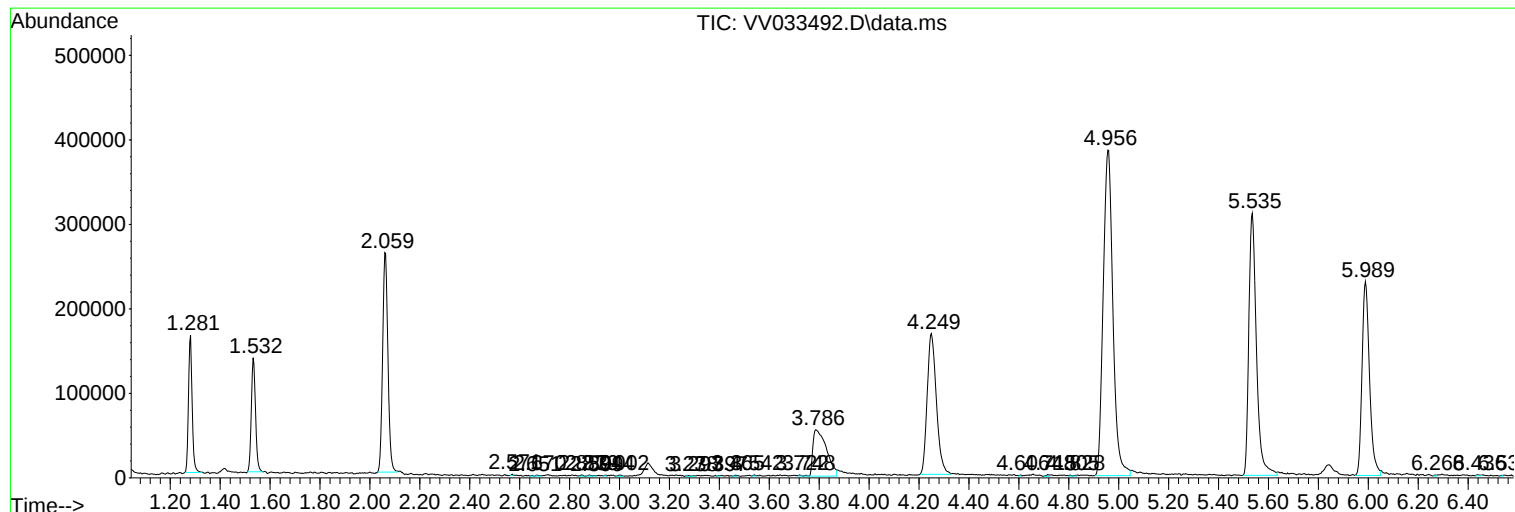

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033492.D
Acq On : 19 Dec 2023 20:46
Operator : SY/MD
Sample : 05912-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033492.D
Acq On : 19 Dec 2023 20:46
Operator : SY/MD
Sample : 05912-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3N2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------