


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121923\
Data File : VV033468.D
Acq On : 19 Dec 2023 10:38
Operator : SY/MD
Sample : BFB249
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB249

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis
Last Update : Wed Dec 20 00:24:21 2023

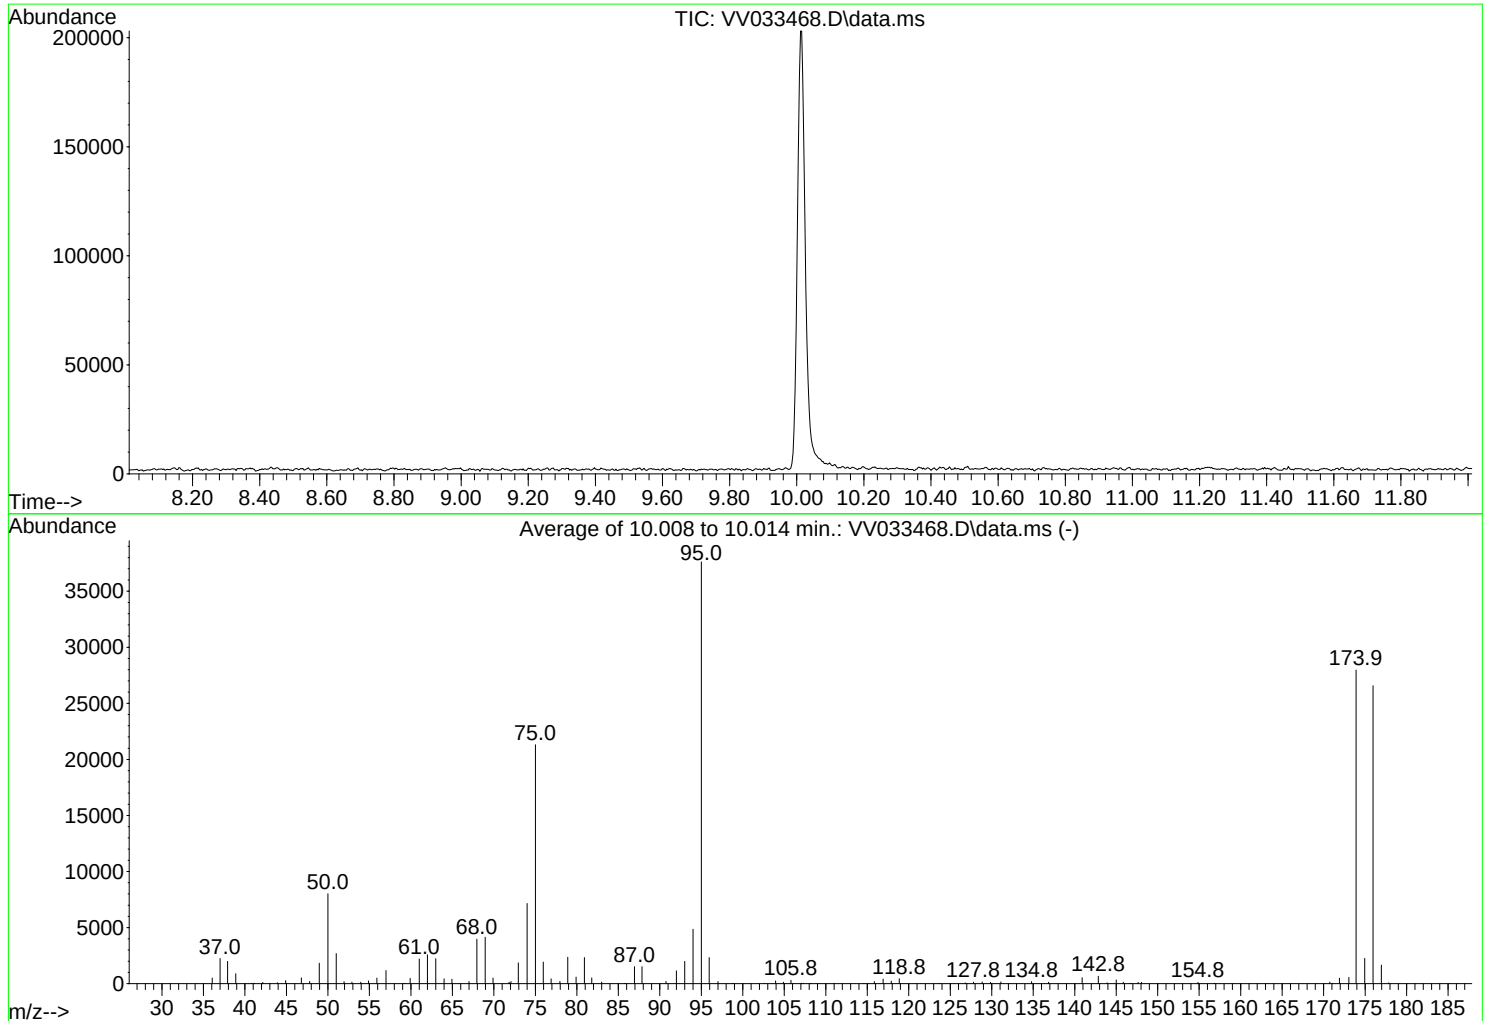

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	8018	PASS
75	95	30	80	56.6	21304	PASS
95	95	100	100	100.0	37621	PASS
96	95	5	9	6.2	2333	PASS
173	174	0.00	2	2.0	551	PASS
174	95	50	120	74.4	27976	PASS
175	174	5	9	8.1	2262	PASS
176	174	95	105	95.0	26579	PASS
177	176	5	10	6.2	1653	PASS

m/z	Abundance
35.60	138.0
37.10	118.0
38.20	131.0
38.80	116.0
39.90	261.0
43.90	479.0
44.90	121.0
46.50	104.0
46.80	111.0
47.80	117.0
56.00	110.0
57.90	130.0
68.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249

m/z	Abundance
36.00	497.0
37.00	2261.0
37.90	1890.0
38.90	896.0
39.70	251.0
41.10	130.0
42.20	106.0
44.00	545.0
45.00	310.0
46.90	649.0
47.80	308.0
49.00	1660.0
50.00	7593.0
51.00	2561.0
51.90	156.0
52.90	125.0
54.00	124.0
54.90	253.0
55.90	548.0
57.00	1097.0
57.80	107.0
59.90	434.0
61.00	1900.0
62.00	2541.0
63.00	2161.0
64.00	399.0
64.90	388.0
67.00	174.0
67.90	3690.0
69.00	4017.0
69.90	520.0
72.10	301.0
73.00	1821.0
74.00	6752.0
75.00	20120.0
76.00	1895.0
76.90	370.0
77.90	204.0
78.90	2308.0
79.90	558.0
80.90	2153.0
81.80	476.0
83.10	136.0
85.80	103.0
87.00	1412.0
87.90	1307.0
90.80	213.0
92.00	1138.0
93.00	1763.0
94.00	4713.0
95.00	35144.0
96.00	2341.0
97.00	207.0
104.00	228.0
104.90	135.0
105.80	295.0
107.10	115.0
115.80	188.0
116.90	379.0
117.90	187.0
118.90	425.0
126.80	116.0
127.80	122.0
128.80	125.0
129.90	107.0
131.10	134.0
134.80	193.0
136.80	159.0
140.90	532.0
142.90	507.0
145.00	261.0
145.80	112.0
147.60	143.0
148.10	104.0
170.70	141.0
171.10	105.0
171.90	422.0
173.10	544.0
173.90	25704.0
175.00	2034.0
175.90	23688.0
177.00	1435.0
177.90	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249

m/z	Abundance
36.10	506.0
37.00	2449.0
37.90	2050.0
39.00	1022.0
39.70	256.0
40.80	104.0
42.20	122.0
44.00	571.0
45.00	414.0
46.80	638.0
47.80	312.0
49.00	1878.0
50.00	8367.0
51.00	2804.0
52.00	197.0
52.90	131.0
53.90	127.0
54.90	244.0
55.90	611.0
57.00	1201.0
57.80	108.0
59.90	484.0
61.00	2258.0
62.00	2679.0
63.00	2336.0
64.00	428.0
64.90	397.0
67.00	211.0
68.00	4094.0
69.00	4387.0
69.90	517.0
71.80	275.0
72.00	279.0
73.00	1878.0
74.00	7377.0
75.00	21856.0
76.00	2016.0
76.90	465.0
77.90	201.0
78.90	2446.0
79.90	598.0
80.90	2421.0
81.80	519.0
83.00	140.0
87.00	1525.0
87.90	1552.0
90.70	189.0
92.00	1134.0
93.00	2068.0
94.00	5059.0
95.00	39096.0
95.90	2397.0
97.00	192.0
98.80	103.0
103.90	246.0
104.90	142.0
105.80	309.0
107.30	104.0
111.00	109.0
115.90	177.0
116.90	451.0
117.90	231.0
118.80	463.0
126.80	111.0
127.80	153.0
128.80	169.0
129.80	110.0
131.10	168.0
134.80	204.0
136.90	139.0
140.90	556.0
142.90	682.0
143.90	107.0
145.00	353.0
145.90	134.0
147.60	115.0
148.10	117.0
154.90	156.0
170.70	136.0
171.90	482.0
173.00	574.0
173.90	28976.0
175.00	2352.0
175.90	27528.0
176.90	1723.0
177.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249

m/z	Abundance
36.00	496.0
37.00	2362.0
37.90	2024.0
39.00	1077.0
39.80	238.0
42.10	126.0
43.00	109.0
43.90	587.0
44.90	464.0
46.80	598.0
47.80	318.0
48.90	1954.0
50.00	8095.0
51.00	2672.0
51.90	218.0
52.90	134.0
53.90	131.0
54.90	256.0
55.90	656.0
57.00	1208.0
57.80	107.0
59.20	100.0
59.90	483.0
61.00	2427.0
62.00	2488.0
63.00	2199.0
64.00	454.0
65.00	418.0
67.00	192.0
68.00	4137.0
69.00	4313.0
69.90	463.0
71.90	277.0
72.90	1883.0
74.00	7334.0
75.00	21936.0
75.90	1886.0
76.90	464.0
78.00	201.0
78.90	2302.0
79.90	597.0
80.90	2405.0
81.80	531.0
82.90	144.0
86.90	1595.0
87.80	1671.0
90.70	183.0
92.00	1148.0
93.00	2128.0
94.00	4777.0
95.00	38624.0
95.90	2261.0
97.00	153.0
102.60	104.0
103.90	256.0
104.90	132.0
105.80	299.0
108.20	110.0
114.60	104.0
115.90	176.0
116.90	407.0
117.90	247.0
118.80	425.0
123.70	103.0
127.80	141.0
128.90	162.0
129.80	146.0
131.10	154.0
134.80	171.0
136.90	105.0
140.90	489.0
142.80	795.0
143.90	102.0
145.00	390.0
145.90	139.0
146.70	105.0
147.70	105.0
148.00	103.0
154.80	195.0
156.80	135.0
170.80	159.0
171.90	546.0
173.00	536.0
173.90	29248.0
174.90	2399.0
176.00	28520.0
176.90	1801.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249