

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_V\DATA\VV122018\  
 Data File : VV009089.D  
 Acq On : 20 Dec 2018 17:26  
 Operator : SY/MD  
 Sample : J6471-05RE  
 Misc : 5.13 G/10ML/MSVOA\_V/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 F9H14RE

Quant Time: Dec 21 01:10:17 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOM2VLM120618S.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Dec 21 00:25:26 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Difluorobenzene     | 5.67  | 114  | 198132   | 25.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 8.90  | 117  | 148991   | 25.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.30 | 152  | 47613    | 25.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |        |       |          |          |      |         |
|--------------------------------|--------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.31   | 65    | 44792    | 21.85    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 30 - 150 | Recovery | =    | 87.40%  |
| 7) Chloroethane-d5             | 1.58   | 69    | 46575    | 30.75    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 30 - 150 | Recovery | =    | 123.00% |
| 10) 1,1-Dichloroethene-d2      | 2.13   | 63    | 85631    | 16.70    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 45 - 110 | Recovery | =    | 66.80%  |
| 20) 2-Butanone-d5              | 3.94   | 46    | 20169    | 27.02    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 20 - 135 | Recovery | =    | 54.04%  |
| 24) Chloroform-d               | 4.40   | 84    | 116955   | 24.55    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 40 - 150 | Recovery | =    | 98.20%  |
| 26) 1,2-Dichloroethane-d4      | 5.08   | 65    | 68159    | 26.22    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 70 - 130 | Recovery | =    | 104.88% |
| 29) Benzene-d6                 | 5.10   | 84    | 224602   | 26.99    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 20 - 135 | Recovery | =    | 107.96% |
| 33) 1,2-Dichloropropane-d6     | 6.12   | 67    | 69805    | 29.96    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 70 - 120 | Recovery | =    | 119.84% |
| 37) Toluene-d8                 | 7.36   | 98    | 185836   | 24.13    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 30 - 130 | Recovery | =    | 96.52%  |
| 38) trans-1,3-Dichloropropene- | 7.66   | 79    | 22307    | 21.79    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 30 - 135 | Recovery | =    | 87.16%  |
| 39) 2-Hexanone-d5              | 8.14   | 63    | 13242    | 31.03    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 20 - 135 | Recovery | =    | 62.06%  |
| 48) 1,1,2,2-Tetrachloroethane- | 10.26  | 84    | 43995    | 22.51    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 45 - 120 | Recovery | =    | 90.04%  |
| 61) 1,2-Dichlorobenzene-d4     | 11.68  | 152   | 40043    | 22.41    | ug/L | 0.00    |
| Spiked Amount                  | 25.000 | Range | 75 - 120 | Recovery | =    | 89.64%  |


| Target Compounds       |      |    |       |            | Qvalue |
|------------------------|------|----|-------|------------|--------|
| 16) Methylene chloride | 2.53 | 84 | 10431 | 3.126 ug/L | 96     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_V\DATA\VV122018\  
Data File : VV009089.D  
Acq On : 20 Dec 2018 17:26  
Operator : SY/MD  
Sample : J6471-05RE  
Misc : 5.13 G/10ML/MSVOA\_V/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
F9H14RE

Quant Time: Dec 21 01:10:17 2018  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_V\METHOD\SOM2VLM120618S.M  
Quant Title : VOC Analysis  
QLast Update : Fri Dec 21 00:25:26 2018  
Response via : Initial Calibration

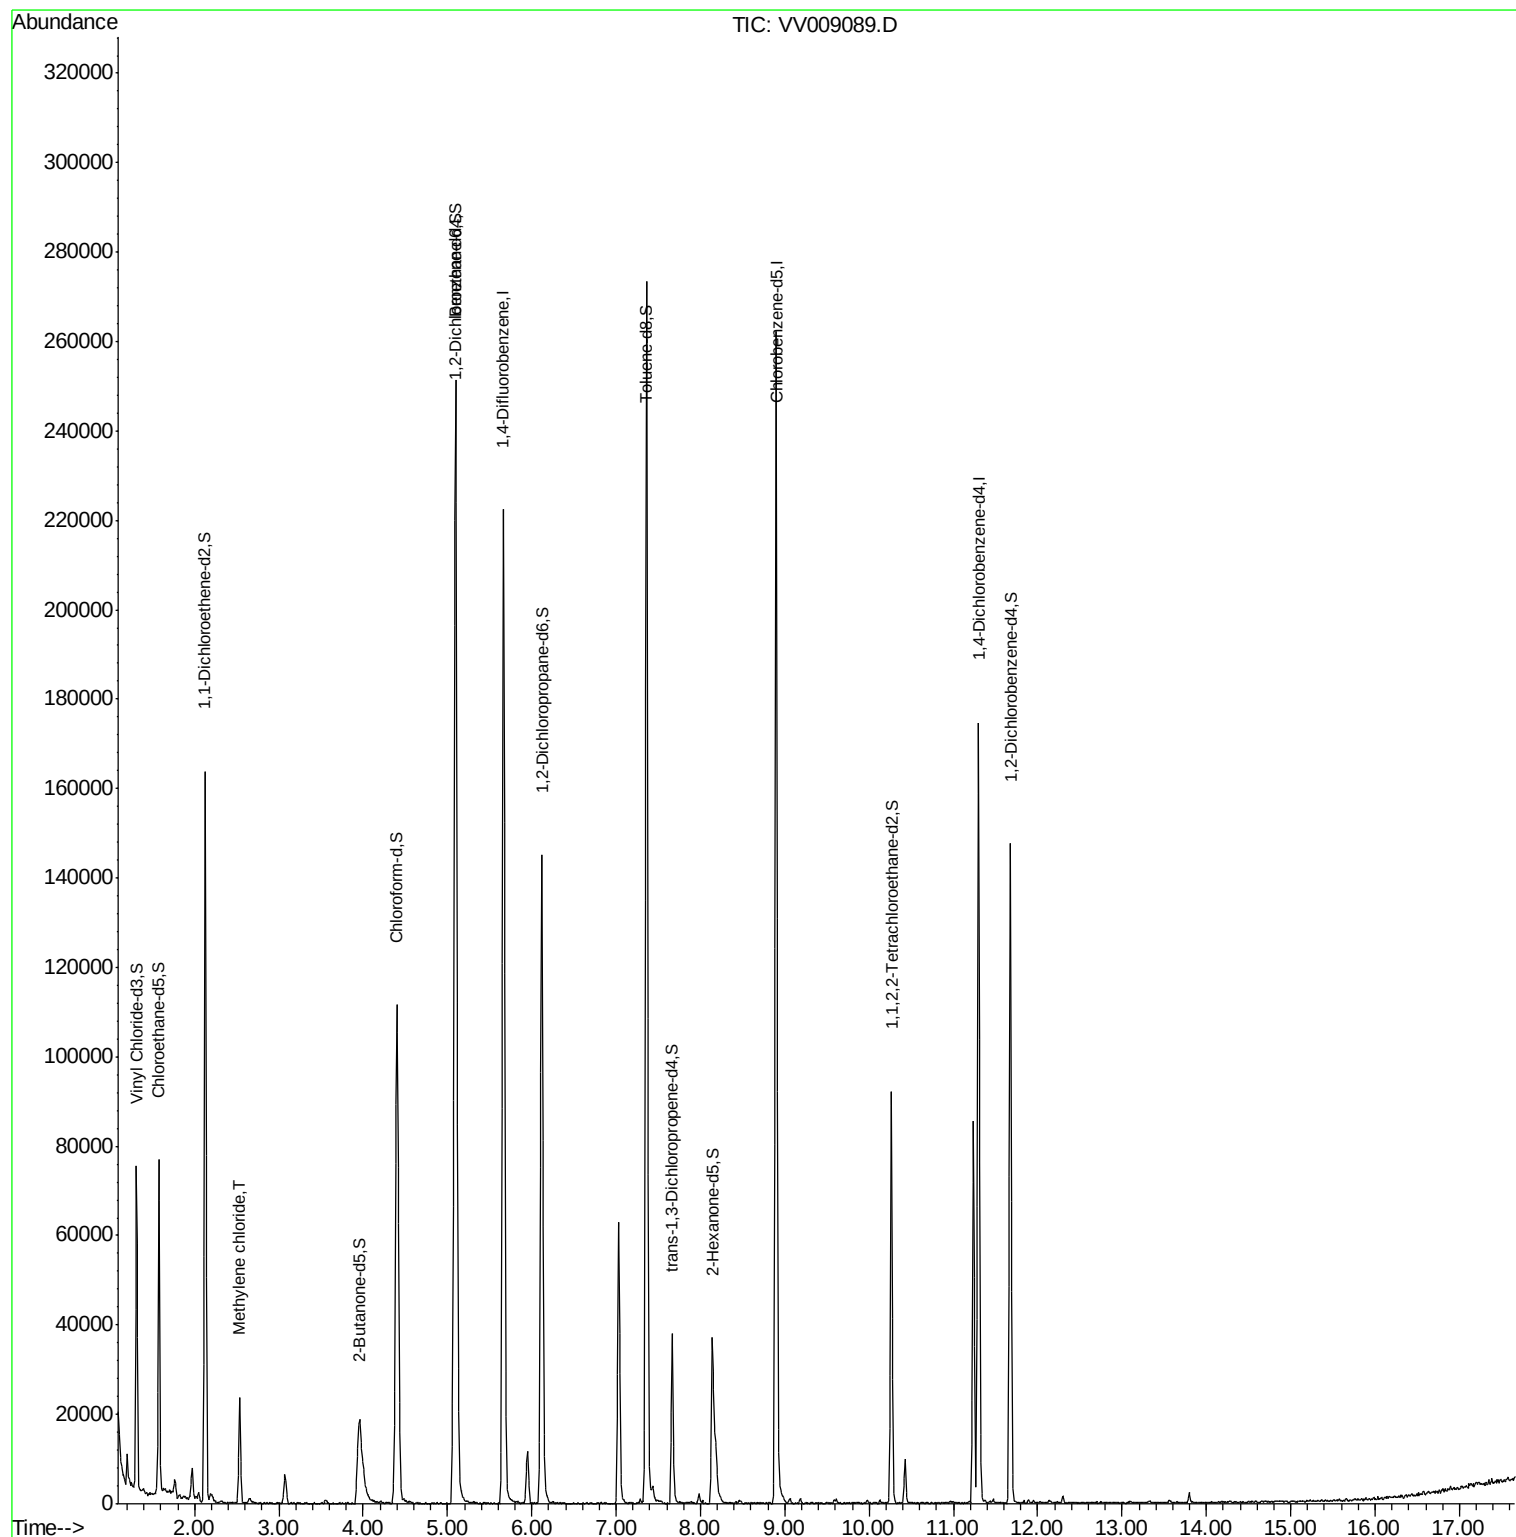

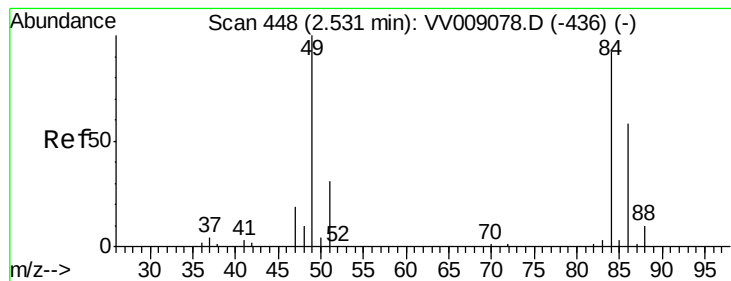

#16  
Methylene chloride  
Concen: 3.126 ug/L  
RT: 2.53 min Scan# 449  
Delta R.T. 0.00 min  
Lab File: VV009089.D  
Acq: 20 Dec 2018 17:26

Instrument :  
MSVOA\_V  
ClientSampleId :  
F9H14RE

Tgt Ion: 84 Resp: 10431  
Ion Ratio Lower Upper  
84 100  
49 108.5 80.5 149.5  
86 64.5 45.5 84.5

