


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122018\
Data File : VV009077.D
Acq On : 20 Dec 2018 09:42
Operator : SY/MD
Sample : BFB64
Misc : 5.00 G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Title : VOC Analysis
Last Update : Fri Dec 21 01:30:11 2018

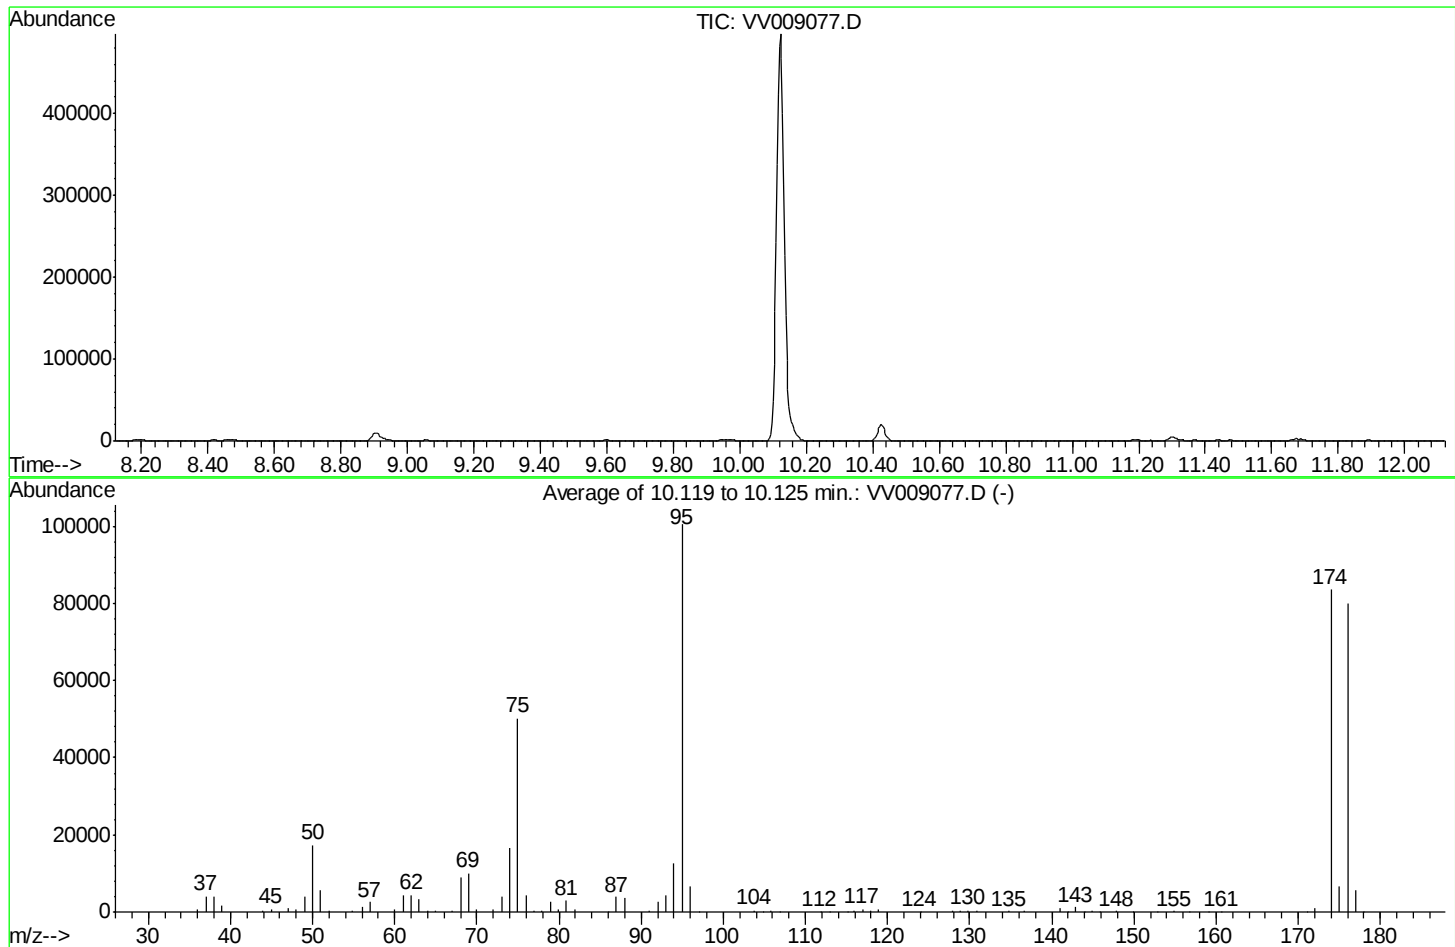

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	17282	PASS
75	95	30	80	50.0	50250	PASS
95	95	100	100	100.0	100461	PASS
96	95	5	9	6.7	6734	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.1	83437	PASS
175	174	5	9	8.0	6639	PASS
176	174	95	101	95.7	79829	PASS
177	176	5	9	7.0	5568	PASS

m/z	Abundance
43.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	698.0
37.00	3933.0
38.00	3861.0
39.00	1450.0
44.00	566.0
45.00	723.0
47.00	884.0
47.90	505.0
49.00	3688.0
50.00	16327.0
51.00	5170.0
52.00	250.0
54.80	274.0
56.00	1272.0
57.00	2521.0
59.90	723.0
61.00	4133.0
62.00	4075.0
63.00	3082.0
63.90	306.0
65.00	339.0
66.90	349.0
68.00	8874.0
69.00	9412.0
70.00	798.0
72.00	476.0
73.00	3681.0
74.00	15886.0
75.00	48184.0
76.00	4117.0
77.00	479.0
78.00	442.0
78.90	2498.0
79.90	786.0
80.90	2694.0
81.90	523.0
87.00	3732.0
88.00	3772.0
90.90	404.0
92.00	2786.0
93.00	4247.0
94.00	12187.0
95.00	96672.0
96.00	6603.0
103.80	451.0
104.90	106.0
105.80	421.0
106.90	101.0
111.80	111.0
112.90	117.0
115.00	103.0
116.00	411.0
116.90	629.0
117.90	493.0
118.90	606.0
124.00	102.0
128.00	300.0
128.80	180.0
129.80	329.0
130.90	216.0
134.80	172.0
136.70	149.0
141.00	924.0
141.90	166.0
142.90	1187.0
144.90	199.0
145.80	114.0
148.00	257.0
149.90	125.0
152.90	150.0
154.90	237.0
156.70	125.0
171.00	110.0
172.00	812.0
174.00	82328.0
175.00	6601.0
176.00	79144.0
177.00	5486.0
177.90	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	820.0
37.00	4215.0
38.00	4228.0
39.00	1589.0
43.90	579.0
45.00	753.0
47.00	923.0
47.90	531.0
49.00	4224.0
50.00	17840.0
51.00	5708.0
52.00	322.0
54.90	305.0
56.00	1368.0
57.00	2578.0
60.00	842.0
61.00	4436.0
62.00	4484.0
63.00	3326.0
64.00	370.0
65.00	360.0
66.90	368.0
68.00	9313.0
69.00	10459.0
70.00	861.0
72.00	539.0
73.00	4209.0
74.00	16856.0
75.00	52016.0
76.00	4305.0
77.00	495.0
78.00	402.0
78.90	2735.0
80.00	842.0
80.90	3023.0
81.90	540.0
86.10	116.0
87.00	3979.0
88.00	3903.0
90.90	427.0
92.00	2897.0
93.00	4392.0
94.00	13050.0
95.00	103584.0
96.00	6881.0
97.00	116.0
103.80	450.0
104.90	117.0
105.90	431.0
106.90	107.0
111.80	126.0
112.90	105.0
115.10	124.0
115.90	453.0
116.90	721.0
117.90	509.0
118.90	707.0
128.00	327.0
128.90	183.0
129.80	362.0
130.80	204.0
134.80	203.0
136.70	199.0
141.00	1023.0
141.90	158.0
142.90	1288.0
144.90	228.0
145.80	124.0
147.90	245.0
149.90	123.0
152.90	136.0
154.90	222.0
156.70	136.0
159.00	111.0
172.00	866.0
174.00	86240.0
175.00	6889.0
176.00	82040.0
177.00	5768.0
177.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	795.0
37.00	4245.0
38.00	4087.0
39.00	1551.0
43.90	592.0
45.00	692.0
47.10	966.0
48.00	526.0
49.00	4289.0
50.00	17680.0
51.00	5596.0
52.00	314.0
54.90	249.0
56.00	1403.0
57.00	2410.0
60.00	874.0
61.00	4434.0
62.00	4631.0
63.00	3403.0
64.00	377.0
65.00	361.0
66.90	334.0
68.00	9190.0
69.00	10318.0
70.00	817.0
71.90	527.0
73.00	4440.0
74.00	16608.0
75.00	50552.0
76.00	4185.0
76.90	514.0
77.90	337.0
78.90	2738.0
80.00	799.0
80.90	3099.0
81.90	552.0
86.00	129.0
86.90	3813.0
88.00	3590.0
90.90	402.0
92.00	2801.0
93.00	4171.0
94.00	12339.0
95.00	101128.0
96.00	6720.0
97.00	140.0
103.80	428.0
104.80	136.0
105.90	428.0
115.10	110.0
115.90	446.0
117.00	747.0
118.00	474.0
118.90	649.0
127.90	358.0
129.00	189.0
129.80	367.0
130.80	210.0
134.80	199.0
136.70	222.0
141.00	1010.0
142.10	141.0
142.90	1323.0
143.90	104.0
144.90	241.0
145.80	118.0
147.80	244.0
152.80	124.0
154.90	213.0
156.80	138.0
159.00	103.0
160.70	124.0
171.00	130.0
172.00	848.0
174.00	81744.0
175.00	6428.0
176.00	78304.0
177.00	5451.0
177.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64