

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029746.D
 Acq On : 20 Dec 2022 13:13
 Operator : SY/MD
 Sample : N6130-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXGJ0

Quant Time: Dec 21 00:17:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	438505	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	412287	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	206732	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	108500	40.406	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.820%
7) Chloroethane-d5	1.564	69	94957	46.376	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.760%
11) 1,1-Dichloroethene-d2	2.105	63	148095	35.360	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.720%
21) 2-Butanone-d5	3.876	46	139636	85.245	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.240%
24) Chloroform-d	4.336	84	209198	41.400	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.800%
26) 1,2-Dichloroethane-d4	5.024	65	126219	43.735	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.480%
32) Benzene-d6	5.043	84	441812	40.555	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.120%
36) 1,2-Dichloropropane-d6	6.063	67	141908	42.646	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.300%
41) Toluene-d8	7.307	98	387890	37.789	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.580%#
43) trans-1,3-Dichloroprop...	7.612	79	58602	34.875	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.760%
47) 2-Hexanone-d5	8.085	63	110532	77.786	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.790%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	200679	42.202	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.400%
66) 1,2-Dichlorobenzene-d4	11.612	152	159501	40.530	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.060%
Target Compounds						
					Qvalue	
13) Acetone	2.166	43	8738	8.188	ug/L	92
61) 1,2,3-Trichloropropane	11.236	75	23131	7.249	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029746.D
Acq On : 20 Dec 2022 13:13
Operator : SY/MD
Sample : N6130-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXGJ0

Quant Time: Dec 21 00:17:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

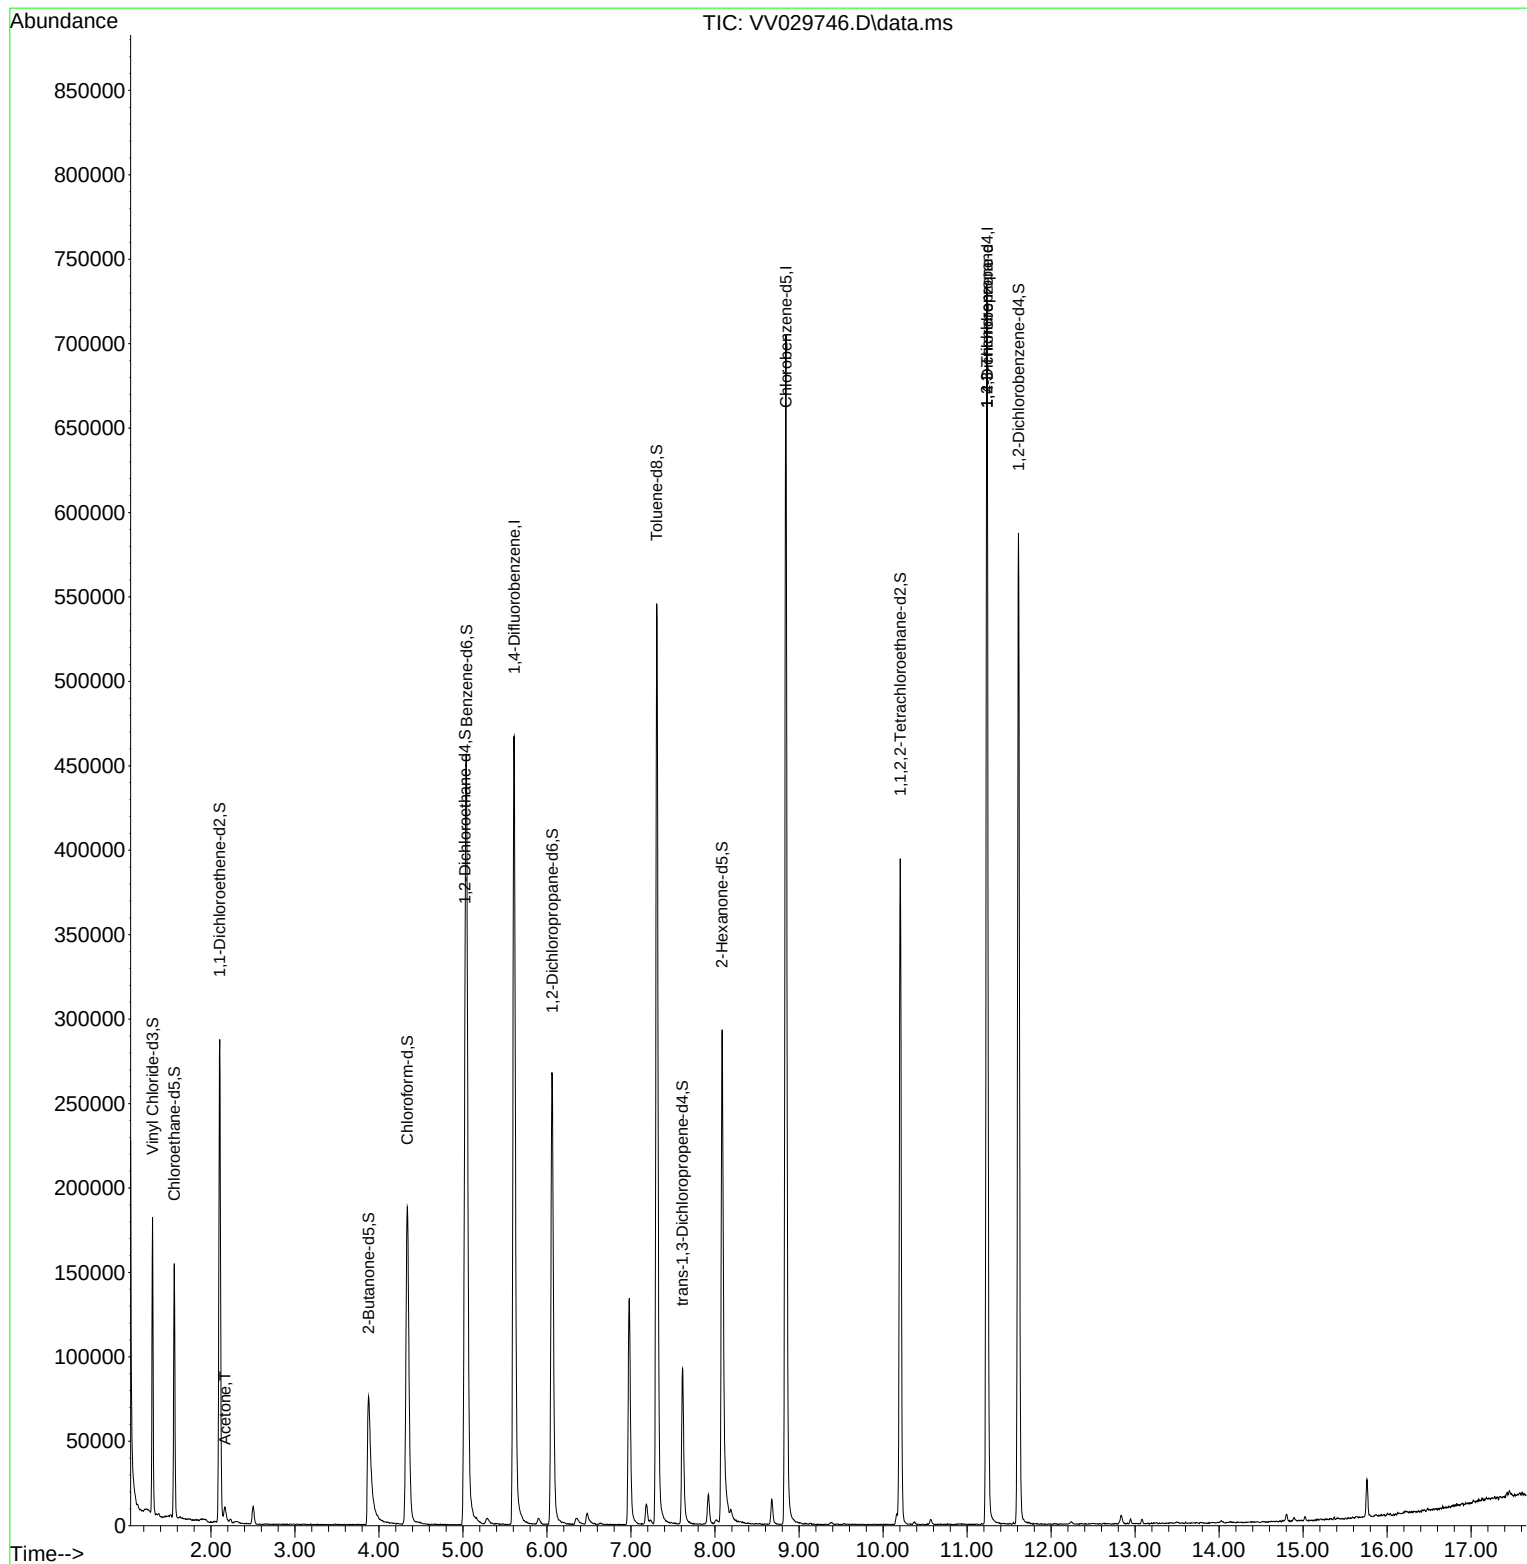

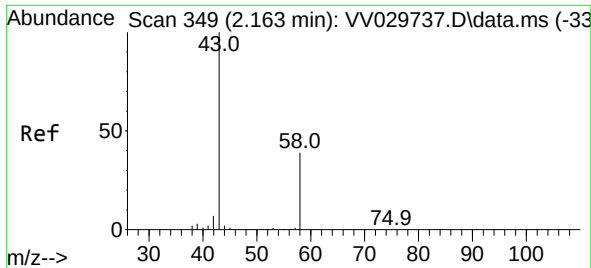

#13

Acetone

Concen: 8.188 ug/L

RT: 2.166 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV029746.D

Acq: 20 Dec 2022 13:13

Instrument :

MSVOA_V

ClientSampleId :





EXGJ0

Tgt Ion: 43 Resp: 8738

Ion Ratio Lower Upper

43 100

58 42.2 0.0 74.8

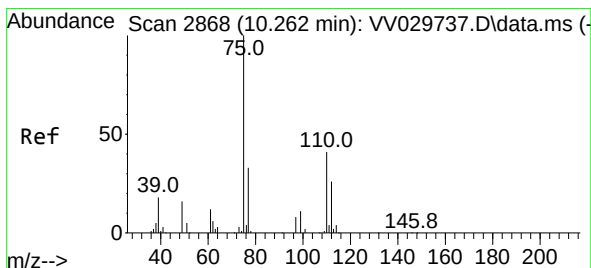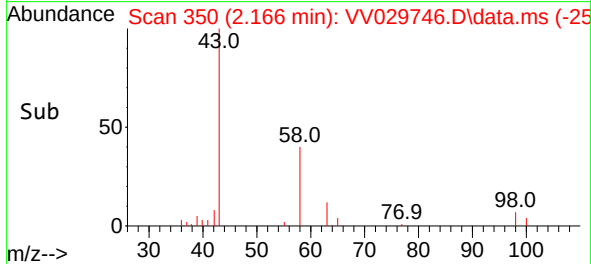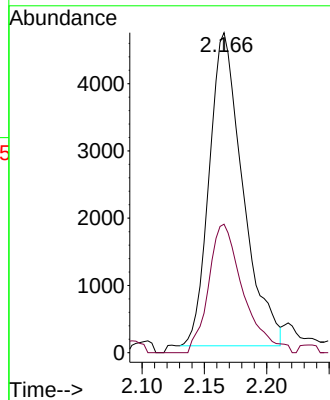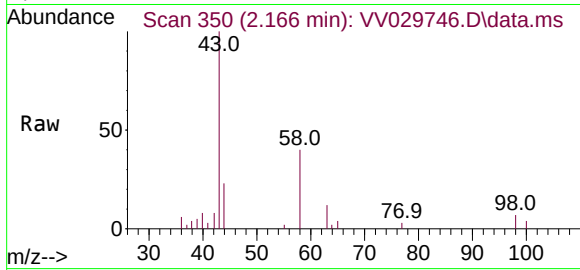

#61

1,2,3-Trichloropropane

Concen: 7.249 ug/L

RT: 11.236 min Scan# 3171

Delta R.T. 0.974 min

Lab File: VV029746.D

Acq: 20 Dec 2022 13:13

Tgt Ion: 75 Resp: 23131

Ion Ratio Lower Upper

75 100

77 31.5 25.4 38.2

110 2.6 32.7 49.1

