

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029747.D
 Acq On : 20 Dec 2022 13:36
 Operator : SY/MD
 Sample : N6133-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXGJ1

Quant Time: Dec 21 00:17:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	498795	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	471723	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	240134	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	125846	41.201	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.400%
7) Chloroethane-d5	1.564	69	110863	47.600	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.200%
11) 1,1-Dichloroethene-d2	2.105	63	169843	35.651	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.300%
21) 2-Butanone-d5	3.876	46	166861	89.553	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.550%
24) Chloroform-d	4.339	84	241256	41.973	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.940%
26) 1,2-Dichloroethane-d4	5.024	65	145961	44.463	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.920%
32) Benzene-d6	5.043	84	514225	41.255	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.520%
36) 1,2-Dichloropropane-d6	6.063	67	165184	43.386	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.780%
41) Toluene-d8	7.307	98	447182	38.076	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.160%#
43) trans-1,3-Dichloroprop...	7.612	79	68142	35.443	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.880%
47) 2-Hexanone-d5	8.085	63	136437	83.919	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.920%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	232390	42.714	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.420%
66) 1,2-Dichlorobenzene-d4	11.612	152	185107	40.494	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.980%
Target Compounds						
13) Acetone	2.172	43	3687	3.038	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029747.D
Acq On : 20 Dec 2022 13:36
Operator : SY/MD
Sample : N6133-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXGJ1

Quant Time: Dec 21 00:17:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

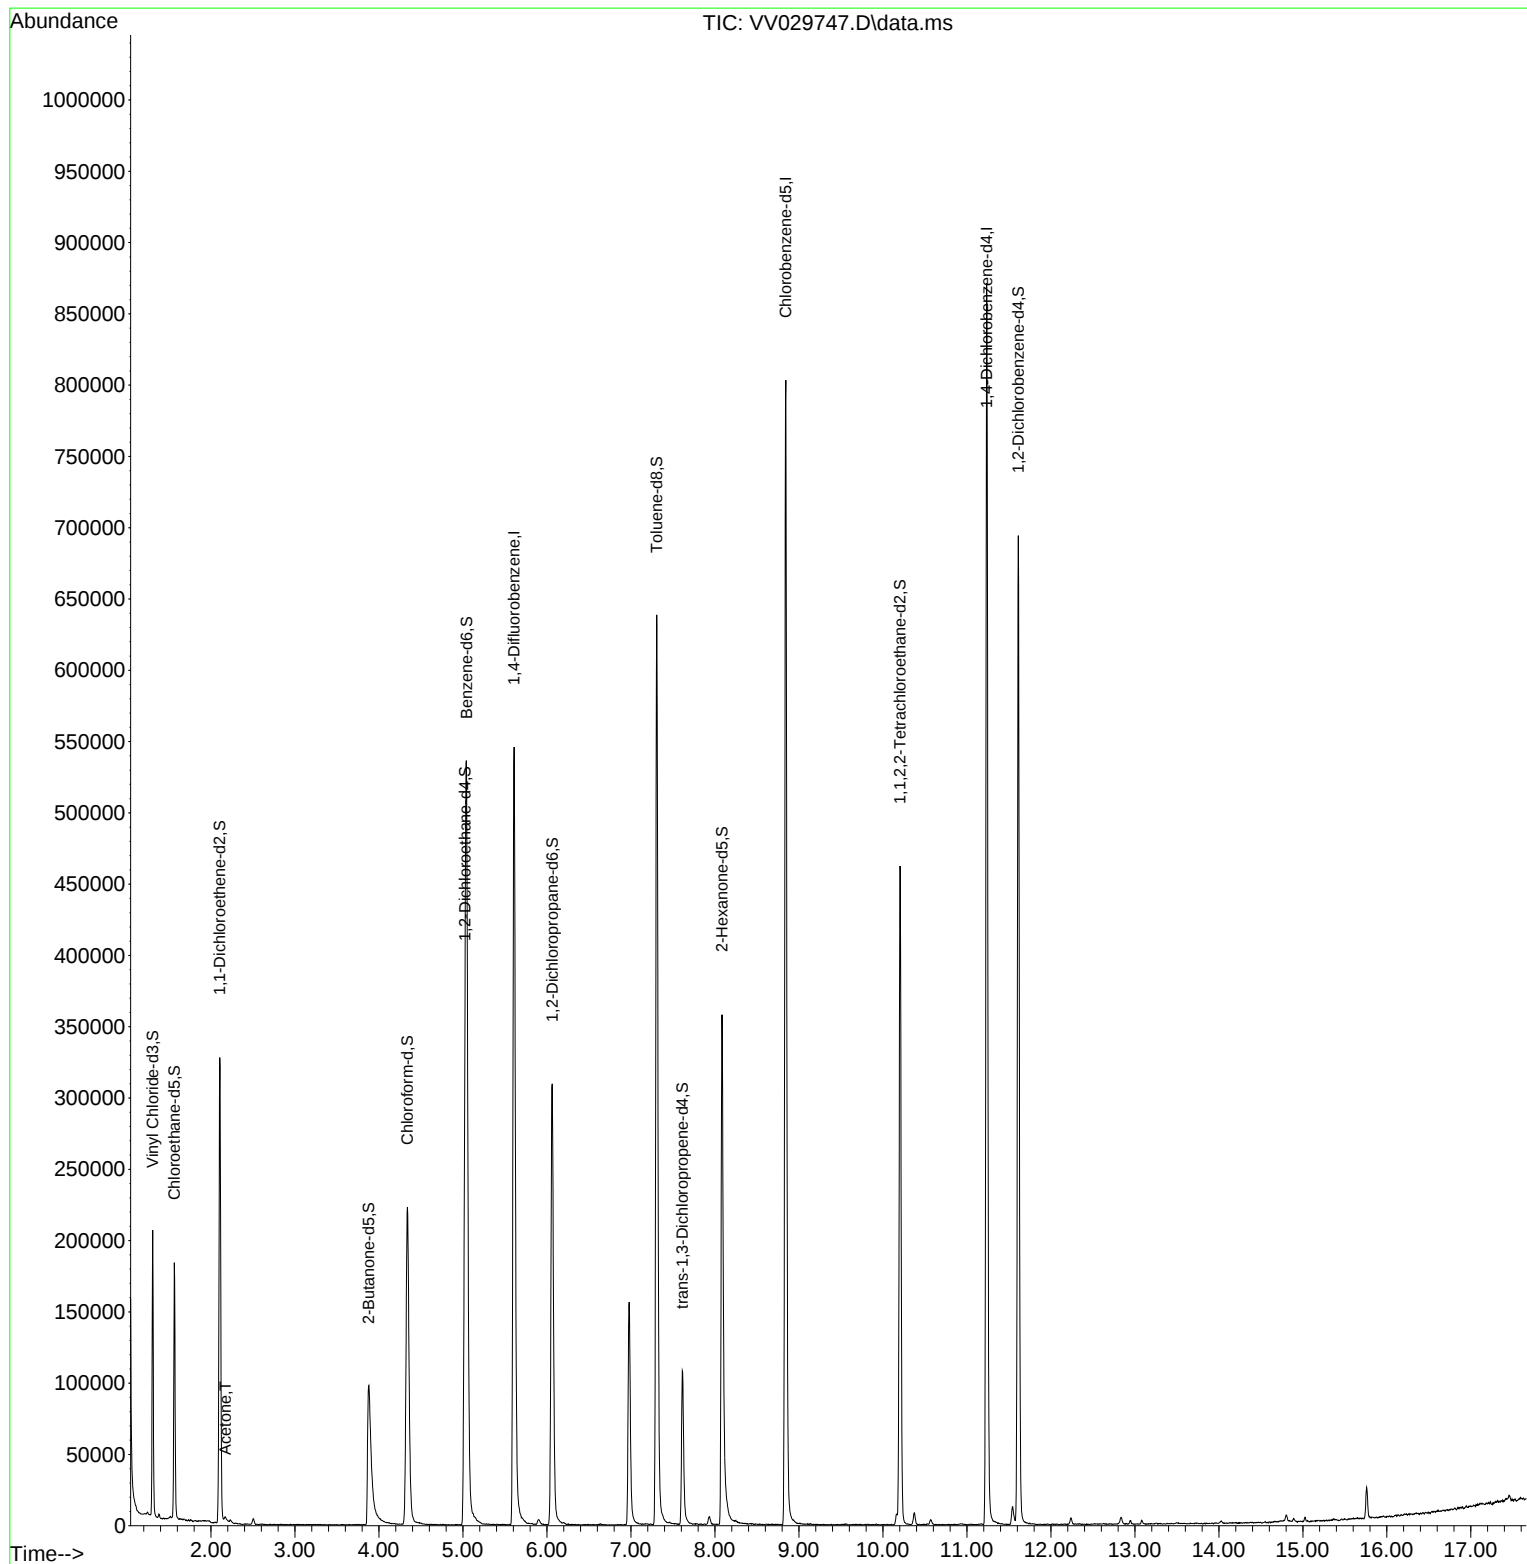

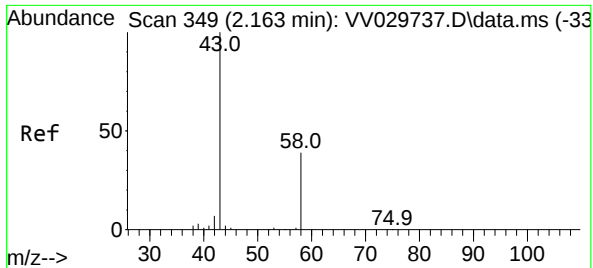

#13
 Acetone
 Concen: 3.038 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. 0.010 min
 Lab File: VV029747.D
 Acq: 20 Dec 2022 13:36

Instrument :
 MSVOA_V
 ClientSampleId :
 EXGJ1

Tgt Ion: 43 Resp: 3687
 Ion Ratio Lower Upper
 43 100
 58 30.1 0.0 74.8

