

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029738.D
 Acq On : 20 Dec 2022 09:51
 Operator : SY/MD
 Sample : VV1220WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	237986	233678	14.98%	1.901%
2	1.561	155	162	176	rVB	204079	226536	14.52%	1.843%
3	2.101	320	330	346	rBV	376913	541659	34.72%	4.407%
4	2.500	445	454	468	rVB2	18257	30053	1.93%	0.244%
5	2.587	478	481	483	rBV2	273	214	0.01%	0.002%
6	2.867	566	568	572	rVB2	303	165	0.01%	0.001%
7	2.902	577	579	582	rBV	210	157	0.01%	0.001%
8	3.149	653	656	659	rBV2	261	160	0.01%	0.001%
9	3.185	666	667	668	rBV	245	70	0.00%	0.001%
10	3.252	684	688	689	rBV2	206	127	0.01%	0.001%
11	3.442	745	747	749	rBV	234	104	0.01%	0.001%
12	3.535	774	776	779	rVB	285	112	0.01%	0.001%
13	3.584	789	791	796	rVB2	241	138	0.01%	0.001%
14	3.693	822	825	827	rBV	202	125	0.01%	0.001%
15	3.712	827	831	836	rVV2	195	206	0.01%	0.002%
16	3.870	870	880	918	rBV	108863	333349	21.37%	2.712%
17	4.333	1009	1024	1059	rBV	237426	590561	37.85%	4.804%
18	4.635	1116	1118	1120	rBV	237	122	0.01%	0.001%
19	4.680	1130	1132	1134	rVB2	321	100	0.01%	0.001%
20	4.751	1149	1154	1158	rBV2	315	325	0.02%	0.003%
21	4.834	1178	1180	1185	rVB2	199	143	0.01%	0.001%
22	4.863	1185	1189	1191	rBV2	196	102	0.01%	0.001%
23	4.892	1194	1198	1200	rBV	118	97	0.01%	0.001%
24	4.921	1204	1207	1208	rBV2	125	73	0.00%	0.001%
25	5.034	1221	1242	1282	rBV2	585571	1560171	100.00%	12.693%
26	5.323	1328	1332	1334	rBV3	295	219	0.01%	0.002%
27	5.365	1343	1345	1350	rVB2	397	210	0.01%	0.002%
28	5.464	1372	1376	1379	rBV3	389	387	0.02%	0.003%
29	5.506	1388	1389	1394	rVB	404	193	0.01%	0.002%
30	5.538	1395	1399	1402	rBV3	180	153	0.01%	0.001%
31	5.606	1406	1420	1461	rBV	530031	1092161	70.00%	8.885%
32	5.899	1500	1511	1525	rBV6	6666	13972	0.90%	0.114%
33	6.059	1546	1561	1599	rBV	334019	694732	44.53%	5.652%
34	6.284	1629	1631	1634	rVB	345	157	0.01%	0.001%
35	6.329	1639	1645	1648	rBB2	229	183	0.01%	0.001%
36	6.352	1648	1652	1655	rBV	244	216	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029738.D
 Acq On : 20 Dec 2022 09:51
 Operator : SY/MD
 Sample : VV1220WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.416	1671	1672	1675	rVB	371	148	0.01%	0.001%
38	6.468	1686	1688	1691	rBV	210	155	0.01%	0.001%
39	6.513	1698	1702	1706	rBV3	367	344	0.02%	0.003%
40	6.609	1729	1732	1734	rBV	99	69	0.00%	0.001%
41	6.625	1734	1737	1742	rBV2	410	472	0.03%	0.004%
42	6.728	1766	1769	1771	rBV2	196	96	0.01%	0.001%
43	6.783	1783	1786	1788	rBV2	198	130	0.01%	0.001%
44	6.882	1812	1817	1819	rBV2	208	121	0.01%	0.001%
45	6.927	1829	1831	1835	rBV2	168	112	0.01%	0.001%
46	6.976	1835	1846	1877	rBV	163337	301581	19.33%	2.454%
47	7.233	1920	1926	1929	rBV6	1227	1119	0.07%	0.009%
48	7.307	1933	1949	1986	rBV	720842	1279715	82.02%	10.411%
49	7.612	2034	2044	2068	rBV	112738	202143	12.96%	1.645%
50	7.898	2128	2133	2135	rBV4	341	300	0.02%	0.002%
51	7.931	2135	2143	2151	rBV4	999	1768	0.11%	0.014%
52	7.963	2151	2153	2157	rBV3	800	671	0.04%	0.005%
53	8.082	2179	2190	2220	rBV	375944	695942	44.61%	5.662%
54	8.506	2319	2322	2325	rVB3	394	274	0.02%	0.002%
55	8.561	2336	2339	2342	rBV2	373	221	0.01%	0.002%
56	8.593	2345	2349	2352	rBV2	239	182	0.01%	0.001%
57	8.622	2355	2358	2360	rBV2	254	133	0.01%	0.001%
58	8.648	2363	2366	2371	rVV2	266	185	0.01%	0.002%
59	8.841	2412	2426	2457	rBV	771897	1278996	81.98%	10.405%
60	9.133	2511	2517	2526	rBV4	922	1536	0.10%	0.012%
61	9.169	2526	2528	2531	rVV3	209	108	0.01%	0.001%
62	9.207	2535	2540	2544	rBV	247	230	0.01%	0.002%
63	9.284	2562	2564	2565	rBV	224	96	0.01%	0.001%
64	9.326	2574	2577	2580	rBV	227	155	0.01%	0.001%
65	9.361	2584	2588	2593	rVB3	248	253	0.02%	0.002%
66	9.419	2601	2606	2608	rBV2	245	205	0.01%	0.002%
67	9.493	2626	2629	2635	rVB2	189	157	0.01%	0.001%
68	9.548	2635	2646	2647	rBV2	1917	2401	0.15%	0.020%
69	9.622	2667	2669	2673	rVB2	264	142	0.01%	0.001%
70	9.686	2687	2689	2694	rVB2	231	144	0.01%	0.001%
71	9.722	2696	2700	2702	rBV	332	277	0.02%	0.002%
72	9.828	2731	2733	2735	rBV2	214	94	0.01%	0.001%
73	9.924	2756	2763	2774	rVB4	1643	2218	0.14%	0.018%
74	10.078	2807	2811	2813	rBV2	214	163	0.01%	0.001%
75	10.162	2827	2837	2840	rBV2	16340	22022	1.41%	0.179%
76	10.204	2841	2850	2877	rVB	459905	720694	46.19%	5.863%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029738.D
 Acq On : 20 Dec 2022 09:51
 Operator : SY/MD
 Sample : VV1220WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.371	2898	2902	2911	rVB4	1342	1664	0.11%	0.014%
78	10.455	2926	2928	2931	rVB	245	104	0.01%	0.001%
79	10.532	2944	2952	2955	rBV3	1839	2360	0.15%	0.019%
80	10.567	2958	2963	2973	rVB2	7629	11289	0.72%	0.092%
81	10.651	2986	2989	2993	rVB2	231	184	0.01%	0.001%
82	10.673	2993	2996	2998	rBV2	127	88	0.01%	0.001%
83	10.760	3018	3023	3026	rBV2	282	266	0.02%	0.002%
84	10.808	3035	3038	3041	rBV	215	149	0.01%	0.001%
85	10.905	3061	3068	3074	rBV4	1804	2720	0.17%	0.022%
86	11.072	3117	3120	3122	rBV2	265	166	0.01%	0.001%
87	11.117	3132	3134	3139	rVB3	329	215	0.01%	0.002%
88	11.175	3144	3152	3159	rBV4	3430	5137	0.33%	0.042%
89	11.236	3159	3171	3200	rVV	807748	1251245	80.20%	10.179%
90	11.455	3234	3239	3244	rVB2	434	441	0.03%	0.004%
91	11.503	3252	3254	3255	rBV2	248	127	0.01%	0.001%
92	11.612	3274	3288	3319	rBV	715920	1130437	72.46%	9.197%
93	11.802	3344	3347	3348	rBV	279	160	0.01%	0.001%
94	11.837	3355	3358	3361	rBV	233	174	0.01%	0.001%
95	11.911	3379	3381	3386	rBV2	330	253	0.02%	0.002%
96	11.998	3406	3408	3412	rVB2	264	166	0.01%	0.001%
97	12.239	3476	3483	3491	rBV3	1099	1966	0.13%	0.016%
98	12.631	3600	3605	3616	rVB3	5562	8142	0.52%	0.066%
99	13.252	3788	3798	3809	rBV3	11047	17078	1.09%	0.139%
100	13.731	3939	3947	3958	rVB2	13466	20416	1.31%	0.166%




Sum of corrected areas: 12291849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029738.D
Acq On : 20 Dec 2022 09:51
Operator : SY/MD
Sample : VV1220WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

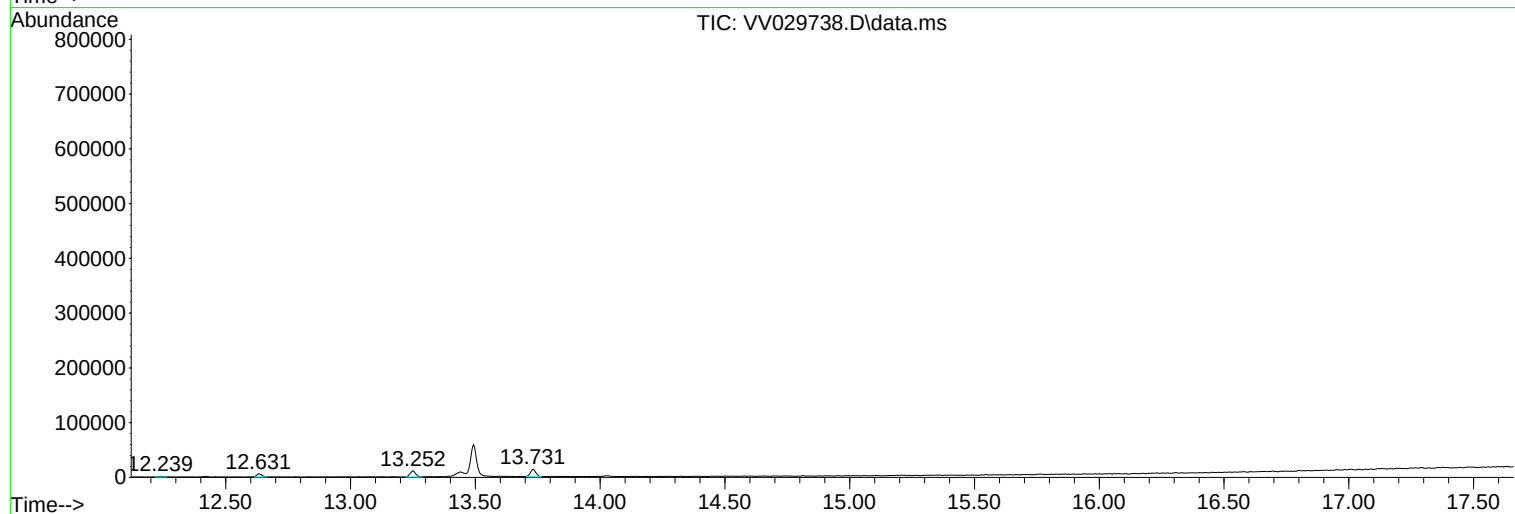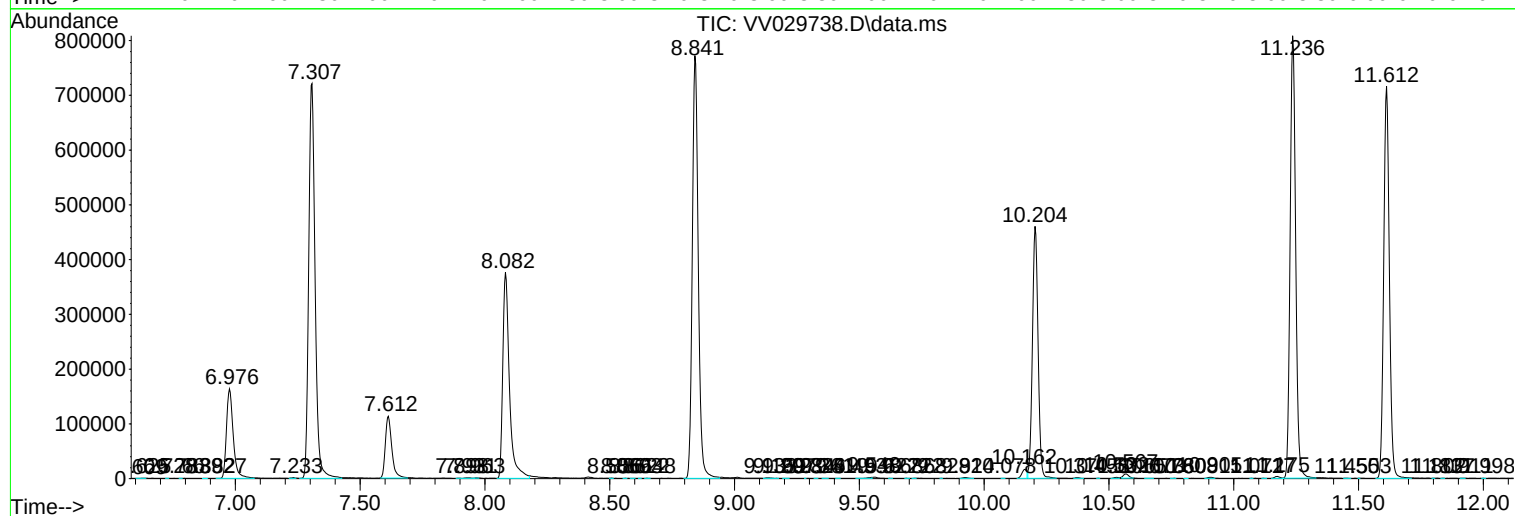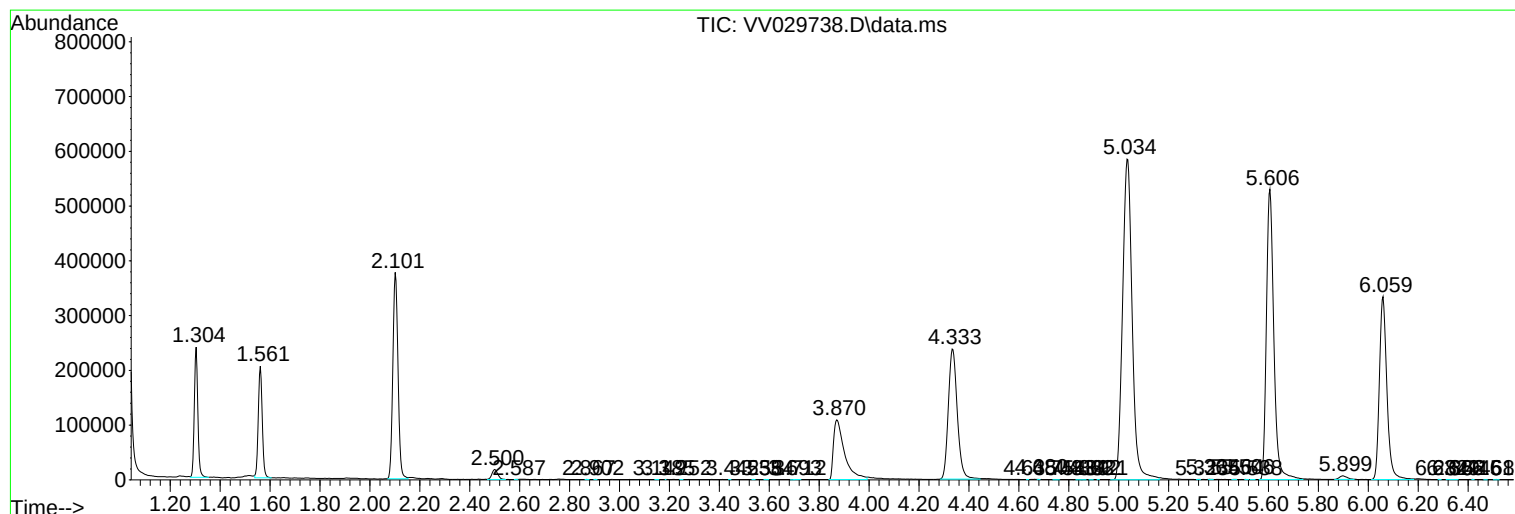

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029738.D
Acq On : 20 Dec 2022 09:51
Operator : SY/MD
Sample : VV1220WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029738.D
Acq On : 20 Dec 2022 09:51
Operator : SY/MD
Sample : VV1220WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc