

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029739.D
 Acq On : 20 Dec 2022 10:28
 Operator : SY/MD
 Sample : N6075-16 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	228371	228672	15.47%	1.877%
2	1.564	156	163	176	rVB	187419	211761	14.32%	1.738%
3	2.105	320	331	344	rBV	357300	516875	34.96%	4.243%
4	2.503	446	455	469	rVB2	3286	5457	0.37%	0.045%
5	2.613	480	489	498	rBV3	940	2064	0.14%	0.017%
6	2.709	517	519	520	rBV	228	56	0.00%	0.000%
7	2.764	531	536	539	rVB4	551	510	0.03%	0.004%
8	2.908	577	581	584	rBV2	188	189	0.01%	0.002%
9	3.137	648	652	656	rBV2	118	121	0.01%	0.001%
10	3.153	656	657	658	rBV	208	55	0.00%	0.000%
11	3.243	683	685	687	rVB2	219	85	0.01%	0.001%
12	3.593	791	794	799	rVV2	284	231	0.02%	0.002%
13	3.632	803	806	809	rBV	117	79	0.01%	0.001%
14	3.667	815	817	820	rBV	79	52	0.00%	0.000%
15	3.744	838	841	842	rBV	93	49	0.00%	0.000%
16	3.818	862	864	868	rVB2	158	65	0.00%	0.001%
17	3.873	868	881	924	rBV2	112138	367681	24.87%	3.018%
18	4.333	1007	1024	1055	rBV	230859	578694	39.15%	4.750%
19	4.625	1110	1115	1121	rVB3	458	517	0.03%	0.004%
20	4.664	1121	1127	1130	rBV3	318	334	0.02%	0.003%
21	4.683	1130	1133	1138	rVB3	376	273	0.02%	0.002%
22	4.719	1138	1144	1146	rVB2	207	217	0.01%	0.002%
23	4.735	1146	1149	1151	rBV	115	83	0.01%	0.001%
24	4.767	1156	1159	1166	rVV2	204	182	0.01%	0.001%
25	4.815	1171	1174	1176	rBV2	162	87	0.01%	0.001%
26	4.831	1176	1179	1183	rBV2	152	109	0.01%	0.001%
27	4.867	1188	1190	1192	rBV2	119	60	0.00%	0.000%
28	4.892	1194	1198	1200	rVV2	135	124	0.01%	0.001%
29	4.905	1200	1202	1206	rVV2	242	128	0.01%	0.001%
30	4.921	1206	1207	1209	rVB	123	45	0.00%	0.000%
31	4.969	1217	1222	1224	rBV2	209	125	0.01%	0.001%
32	5.034	1224	1242	1270	rBV2	561261	1478311	100.00%	12.135%
33	5.394	1350	1354	1358	rBV2	322	356	0.02%	0.003%
34	5.445	1367	1370	1371	rBV	269	98	0.01%	0.001%
35	5.465	1371	1376	1381	rVV2	241	348	0.02%	0.003%
36	5.603	1406	1419	1456	rBV	546146	1123121	75.97%	9.219%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029739.D
 Acq On : 20 Dec 2022 10:28
 Operator : SY/MD
 Sample : N6075-16 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.899	1500	1511	1525	rVB7	5516	12375	0.84%	0.102%
38	6.056	1546	1560	1589	rBV	322107	665058	44.99%	5.459%
39	6.304	1635	1637	1638	rBV	144	63	0.00%	0.001%
40	6.333	1643	1646	1649	rVB2	204	119	0.01%	0.001%
41	6.387	1661	1663	1668	rBV	173	100	0.01%	0.001%
42	6.490	1690	1695	1696	rBV	196	169	0.01%	0.001%
43	6.532	1707	1708	1709	rVB	225	43	0.00%	0.000%
44	6.542	1709	1711	1712	rBV	171	41	0.00%	0.000%
45	6.548	1712	1713	1715	rVB	224	46	0.00%	0.000%
46	6.612	1728	1733	1734	rBV	191	168	0.01%	0.001%
47	6.825	1796	1799	1802	rBV	98	60	0.00%	0.000%
48	6.847	1802	1806	1808	rBV	150	117	0.01%	0.001%
49	6.899	1816	1822	1825	rBV	149	181	0.01%	0.001%
50	6.976	1834	1846	1873	rBV	161797	301043	20.36%	2.471%
51	7.211	1918	1919	1920	rVB	224	43	0.00%	0.000%
52	7.233	1920	1926	1933	rBV3	508	622	0.04%	0.005%
53	7.304	1935	1948	1982	rBV	673637	1211986	81.98%	9.948%
54	7.609	2033	2043	2072	rBV	114126	204674	13.85%	1.680%
55	7.767	2090	2092	2093	rBV	357	145	0.01%	0.001%
56	7.892	2128	2131	2132	rBV2	248	102	0.01%	0.001%
57	8.082	2180	2190	2226	rBV	348033	651136	44.05%	5.345%
58	8.468	2306	2310	2313	rVB3	431	360	0.02%	0.003%
59	8.497	2316	2319	2320	rBV	276	150	0.01%	0.001%
60	8.545	2330	2334	2339	rVB3	440	376	0.03%	0.003%
61	8.567	2339	2341	2343	rVB	161	45	0.00%	0.000%
62	8.590	2346	2348	2350	rBV2	219	96	0.01%	0.001%
63	8.664	2370	2371	2374	rBV	365	142	0.01%	0.001%
64	8.693	2378	2380	2382	rBV	137	80	0.01%	0.001%
65	8.709	2382	2385	2386	rBV2	165	102	0.01%	0.001%
66	8.841	2413	2426	2455	rBV	801239	1320186	89.30%	10.837%
67	9.120	2510	2513	2514	rBV2	642	390	0.03%	0.003%
68	9.198	2535	2537	2539	rBV	115	60	0.00%	0.000%
69	9.278	2560	2562	2565	rBV2	175	59	0.00%	0.000%
70	9.349	2581	2584	2586	rBV	225	160	0.01%	0.001%
71	9.452	2614	2616	2618	rVB	177	73	0.00%	0.001%
72	9.519	2633	2637	2638	rBV2	186	134	0.01%	0.001%
73	9.532	2638	2641	2642	rBV2	461	256	0.02%	0.002%
74	9.590	2658	2659	2660	rBV2	118	38	0.00%	0.000%
75	9.599	2660	2662	2666	rVB2	205	104	0.01%	0.001%
76	9.677	2684	2686	2688	rBV	191	95	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029739.D
 Acq On : 20 Dec 2022 10:28
 Operator : SY/MD
 Sample : N6075-16 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.989	2780	2783	2786	rBV	176	114	0.01%	0.001%
78	10.082	2809	2812	2819	rVB2	289	239	0.02%	0.002%
79	10.114	2819	2822	2824	rBV	334	174	0.01%	0.001%
80	10.162	2827	2837	2840	rBV2	17220	24006	1.62%	0.197%
81	10.204	2841	2850	2867	rVB	456191	723852	48.96%	5.942%
82	10.371	2898	2902	2911	rVB4	1292	1712	0.12%	0.014%
83	10.407	2911	2913	2914	rBV	185	81	0.01%	0.001%
84	10.497	2938	2941	2944	rVB2	190	93	0.01%	0.001%
85	10.529	2944	2951	2954	rBV4	578	770	0.05%	0.006%
86	10.567	2955	2963	2974	rVB2	8250	12448	0.84%	0.102%
87	10.654	2988	2990	2991	rBV	192	78	0.01%	0.001%
88	10.834	3045	3046	3047	rBV	224	45	0.00%	0.000%
89	10.908	3063	3069	3074	rBV3	822	1014	0.07%	0.008%
90	11.069	3117	3119	3125	rVB2	292	191	0.01%	0.002%
91	11.149	3137	3144	3147	rBV6	921	1050	0.07%	0.009%
92	11.236	3159	3171	3194	rBV	869395	1353032	91.53%	11.106%
93	11.612	3275	3288	3313	rBV	715554	1138888	77.04%	9.348%
94	11.821	3351	3353	3356	rBV	286	130	0.01%	0.001%
95	11.915	3380	3382	3384	rBV	216	81	0.01%	0.001%
96	12.165	3458	3460	3465	rBV2	273	240	0.02%	0.002%
97	12.336	3507	3513	3521	rBV6	2515	3526	0.24%	0.029%
98	13.252	3792	3798	3812	rVB4	3339	5304	0.36%	0.044%
99	13.496	3866	3874	3887	rVB	13054	21409	1.45%	0.176%
100	13.728	3941	3946	3958	rVB4	3476	5714	0.39%	0.047%




Sum of corrected areas: 12182602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029739.D
Acq On : 20 Dec 2022 10:28
Operator : SY/MD
Sample : N6075-16 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

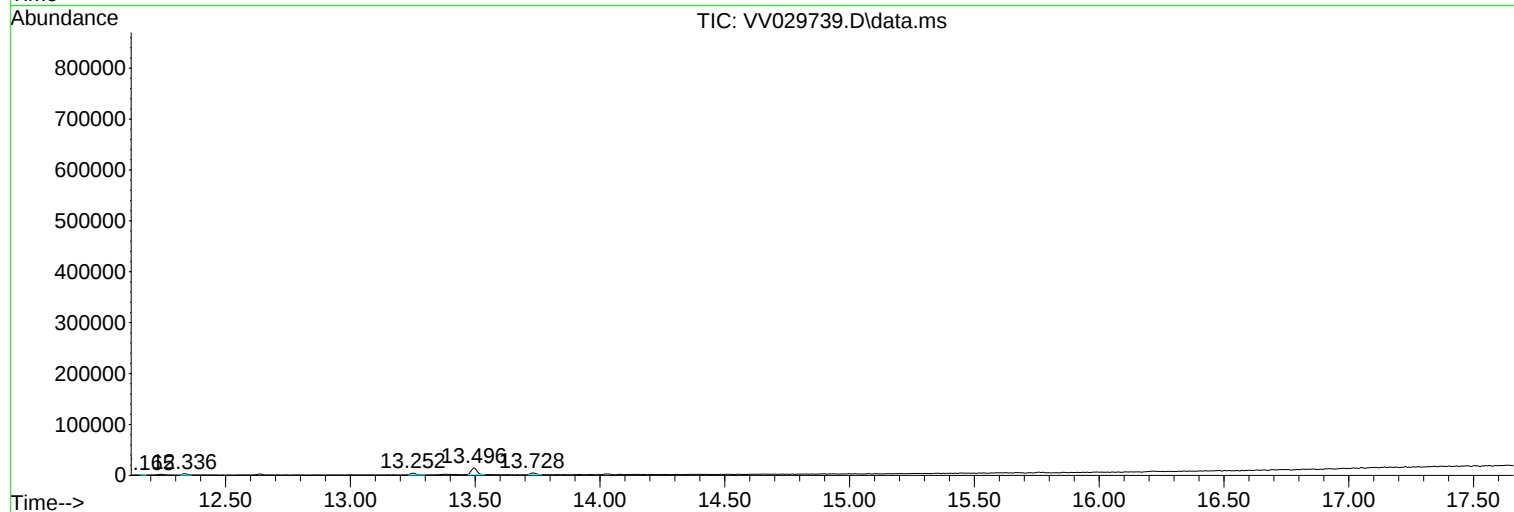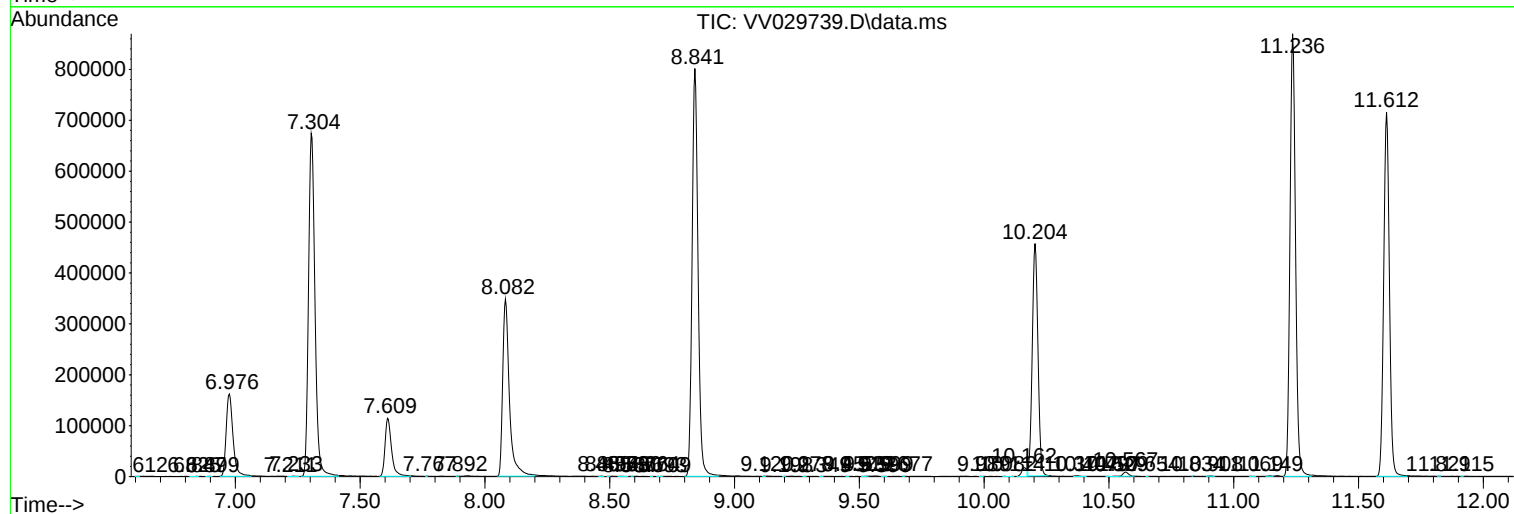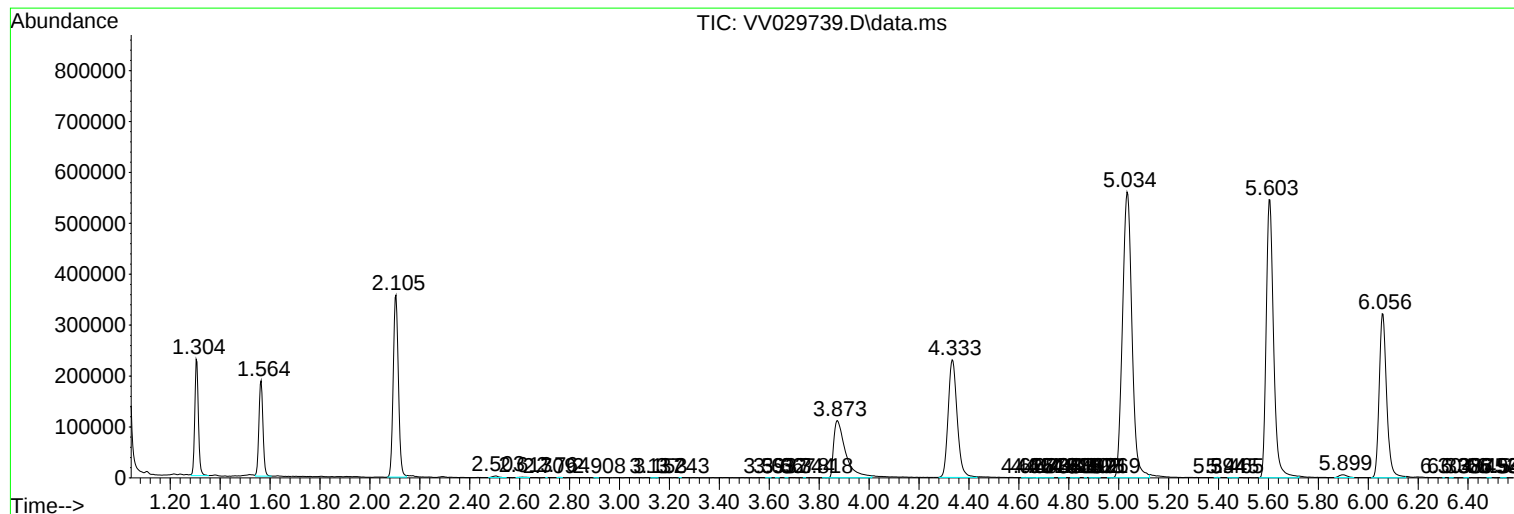

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029739.D
Acq On : 20 Dec 2022 10:28
Operator : SY/MD
Sample : N6075-16 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029739.D
Acq On : 20 Dec 2022 10:28
Operator : SY/MD
Sample : N6075-16 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------