

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029740.D
 Acq On : 20 Dec 2022 10:52
 Operator : SY/MD
 Sample : N6093-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	213778	217228	14.19%	1.808%
2	1.564	156	163	178	rVB	189314	209953	13.71%	1.747%
3	2.105	321	331	349	rBV	356355	513837	33.56%	4.276%
4	2.503	445	455	469	rVB2	17706	28809	1.88%	0.240%
5	2.597	481	484	486	rBV2	212	129	0.01%	0.001%
6	2.780	539	541	543	rBV	189	101	0.01%	0.001%
7	2.838	554	559	562	rBV3	301	261	0.02%	0.002%
8	2.915	580	583	587	rVB3	354	253	0.02%	0.002%
9	2.937	587	590	593	rBV	186	154	0.01%	0.001%
10	3.079	632	634	639	rBV3	214	194	0.01%	0.002%
11	3.179	662	665	669	rBV3	212	174	0.01%	0.001%
12	3.298	699	702	704	rBV	175	103	0.01%	0.001%
13	3.314	704	707	710	rVB2	185	106	0.01%	0.001%
14	3.352	717	719	724	rVB	227	131	0.01%	0.001%
15	3.381	724	728	731	rBV2	200	183	0.01%	0.002%
16	3.429	740	743	744	rBV	231	89	0.01%	0.001%
17	3.445	744	748	752	rVV2	171	166	0.01%	0.001%
18	3.500	762	765	770	rVB2	281	215	0.01%	0.002%
19	3.603	791	797	799	rBV2	188	174	0.01%	0.001%
20	3.632	804	806	810	rVB	150	97	0.01%	0.001%
21	3.818	853	864	869	rVB2	176	279	0.02%	0.002%
22	3.876	869	882	937	rBV2	109940	347772	22.71%	2.894%
23	4.339	1011	1026	1057	rBV	234147	574801	37.54%	4.783%
24	4.616	1108	1112	1115	rBV2	298	237	0.02%	0.002%
25	4.638	1118	1119	1120	rBV2	248	85	0.01%	0.001%
26	4.696	1133	1137	1139	rBV2	238	186	0.01%	0.002%
27	4.738	1148	1150	1153	rVB2	231	115	0.01%	0.001%
28	4.760	1153	1157	1160	rBV2	227	169	0.01%	0.001%
29	4.786	1163	1165	1170	rVB2	177	130	0.01%	0.001%
30	4.873	1190	1192	1198	rBV3	178	142	0.01%	0.001%
31	4.912	1198	1204	1207	rBV2	174	191	0.01%	0.002%
32	4.947	1211	1215	1217	rBV	141	103	0.01%	0.001%
33	5.040	1223	1244	1292	rBV2	575221	1531163	100.00%	12.740%
34	5.452	1369	1372	1374	rBV2	263	136	0.01%	0.001%
35	5.478	1374	1380	1384	rBV3	345	441	0.03%	0.004%
36	5.532	1392	1397	1400	rBV3	195	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029740.D
 Acq On : 20 Dec 2022 10:52
 Operator : SY/MD
 Sample : N6093-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.564	1403	1407	1408	rBV2	162	108	0.01%	0.001%
38	5.609	1408	1421	1450	rBV	514659	1049922	68.57%	8.736%
39	5.902	1501	1512	1533	rVB3	7040	14947	0.98%	0.124%
40	6.063	1547	1562	1600	rBV	333174	687039	44.87%	5.717%
41	6.349	1647	1651	1654	rBB2	247	133	0.01%	0.001%
42	6.420	1670	1673	1675	rBV	209	105	0.01%	0.001%
43	6.471	1685	1689	1691	rBV	125	96	0.01%	0.001%
44	6.529	1703	1707	1709	rBV2	176	105	0.01%	0.001%
45	6.603	1726	1730	1733	rBV	238	150	0.01%	0.001%
46	6.625	1733	1737	1741	rBV2	436	419	0.03%	0.003%
47	6.712	1761	1764	1766	rBV2	136	87	0.01%	0.001%
48	6.873	1811	1814	1818	rVB2	212	166	0.01%	0.001%
49	6.899	1819	1822	1823	rBV2	250	106	0.01%	0.001%
50	6.979	1836	1847	1878	rVV	157097	293488	19.17%	2.442%
51	7.159	1901	1903	1906	rBV2	482	234	0.02%	0.002%
52	7.220	1919	1922	1923	rBV2	314	179	0.01%	0.001%
53	7.252	1928	1932	1935	rVB4	368	242	0.02%	0.002%
54	7.307	1935	1949	1983	rBV	701277	1239880	80.98%	10.317%
55	7.616	2034	2045	2067	rBV	110032	195658	12.78%	1.628%
56	7.847	2114	2117	2119	rBV2	381	191	0.01%	0.002%
57	7.973	2154	2156	2158	rVB	261	139	0.01%	0.001%
58	8.085	2180	2191	2227	rBV	378179	709069	46.31%	5.900%
59	8.503	2318	2321	2322	rBV	311	177	0.01%	0.001%
60	8.561	2336	2339	2342	rBV	315	184	0.01%	0.002%
61	8.580	2342	2345	2349	rBV2	356	230	0.02%	0.002%
62	8.612	2351	2355	2357	rBV2	304	239	0.02%	0.002%
63	8.657	2366	2369	2373	rVV3	393	259	0.02%	0.002%
64	8.776	2404	2406	2409	rBV	143	101	0.01%	0.001%
65	8.799	2410	2413	2415	rBV2	186	90	0.01%	0.001%
66	8.844	2415	2427	2453	rBV	764691	1248635	81.55%	10.390%
67	9.130	2513	2516	2518	rBV2	670	469	0.03%	0.004%
68	9.210	2538	2541	2542	rBV2	182	93	0.01%	0.001%
69	9.304	2568	2570	2574	rVB	266	133	0.01%	0.001%
70	9.323	2574	2576	2578	rBV	221	98	0.01%	0.001%
71	9.500	2627	2631	2633	rBV	177	129	0.01%	0.001%
72	9.529	2638	2640	2642	rBV2	192	98	0.01%	0.001%
73	9.542	2642	2644	2646	rBV	375	209	0.01%	0.002%
74	9.735	2701	2704	2706	rBV	227	160	0.01%	0.001%
75	9.834	2731	2735	2741	rBV	230	222	0.01%	0.002%
76	9.882	2746	2750	2755	rBV3	263	260	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029740.D
 Acq On : 20 Dec 2022 10:52
 Operator : SY/MD
 Sample : N6093-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2827	2837	2841	rBV2	16878	24659	1.61%	0.205%
78	10.204	2841	2850	2867	rVB	476354	759916	49.63%	6.323%
79	10.371	2895	2902	2918	rBV5	1223	2154	0.14%	0.018%
80	10.487	2935	2938	2940	rBV	203	125	0.01%	0.001%
81	10.532	2943	2952	2953	rVV3	666	686	0.04%	0.006%
82	10.567	2956	2963	2981	rVB2	8324	14480	0.95%	0.120%
83	10.635	2981	2984	2989	rBV2	303	226	0.01%	0.002%
84	10.841	3045	3048	3051	rBV	447	308	0.02%	0.003%
85	10.886	3060	3062	3064	rBV2	252	129	0.01%	0.001%
86	10.905	3065	3068	3077	rVB3	806	836	0.05%	0.007%
87	10.950	3077	3082	3085	rBV2	264	266	0.02%	0.002%
88	11.088	3123	3125	3127	rVB	346	118	0.01%	0.001%
89	11.178	3148	3153	3158	rVB3	933	1030	0.07%	0.009%
90	11.236	3159	3171	3199	rBV	785744	1227323	80.16%	10.212%
91	11.612	3275	3288	3308	rBV	704906	1109735	72.48%	9.234%
92	11.937	3386	3389	3393	rVB	327	217	0.01%	0.002%
93	11.956	3393	3395	3396	rBV	255	111	0.01%	0.001%
94	11.966	3396	3398	3401	rVB2	247	138	0.01%	0.001%
95	12.107	3437	3442	3446	rBV3	329	444	0.03%	0.004%
96	12.291	3497	3499	3506	rVB3	476	316	0.02%	0.003%
97	12.323	3506	3509	3512	rVB2	309	194	0.01%	0.002%
98	12.342	3512	3515	3518	rBV2	263	268	0.02%	0.002%
99	12.426	3539	3541	3543	rBV2	270	107	0.01%	0.001%
100	12.635	3600	3606	3610	rBV4	1414	1593	0.10%	0.013%




Sum of corrected areas: 12018124

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029740.D
Acq On : 20 Dec 2022 10:52
Operator : SY/MD
Sample : N6093-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

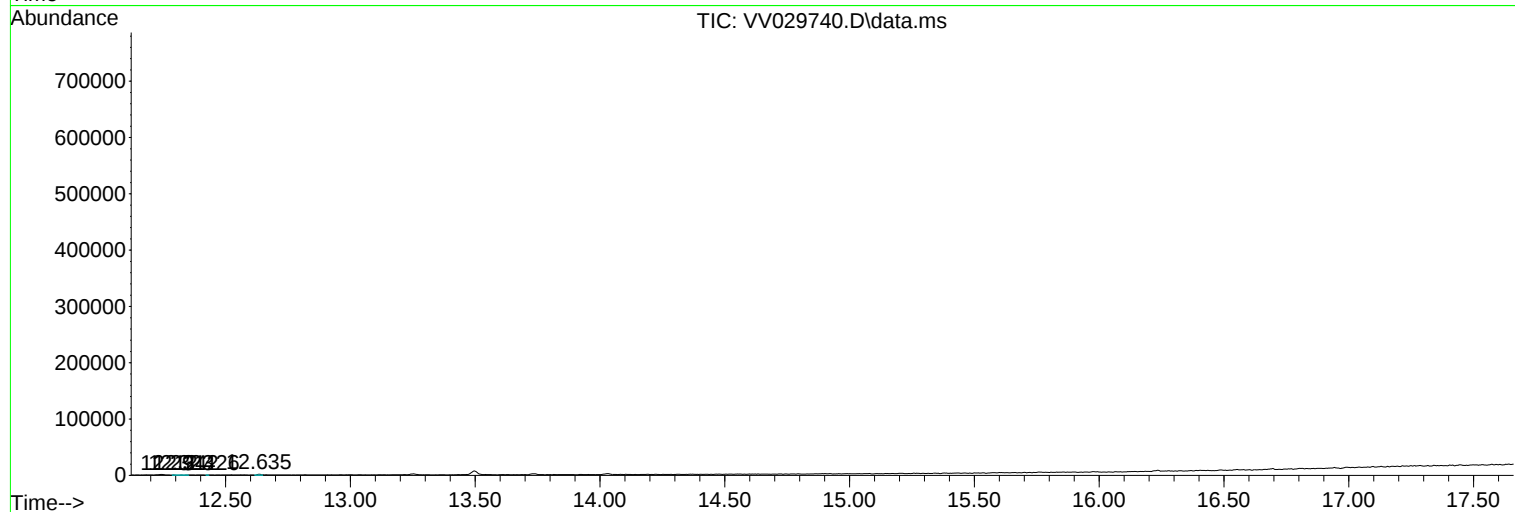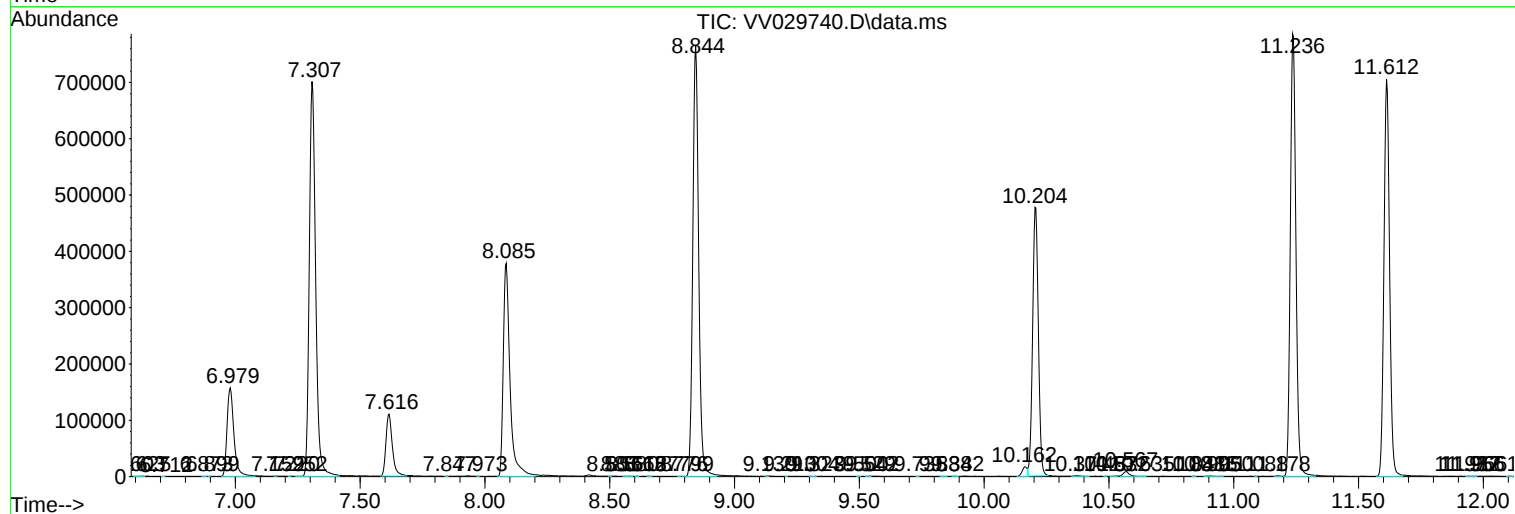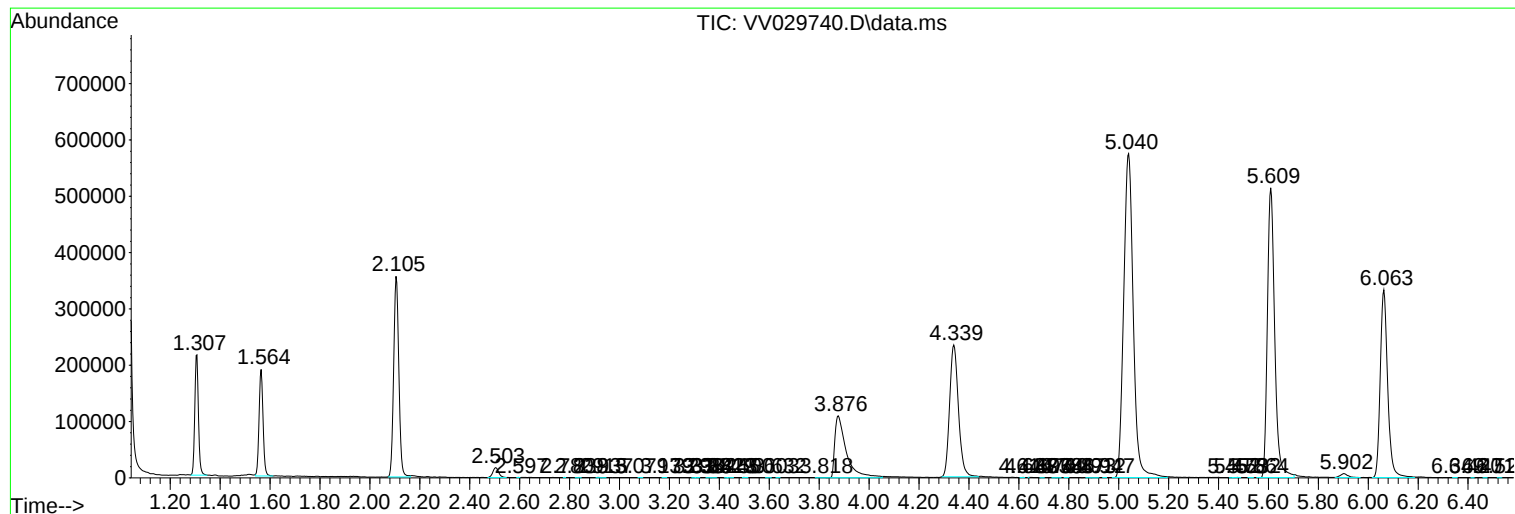

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029740.D
Acq On : 20 Dec 2022 10:52
Operator : SY/MD
Sample : N6093-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029740.D
Acq On : 20 Dec 2022 10:52
Operator : SY/MD
Sample : N6093-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc