

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029741.D
 Acq On : 20 Dec 2022 11:15
 Operator : SY/MD
 Sample : N6075-17 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	199335	200384	13.56%	1.690%
2	1.565	156	163	178	rVB	180095	200758	13.58%	1.693%
3	2.105	321	331	346	rBV	338617	487984	33.02%	4.115%
4	2.446	434	437	439	rBV2	269	178	0.01%	0.002%
5	2.503	446	455	465	rBV3	3670	6013	0.41%	0.051%
6	2.667	503	506	512	rVB3	636	471	0.03%	0.004%
7	2.751	530	532	534	rBV	220	103	0.01%	0.001%
8	2.802	544	548	550	rBV2	202	118	0.01%	0.001%
9	2.931	586	588	589	rBV	158	81	0.01%	0.001%
10	2.999	604	609	613	rBV2	235	237	0.02%	0.002%
11	3.185	663	667	670	rBV	203	182	0.01%	0.002%
12	3.243	683	685	686	rBV	163	72	0.00%	0.001%
13	3.323	705	710	720	rBV2	305	574	0.04%	0.005%
14	3.529	771	774	778	rVB2	207	142	0.01%	0.001%
15	3.552	778	781	785	rBV2	183	170	0.01%	0.001%
16	3.741	835	840	845	rVB2	271	298	0.02%	0.003%
17	3.767	845	848	850	rBV2	159	86	0.01%	0.001%
18	3.796	850	857	861	rBV2	147	192	0.01%	0.002%
19	3.876	868	882	930	rBV2	122425	401254	27.15%	3.384%
20	4.339	1009	1026	1064	rBV	231743	578337	39.13%	4.877%
21	4.606	1108	1109	1111	rBV	227	93	0.01%	0.001%
22	4.674	1120	1130	1131	rBV3	272	454	0.03%	0.004%
23	4.732	1145	1148	1153	rVB2	167	91	0.01%	0.001%
24	4.757	1153	1156	1159	rBV	201	151	0.01%	0.001%
25	4.815	1171	1174	1175	rBV2	157	89	0.01%	0.001%
26	4.912	1202	1204	1207	rBV	162	103	0.01%	0.001%
27	4.934	1207	1211	1216	rVB2	230	225	0.02%	0.002%
28	4.960	1216	1219	1222	rBV	147	101	0.01%	0.001%
29	5.040	1226	1244	1290	rBV2	560972	1477924	100.00%	12.464%
30	5.416	1359	1361	1362	rBV2	328	120	0.01%	0.001%
31	5.449	1369	1371	1372	rVB	253	85	0.01%	0.001%
32	5.465	1373	1376	1378	rBV2	392	230	0.02%	0.002%
33	5.539	1397	1399	1402	rVB	184	121	0.01%	0.001%
34	5.609	1405	1421	1455	rBV	516042	1061421	71.82%	8.951%
35	5.902	1502	1512	1526	rVB3	5695	12057	0.82%	0.102%
36	5.998	1540	1542	1545	rBV2	298	139	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029741.D
 Acq On : 20 Dec 2022 11:15
 Operator : SY/MD
 Sample : N6075-17 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1547	1562	1600	rVV	324690	669674	45.31%	5.648%
38	6.272	1626	1627	1628	rBV	244	78	0.01%	0.001%
39	6.304	1634	1637	1641	rBV3	205	163	0.01%	0.001%
40	6.326	1641	1644	1647	rVV	211	146	0.01%	0.001%
41	6.387	1661	1663	1666	rBV2	169	96	0.01%	0.001%
42	6.413	1669	1671	1674	rBV	152	81	0.01%	0.001%
43	6.532	1705	1708	1710	rVV	257	149	0.01%	0.001%
44	6.561	1714	1717	1720	rBV	154	93	0.01%	0.001%
45	6.580	1720	1723	1725	rBV2	103	71	0.00%	0.001%
46	6.622	1733	1736	1738	rBV	318	232	0.02%	0.002%
47	6.712	1761	1764	1769	rVB2	121	108	0.01%	0.001%
48	6.741	1769	1773	1777	rBV	97	93	0.01%	0.001%
49	6.764	1777	1780	1782	rBV	108	68	0.00%	0.001%
50	6.786	1785	1787	1790	rVB	323	156	0.01%	0.001%
51	6.815	1790	1796	1798	rBV2	176	201	0.01%	0.002%
52	6.854	1803	1808	1813	rBV2	254	292	0.02%	0.002%
53	6.979	1836	1847	1874	rBV	160550	297773	20.15%	2.511%
54	7.307	1937	1949	1987	rVV	667649	1200304	81.22%	10.123%
55	7.613	2034	2044	2071	rBV	110099	202518	13.70%	1.708%
56	7.937	2133	2145	2155	rBV4	2943	5224	0.35%	0.044%
57	8.085	2180	2191	2234	rBV	378217	705360	47.73%	5.949%
58	8.461	2307	2308	2311	rBV2	241	142	0.01%	0.001%
59	8.481	2311	2314	2317	rBV2	406	306	0.02%	0.003%
60	8.555	2335	2337	2338	rBV2	301	170	0.01%	0.001%
61	8.664	2370	2371	2373	rVB	314	114	0.01%	0.001%
62	8.683	2373	2377	2383	rBV3	278	360	0.02%	0.003%
63	8.751	2396	2398	2403	rVB3	288	192	0.01%	0.002%
64	8.773	2403	2405	2409	rBV2	211	116	0.01%	0.001%
65	8.844	2414	2427	2455	rBV	766835	1249721	84.56%	10.539%
66	9.175	2528	2530	2534	rVB	254	173	0.01%	0.001%
67	9.198	2534	2537	2538	rBV	172	105	0.01%	0.001%
68	9.301	2567	2569	2572	rVB2	181	76	0.01%	0.001%
69	9.426	2604	2608	2611	rVB2	217	150	0.01%	0.001%
70	9.526	2637	2639	2641	rVB	235	94	0.01%	0.001%
71	9.538	2641	2643	2646	rBV3	359	197	0.01%	0.002%
72	9.558	2647	2649	2652	rVB2	392	164	0.01%	0.001%
73	9.574	2652	2654	2657	rBV	235	158	0.01%	0.001%
74	9.625	2663	2670	2672	rBV2	337	276	0.02%	0.002%
75	9.651	2672	2678	2679	rBV	203	168	0.01%	0.001%
76	9.715	2696	2698	2702	rVB	225	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029741.D
 Acq On : 20 Dec 2022 11:15
 Operator : SY/MD
 Sample : N6075-17 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.812	2726	2728	2729	rBV	202	76	0.01%	0.001%
78	9.834	2734	2735	2737	rVB	225	67	0.00%	0.001%
79	9.911	2755	2759	2760	rBV2	440	280	0.02%	0.002%
80	10.014	2789	2791	2794	rBV	160	87	0.01%	0.001%
81	10.059	2803	2805	2806	rBV	212	101	0.01%	0.001%
82	10.165	2828	2838	2841	rVV2	16767	24008	1.62%	0.202%
83	10.207	2842	2851	2877	rVB	474882	746487	50.51%	6.295%
84	10.355	2894	2897	2898	rBV2	450	242	0.02%	0.002%
85	10.371	2898	2902	2910	rVB4	2154	2615	0.18%	0.022%
86	10.532	2946	2952	2954	rBV2	348	360	0.02%	0.003%
87	10.567	2955	2963	2975	rVB2	7639	12309	0.83%	0.104%
88	10.696	3000	3003	3005	rBV	145	89	0.01%	0.001%
89	10.783	3028	3030	3035	rVB2	232	158	0.01%	0.001%
90	10.847	3047	3050	3052	rVB	355	154	0.01%	0.001%
91	10.989	3092	3094	3097	rBV	209	147	0.01%	0.001%
92	11.159	3145	3147	3149	rBV2	281	141	0.01%	0.001%
93	11.175	3150	3152	3154	rVV	506	235	0.02%	0.002%
94	11.239	3159	3172	3199	rBV	781790	1217787	82.40%	10.270%
95	11.429	3227	3231	3238	rVB4	641	734	0.05%	0.006%
96	11.612	3275	3288	3317	rBV	690438	1082644	73.25%	9.130%
97	12.188	3462	3467	3469	rBV3	298	345	0.02%	0.003%
98	12.230	3477	3480	3482	rBV2	765	565	0.04%	0.005%
99	12.413	3534	3537	3538	rBV2	271	131	0.01%	0.001%
100	13.252	3794	3798	3800	rBV3	1392	1051	0.07%	0.009%




Sum of corrected areas: 11857523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029741.D
Acq On : 20 Dec 2022 11:15
Operator : SY/MD
Sample : N6075-17 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

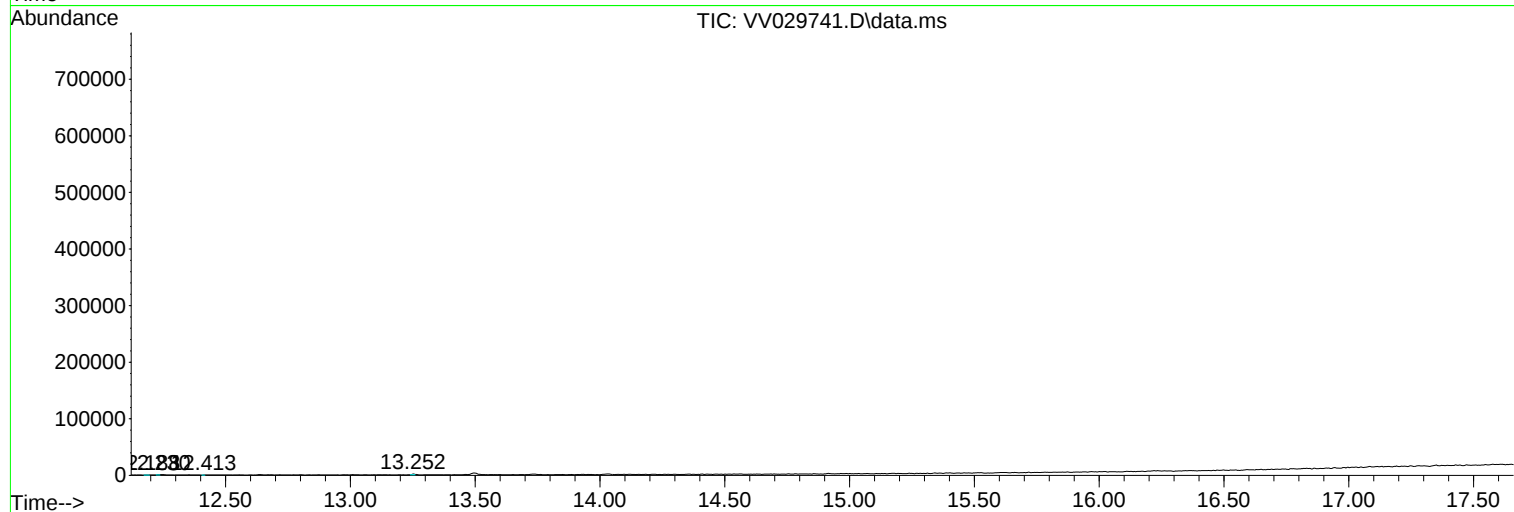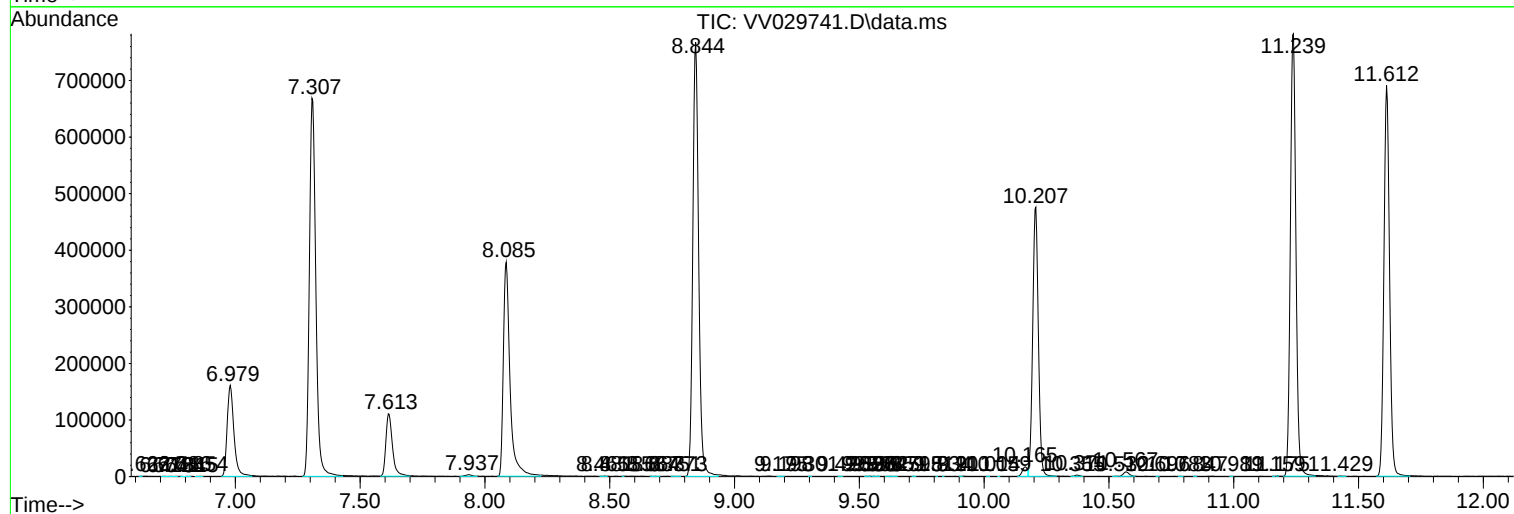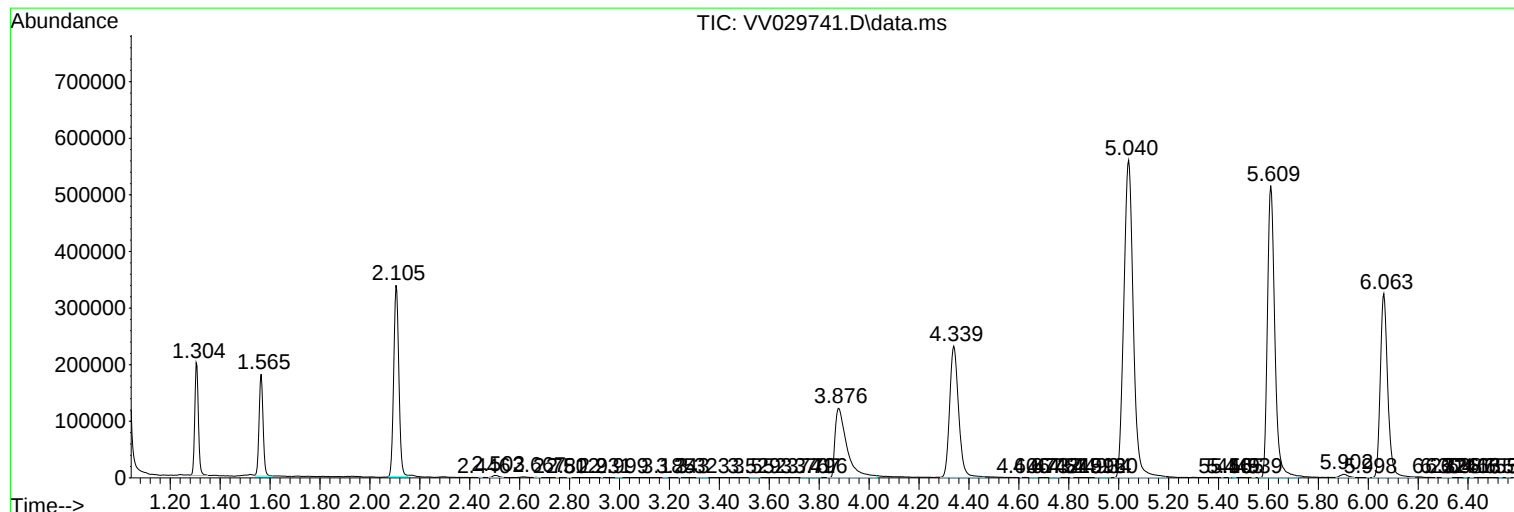

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029741.D
Acq On : 20 Dec 2022 11:15
Operator : SY/MD
Sample : N6075-17 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029741.D
Acq On : 20 Dec 2022 11:15
Operator : SY/MD
Sample : N6075-17 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc