

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029742.D
 Acq On : 20 Dec 2022 11:39
 Operator : SY/MD
 Sample : N6075-18 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	196791	197709	13.81%	1.681%
2	1.564	156	163	177	rVB	169965	192891	13.48%	1.640%
3	2.105	320	331	345	rBV	329962	474398	33.14%	4.034%
4	2.506	446	456	465	rBV2	4903	8212	0.57%	0.070%
5	2.761	532	535	536	rBV2	229	95	0.01%	0.001%
6	2.815	549	552	556	rVB2	207	138	0.01%	0.001%
7	2.834	556	558	560	rBV2	172	94	0.01%	0.001%
8	3.053	622	626	630	rBV2	188	165	0.01%	0.001%
9	3.088	634	637	639	rVV2	204	118	0.01%	0.001%
10	3.114	643	645	649	rVB2	277	141	0.01%	0.001%
11	3.188	666	668	671	rVB2	222	116	0.01%	0.001%
12	3.246	680	686	687	rBV	136	132	0.01%	0.001%
13	3.387	727	730	737	rBV2	200	186	0.01%	0.002%
14	3.452	747	750	751	rBV2	220	131	0.01%	0.001%
15	3.568	783	786	788	rBV2	87	40	0.00%	0.000%
16	3.584	788	791	796	rVV2	117	84	0.01%	0.001%
17	3.616	800	801	802	rVB2	127	25	0.00%	0.000%
18	3.645	808	810	812	rBV	204	127	0.01%	0.001%
19	3.683	818	822	826	rBV2	167	181	0.01%	0.002%
20	3.770	845	849	851	rBV2	124	99	0.01%	0.001%
21	3.805	857	860	867	rVB	258	250	0.02%	0.002%
22	3.876	867	882	930	rBV2	109629	354042	24.73%	3.010%
23	4.339	1009	1026	1056	rBV	224470	557610	38.96%	4.741%
24	4.625	1111	1115	1118	rBV2	325	207	0.01%	0.002%
25	4.693	1133	1136	1137	rBV	155	109	0.01%	0.001%
26	4.789	1164	1166	1169	rVB	155	100	0.01%	0.001%
27	4.825	1175	1177	1180	rVB2	111	50	0.00%	0.000%
28	4.857	1185	1187	1189	rBV	108	56	0.00%	0.000%
29	4.899	1198	1200	1202	rBV	158	66	0.00%	0.001%
30	4.921	1204	1207	1210	rVV2	204	138	0.01%	0.001%
31	4.944	1212	1214	1221	rBV	183	155	0.01%	0.001%
32	5.040	1226	1244	1289	rBV2	537455	1431396	100.00%	12.171%
33	5.378	1345	1349	1351	rBV	378	287	0.02%	0.002%
34	5.439	1365	1368	1369	rBV	136	79	0.01%	0.001%
35	5.526	1394	1395	1397	rVB	118	43	0.00%	0.000%
36	5.609	1407	1421	1450	rBV	534224	1092824	76.35%	9.292%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029742.D
 Acq On : 20 Dec 2022 11:39
 Operator : SY/MD
 Sample : N6075-18 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.902	1502	1512	1526	rVB6	5030	11086	0.77%	0.094%
38	6.011	1544	1546	1547	rBV6	231	96	0.01%	0.001%
39	6.063	1548	1562	1600	rVV	311993	650681	45.46%	5.533%
40	6.297	1631	1635	1638	rBV2	329	266	0.02%	0.002%
41	6.397	1665	1666	1667	rBV2	113	25	0.00%	0.000%
42	6.455	1682	1684	1689	rVB2	249	156	0.01%	0.001%
43	6.493	1689	1696	1697	rBV2	246	223	0.02%	0.002%
44	6.596	1726	1728	1730	rVB	162	45	0.00%	0.000%
45	6.629	1735	1738	1739	rBV	298	161	0.01%	0.001%
46	6.760	1774	1779	1782	rBV2	98	114	0.01%	0.001%
47	6.796	1788	1790	1796	rBV3	309	252	0.02%	0.002%
48	6.844	1804	1805	1808	rVB	164	44	0.00%	0.000%
49	6.876	1811	1815	1816	rBV2	167	145	0.01%	0.001%
50	6.892	1818	1820	1821	rBV	183	90	0.01%	0.001%
51	6.934	1829	1833	1835	rBV2	204	134	0.01%	0.001%
52	6.979	1835	1847	1877	rBV	155323	288147	20.13%	2.450%
53	7.162	1901	1904	1905	rBV2	272	126	0.01%	0.001%
54	7.207	1917	1918	1919	rBV2	260	68	0.00%	0.001%
55	7.307	1937	1949	1982	rBV	649574	1157120	80.84%	9.839%
56	7.612	2034	2044	2076	rBV	108168	194808	13.61%	1.656%
57	7.870	2122	2124	2126	rBV	306	206	0.01%	0.002%
58	8.085	2180	2191	2223	rBV	362023	674705	47.14%	5.737%
59	8.387	2283	2285	2287	rVB	455	169	0.01%	0.001%
60	8.416	2292	2294	2295	rBV	236	98	0.01%	0.001%
61	8.535	2328	2331	2334	rBV3	540	280	0.02%	0.002%
62	8.616	2353	2356	2358	rVB2	600	287	0.02%	0.002%
63	8.661	2368	2370	2372	rVB	221	87	0.01%	0.001%
64	8.686	2375	2378	2379	rBV	210	134	0.01%	0.001%
65	8.693	2379	2380	2381	rBV	232	46	0.00%	0.000%
66	8.722	2387	2389	2393	rBV	231	141	0.01%	0.001%
67	8.744	2393	2396	2398	rVV2	168	84	0.01%	0.001%
68	8.844	2415	2427	2459	rBV	781802	1295181	90.48%	11.013%
69	9.140	2516	2519	2524	rVB5	840	712	0.05%	0.006%
70	9.191	2532	2535	2538	rBV2	284	169	0.01%	0.001%
71	9.207	2538	2540	2541	rBV2	133	31	0.00%	0.000%
72	9.265	2556	2558	2559	rBV2	231	80	0.01%	0.001%
73	9.387	2595	2596	2599	rBV2	162	66	0.00%	0.001%
74	9.522	2635	2638	2640	rBV3	258	171	0.01%	0.001%
75	9.635	2670	2673	2678	rBV2	160	122	0.01%	0.001%
76	9.712	2694	2697	2701	rVB2	290	177	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029742.D
 Acq On : 20 Dec 2022 11:39
 Operator : SY/MD
 Sample : N6075-18 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.728	2701	2702	2703	rBV2	143	45	0.00%	0.000%
78	9.950	2769	2771	2780	rVB	340	271	0.02%	0.002%
79	9.995	2782	2785	2790	rVB2	248	215	0.02%	0.002%
80	10.034	2795	2797	2799	rBV	223	72	0.01%	0.001%
81	10.069	2806	2808	2811	rVB	307	85	0.01%	0.001%
82	10.162	2827	2837	2840	rBV	16060	20884	1.46%	0.178%
83	10.207	2842	2851	2873	rVB	455532	722342	50.46%	6.142%
84	10.522	2946	2949	2951	rBV2	366	271	0.02%	0.002%
85	10.567	2956	2963	2982	rVB	7539	12969	0.91%	0.110%
86	10.902	3064	3067	3072	rBV	710	493	0.03%	0.004%
87	11.175	3148	3152	3158	rBV2	517	531	0.04%	0.005%
88	11.236	3160	3171	3202	rBV	844264	1319165	92.16%	11.217%
89	11.612	3275	3288	3310	rBV	686144	1092097	76.30%	9.286%
90	11.805	3344	3348	3350	rBV2	261	208	0.01%	0.002%
91	11.821	3351	3353	3359	rVV3	601	400	0.03%	0.003%
92	11.857	3361	3364	3373	rVB4	535	555	0.04%	0.005%
93	12.291	3497	3499	3504	rBV2	290	210	0.01%	0.002%
94	12.516	3567	3569	3573	rBV2	282	258	0.02%	0.002%




Sum of corrected areas: 11760298

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029742.D
Acq On : 20 Dec 2022 11:39
Operator : SY/MD
Sample : N6075-18 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

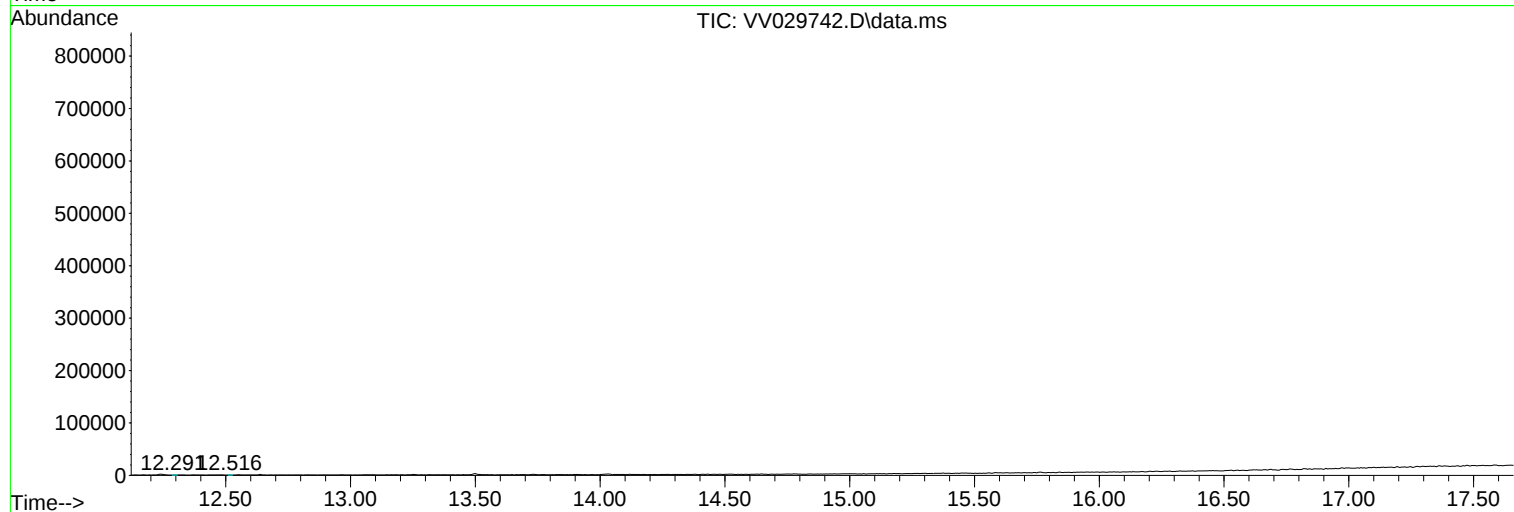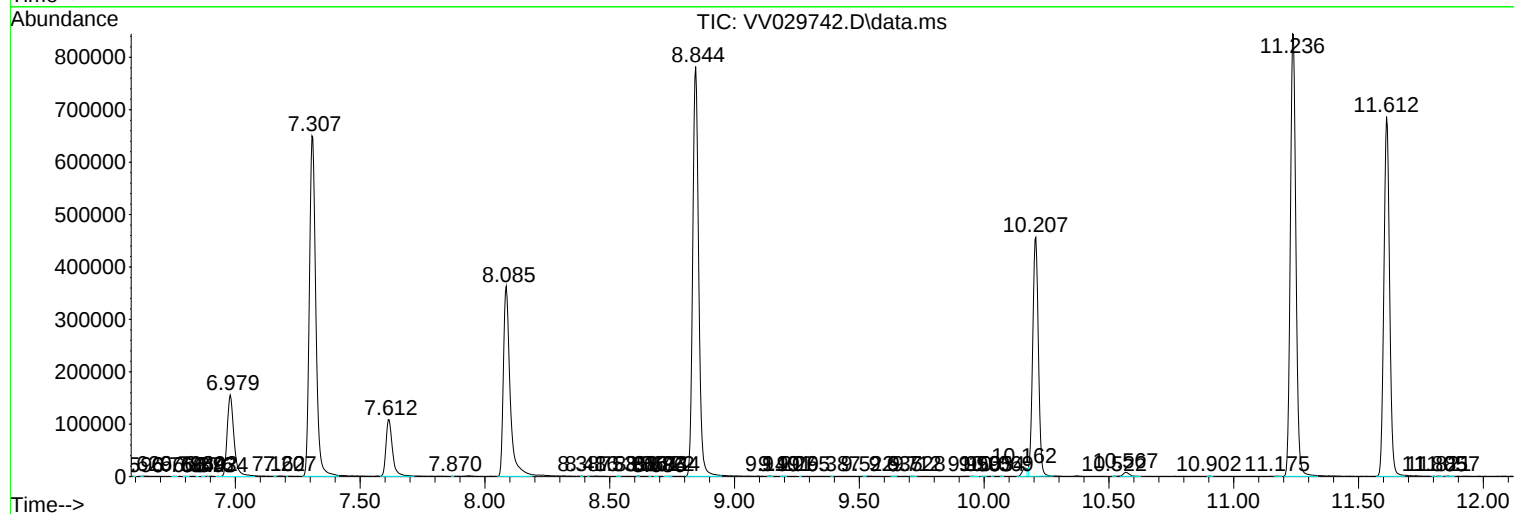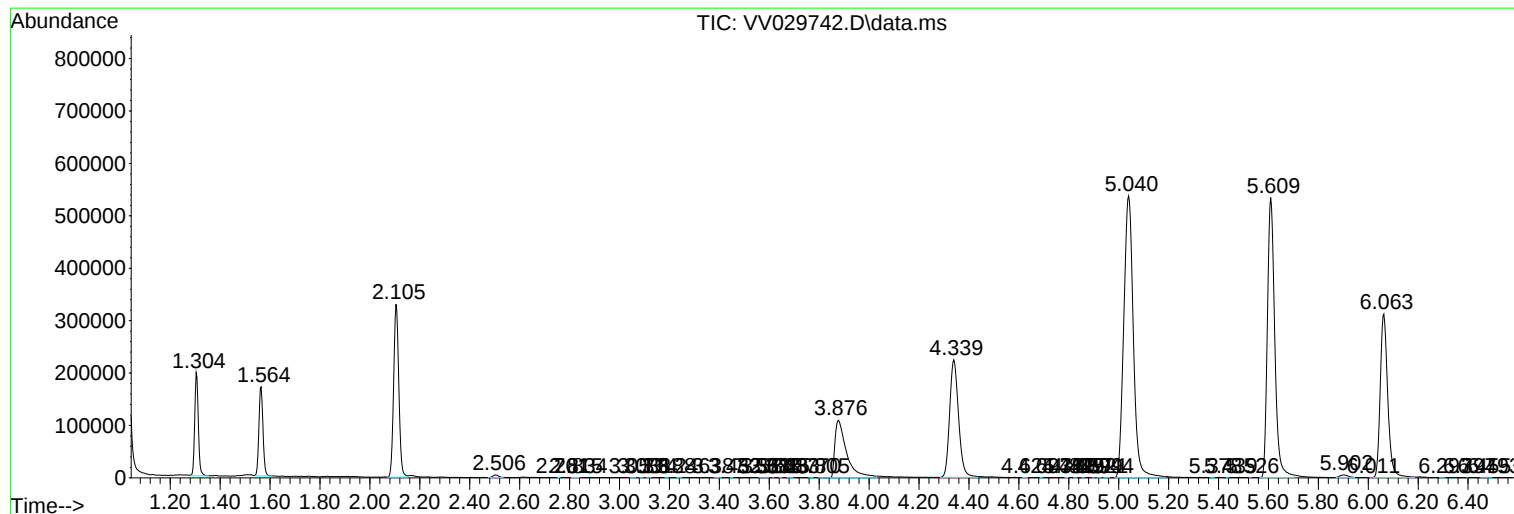

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029742.D
Acq On : 20 Dec 2022 11:39
Operator : SY/MD
Sample : N6075-18 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029742.D
Acq On : 20 Dec 2022 11:39
Operator : SY/MD
Sample : N6075-18 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc