

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029746.D
 Acq On : 20 Dec 2022 13:13
 Operator : SY/MD
 Sample : N6130-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXGJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rVB	176101	172780	14.16%	1.688%
2	1.564	156	163	176	rVB	150679	167435	13.73%	1.635%
3	2.105	320	331	344	rBV	285636	408940	33.52%	3.994%
4	2.503	445	455	468	rVB	10441	17062	1.40%	0.167%
5	2.712	517	520	521	rBV	225	134	0.01%	0.001%
6	2.757	532	534	538	rBV3	221	147	0.01%	0.001%
7	2.883	569	573	574	rBV3	191	131	0.01%	0.001%
8	2.941	587	591	592	rBV2	267	167	0.01%	0.002%
9	3.024	614	617	619	rBV2	270	201	0.02%	0.002%
10	3.269	690	693	695	rVB	316	176	0.01%	0.002%
11	3.326	710	711	716	rBV2	166	131	0.01%	0.001%
12	3.468	751	755	757	rBV	247	201	0.02%	0.002%
13	3.523	769	772	774	rBV	255	138	0.01%	0.001%
14	3.590	787	793	797	rBV	229	233	0.02%	0.002%
15	3.616	799	801	803	rVB2	237	99	0.01%	0.001%
16	3.876	871	882	922	rBV	75890	239707	19.65%	2.341%
17	4.336	1007	1025	1056	rBV	188066	481395	39.46%	4.702%
18	4.600	1105	1107	1111	rVB2	255	145	0.01%	0.001%
19	4.629	1111	1116	1118	rBV3	327	290	0.02%	0.003%
20	4.674	1127	1130	1133	rVB2	347	234	0.02%	0.002%
21	4.712	1136	1142	1145	rBV2	175	180	0.01%	0.002%
22	4.732	1145	1148	1151	rVB	462	282	0.02%	0.003%
23	4.754	1151	1155	1158	rBV2	319	243	0.02%	0.002%
24	4.773	1158	1161	1163	rBV	188	110	0.01%	0.001%
25	4.793	1165	1167	1171	rVB2	188	113	0.01%	0.001%
26	4.854	1183	1186	1190	rBV2	103	96	0.01%	0.001%
27	5.037	1224	1243	1280	rBV2	456572	1219830	100.00%	11.915%
28	5.468	1375	1377	1378	rBV	328	120	0.01%	0.001%
29	5.535	1393	1398	1400	rBV3	280	244	0.02%	0.002%
30	5.551	1401	1403	1406	rBV2	254	158	0.01%	0.002%
31	5.609	1408	1421	1456	rBV	466470	971173	79.62%	9.486%
32	5.899	1503	1511	1522	rBV5	3172	6240	0.51%	0.061%
33	6.059	1547	1561	1587	rBV	267556	558060	45.75%	5.451%
34	6.352	1643	1652	1653	rBV4	3383	4526	0.37%	0.044%
35	6.477	1683	1691	1704	rBV3	6358	13967	1.14%	0.136%
36	6.596	1725	1728	1731	rBV3	259	214	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029746.D
 Acq On : 20 Dec 2022 13:13
 Operator : SY/MD
 Sample : N6130-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXGJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.715	1763	1765	1770	rVB3	397	242	0.02%	0.002%
38	6.757	1776	1778	1782	rBV2	363	190	0.02%	0.002%
39	6.799	1787	1791	1795	rBV3	273	235	0.02%	0.002%
40	6.825	1795	1799	1800	rBV	191	96	0.01%	0.001%
41	6.847	1804	1806	1808	rBV	191	99	0.01%	0.001%
42	6.873	1812	1814	1815	rBV2	216	88	0.01%	0.001%
43	6.902	1821	1823	1827	rVB	339	140	0.01%	0.001%
44	6.928	1827	1831	1832	rBV2	167	124	0.01%	0.001%
45	6.979	1835	1847	1879	rVV	134009	256029	20.99%	2.501%
46	7.182	1902	1910	1920	rBV	11234	20170	1.65%	0.197%
47	7.307	1937	1949	1983	rBV	544803	981953	80.50%	9.591%
48	7.612	2035	2044	2067	rBV	91436	163715	13.42%	1.599%
49	7.747	2083	2086	2089	rBV3	536	347	0.03%	0.003%
50	7.921	2132	2140	2154	rVB2	17233	29366	2.41%	0.287%
51	8.085	2180	2191	2218	rBV	291165	566239	46.42%	5.531%
52	8.587	2343	2347	2351	rBV4	407	460	0.04%	0.004%
53	8.673	2366	2374	2389	rBV	14561	23250	1.91%	0.227%
54	8.844	2414	2427	2464	rBV	703906	1170153	95.93%	11.429%
55	9.136	2512	2518	2521	rBV3	639	745	0.06%	0.007%
56	9.178	2528	2531	2534	rVB2	292	159	0.01%	0.002%
57	9.214	2539	2542	2545	rBV	329	180	0.01%	0.002%
58	9.233	2545	2548	2553	rBV3	265	232	0.02%	0.002%
59	9.294	2564	2567	2568	rBV	188	89	0.01%	0.001%
60	9.381	2585	2594	2596	rBV5	1322	1638	0.13%	0.016%
61	9.436	2608	2611	2612	rBV	250	116	0.01%	0.001%
62	9.715	2695	2698	2699	rBV	201	101	0.01%	0.001%
63	9.850	2735	2740	2744	rBV3	278	307	0.03%	0.003%
64	9.947	2766	2770	2772	rBV	211	177	0.01%	0.002%
65	10.008	2785	2789	2792	rBV2	289	203	0.02%	0.002%
66	10.030	2792	2796	2798	rBV	172	142	0.01%	0.001%
67	10.043	2798	2800	2804	rBV2	246	186	0.02%	0.002%
68	10.098	2813	2817	2820	rBV	279	283	0.02%	0.003%
69	10.165	2827	2838	2840	rBV3	6350	8497	0.70%	0.083%
70	10.204	2840	2850	2878	rVB	394182	630933	51.72%	6.163%
71	10.368	2896	2901	2902	rBV3	1124	898	0.07%	0.009%
72	10.471	2927	2933	2940	rBV3	390	586	0.05%	0.006%
73	10.532	2948	2952	2954	rBV3	621	376	0.03%	0.004%
74	10.564	2954	2962	2976	rVV5	3056	5371	0.44%	0.052%
75	10.619	2977	2979	2983	rVB	293	166	0.01%	0.002%
76	10.651	2987	2989	2992	rVB2	321	148	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029746.D
 Acq On : 20 Dec 2022 13:13
 Operator : SY/MD
 Sample : N6130-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXGJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.683	2998	2999	3002	rVB	294	116	0.01%	0.001%
78	10.760	3020	3023	3024	rBV	300	160	0.01%	0.002%
79	10.789	3030	3032	3035	rBV	300	208	0.02%	0.002%
80	10.815	3038	3040	3043	rBV	176	92	0.01%	0.001%
81	10.863	3052	3055	3058	rBV3	273	189	0.02%	0.002%
82	10.876	3058	3059	3061	rBV	231	104	0.01%	0.001%
83	10.902	3064	3067	3069	rBV	376	221	0.02%	0.002%
84	10.931	3074	3076	3078	rBV	314	141	0.01%	0.001%
85	11.079	3120	3122	3126	rVB2	385	227	0.02%	0.002%
86	11.104	3126	3130	3131	rBV	401	228	0.02%	0.002%
87	11.172	3149	3151	3154	rBV3	492	278	0.02%	0.003%
88	11.236	3159	3171	3205	rBV	734729	1162465	95.30%	11.354%
89	11.612	3276	3288	3306	rBV	586347	924958	75.83%	9.034%
90	11.796	3342	3345	3348	rBV3	574	350	0.03%	0.003%
91	11.937	3387	3389	3394	rBV3	305	255	0.02%	0.002%
92	11.988	3403	3405	3410	rVB3	370	240	0.02%	0.002%
93	12.091	3434	3437	3439	rBV3	362	232	0.02%	0.002%
94	12.619	3598	3601	3602	rBV2	416	266	0.02%	0.003%
95	12.728	3632	3635	3640	rVB3	406	316	0.03%	0.003%
96	12.751	3640	3642	3645	rBV2	510	383	0.03%	0.004%
97	12.834	3657	3668	3679	rBV8	5053	9747	0.80%	0.095%
98	12.947	3697	3703	3710	rBV4	2916	3406	0.28%	0.033%
99	13.082	3739	3745	3754	rBV7	2686	3524	0.29%	0.034%
100	13.175	3772	3774	3775	rBV7	553	229	0.02%	0.002%




Sum of corrected areas: 10238066

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029746.D
Acq On : 20 Dec 2022 13:13
Operator : SY/MD
Sample : N6130-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXGJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

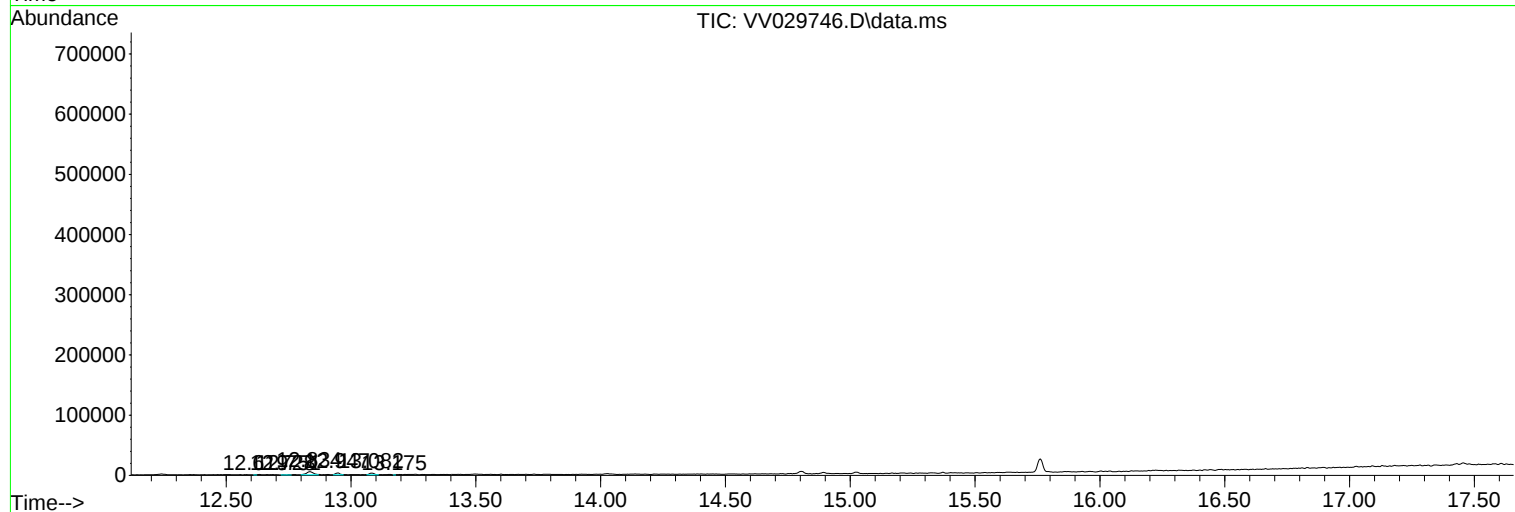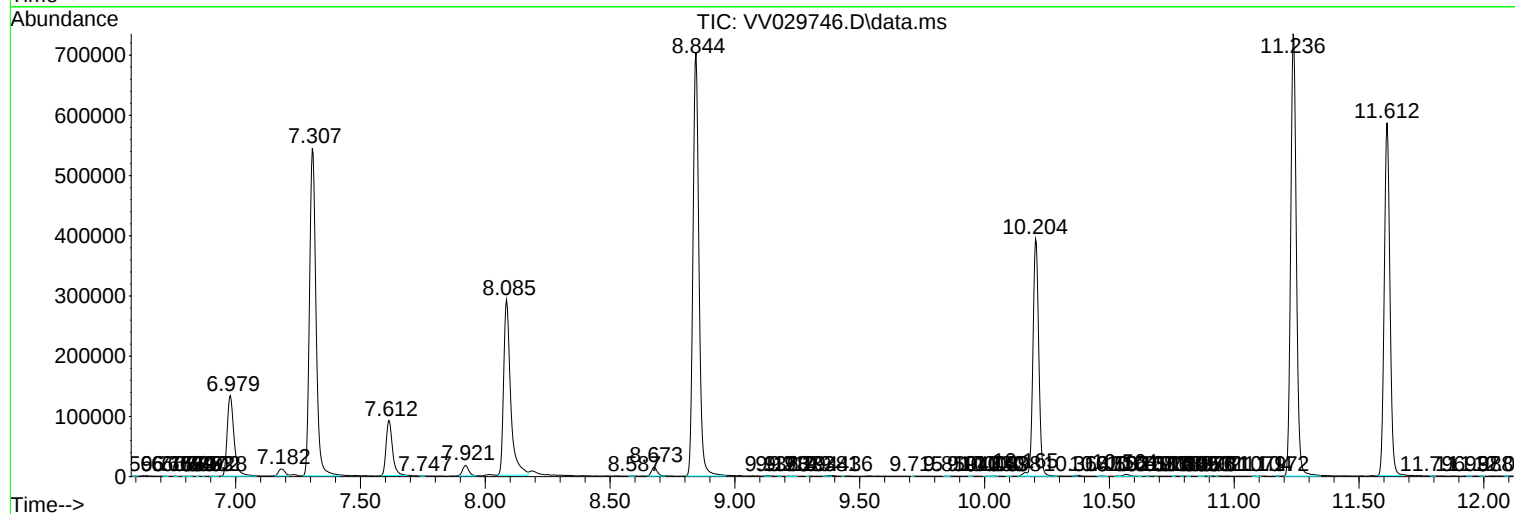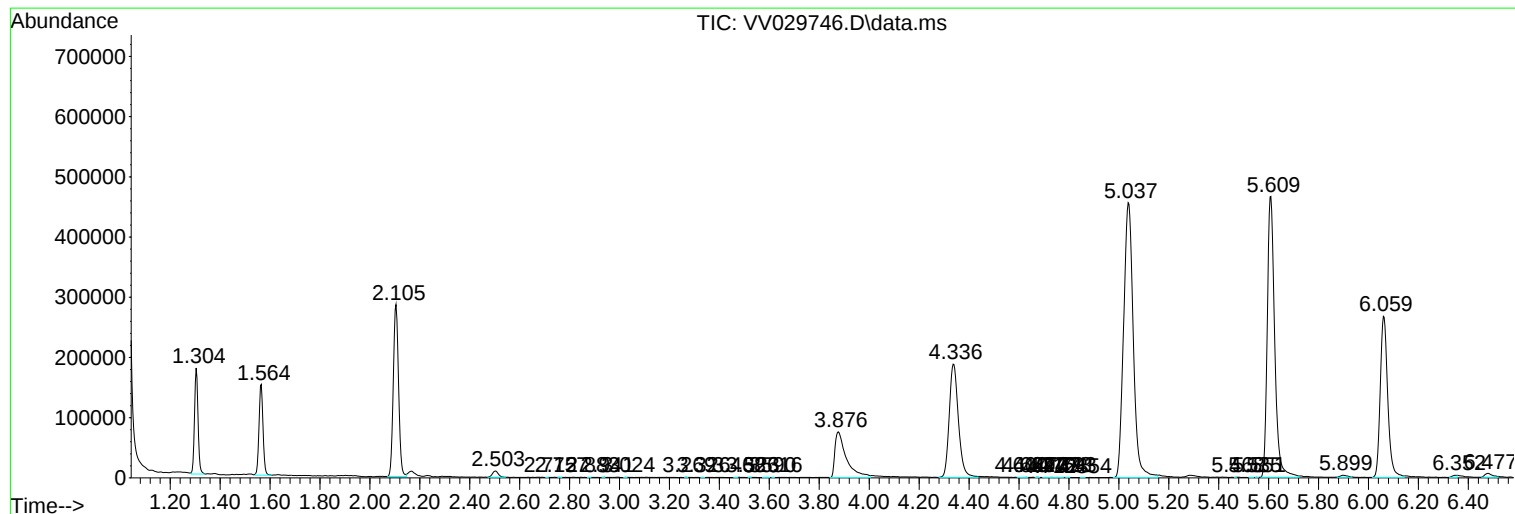

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029746.D
Acq On : 20 Dec 2022 13:13
Operator : SY/MD
Sample : N6130-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXGJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029746.D
Acq On : 20 Dec 2022 13:13
Operator : SY/MD
Sample : N6130-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXGJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------