

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
 Data File : VV029751.D
 Acq On : 20 Dec 2022 15:14
 Operator : SY/MD
 Sample : N6130-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029751.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	212518	213683	13.92%	1.703%
2	1.565	156	163	179	rVB	184525	206115	13.43%	1.642%
3	2.105	321	331	364	rVB	359154	520574	33.92%	4.148%
4	2.503	447	455	465	rBV4	4312	6808	0.44%	0.054%
5	2.928	584	587	591	rBV3	317	272	0.02%	0.002%
6	2.970	597	600	603	rVB3	246	187	0.01%	0.001%
7	2.999	606	609	615	rBV3	276	369	0.02%	0.003%
8	3.079	630	634	636	rBV	260	191	0.01%	0.002%
9	3.214	673	676	678	rBV2	235	135	0.01%	0.001%
10	3.304	701	704	705	rBV2	233	139	0.01%	0.001%
11	3.397	730	733	735	rBV	177	121	0.01%	0.001%
12	3.516	764	770	774	rBV3	267	292	0.02%	0.002%
13	3.539	774	777	778	rBV	219	103	0.01%	0.001%
14	3.667	815	817	822	rVB2	208	145	0.01%	0.001%
15	3.741	837	840	842	rVB2	243	148	0.01%	0.001%
16	3.796	853	857	865	rBV3	306	394	0.03%	0.003%
17	3.831	865	868	870	rBV2	114	87	0.01%	0.001%
18	3.873	870	881	917	rBV	95259	286105	18.64%	2.280%
19	4.336	1009	1025	1064	rBV	235192	599289	39.04%	4.776%
20	4.725	1144	1146	1148	rBV	166	82	0.01%	0.001%
21	4.767	1155	1159	1161	rVB2	260	188	0.01%	0.001%
22	4.857	1185	1187	1189	rBV	265	182	0.01%	0.001%
23	4.908	1200	1203	1206	rBV	198	108	0.01%	0.001%
24	4.928	1206	1209	1210	rBV	134	86	0.01%	0.001%
25	5.037	1224	1243	1274	rBV2	582755	1534868	100.00%	12.231%
26	5.355	1340	1342	1343	rBV	295	113	0.01%	0.001%
27	5.471	1375	1378	1380	rBV3	335	236	0.02%	0.002%
28	5.606	1407	1420	1464	rVV	533132	1096006	71.41%	8.734%
29	5.899	1501	1511	1524	rVB8	5042	11303	0.74%	0.090%
30	6.060	1546	1561	1590	rBV	334365	692773	45.14%	5.521%
31	6.326	1638	1644	1645	rBV	323	195	0.01%	0.002%
32	6.407	1667	1669	1672	rVB	367	147	0.01%	0.001%
33	6.439	1676	1679	1683	rBV2	275	181	0.01%	0.001%
34	6.561	1714	1717	1719	rBV	226	173	0.01%	0.001%
35	6.600	1726	1729	1730	rBV	382	156	0.01%	0.001%
36	6.732	1768	1770	1771	rBV	218	93	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029751.D
 Acq On : 20 Dec 2022 15:14
 Operator : SY/MD
 Sample : N6130-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.857	1807	1809	1812	rVB2	174	90	0.01%	0.001%
38	6.908	1823	1825	1829	rVB	251	125	0.01%	0.001%
39	6.934	1829	1833	1835	rBV	207	108	0.01%	0.001%
40	6.976	1835	1846	1872	rBV	179609	331550	21.60%	2.642%
41	7.162	1901	1904	1907	rBV3	386	295	0.02%	0.002%
42	7.233	1918	1926	1928	rBV2	1256	1509	0.10%	0.012%
43	7.307	1937	1949	1972	rBV	708043	1243370	81.01%	9.908%
44	7.613	2034	2044	2065	rBV	121958	216471	14.10%	1.725%
45	7.793	2096	2100	2107	rVB4	650	853	0.06%	0.007%
46	7.838	2107	2114	2119	rBV4	983	991	0.06%	0.008%
47	7.905	2132	2135	2137	rBV2	354	225	0.01%	0.002%
48	8.082	2179	2190	2221	rBV	363238	679951	44.30%	5.418%
49	8.387	2283	2285	2287	rBV2	465	257	0.02%	0.002%
50	8.564	2335	2340	2342	rBV3	402	319	0.02%	0.003%
51	8.606	2345	2353	2358	rBV3	591	947	0.06%	0.008%
52	8.667	2368	2372	2373	rBV	322	201	0.01%	0.002%
53	8.693	2379	2380	2383	rVB2	311	118	0.01%	0.001%
54	8.722	2386	2389	2390	rBV2	257	142	0.01%	0.001%
55	8.741	2392	2395	2398	rBV3	248	195	0.01%	0.002%
56	8.789	2407	2410	2413	rVB2	273	189	0.01%	0.002%
57	8.841	2413	2426	2457	rBV	769333	1296503	84.47%	10.331%
58	9.130	2510	2516	2527	rVB5	1616	2935	0.19%	0.023%
59	9.194	2534	2536	2541	rVB4	324	202	0.01%	0.002%
60	9.217	2541	2543	2545	rVB	250	114	0.01%	0.001%
61	9.236	2545	2549	2552	rBV	295	214	0.01%	0.002%
62	9.272	2558	2560	2562	rBV3	240	149	0.01%	0.001%
63	9.291	2565	2566	2569	rBV	221	115	0.01%	0.001%
64	9.307	2569	2571	2573	rVB	355	161	0.01%	0.001%
65	9.326	2573	2577	2579	rBV2	372	261	0.02%	0.002%
66	9.400	2597	2600	2605	rVV2	414	310	0.02%	0.002%
67	9.436	2609	2611	2619	rVB3	403	426	0.03%	0.003%
68	9.474	2619	2623	2627	rBV3	339	320	0.02%	0.003%
69	9.558	2633	2649	2660	rBV6	3143	7871	0.51%	0.063%
70	9.622	2667	2669	2673	rVB	294	130	0.01%	0.001%
71	9.641	2673	2675	2678	rBV	314	185	0.01%	0.001%
72	9.699	2690	2693	2695	rBV2	149	105	0.01%	0.001%
73	9.786	2718	2720	2721	rBV	222	95	0.01%	0.001%
74	9.924	2756	2763	2769	rBV4	2018	2949	0.19%	0.023%
75	10.066	2802	2807	2809	rBV3	449	414	0.03%	0.003%
76	10.162	2828	2837	2839	rBV2	8341	9942	0.65%	0.079%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122022\
 Data File : VW029751.D
 Acq On : 20 Dec 2022 15:14
 Operator : SY/MD
 Sample : N6130-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.204	2840	2850	2877	rVB	495337	781539	50.92%	6.228%
78	10.375	2895	2903	2911	rBV4	2063	3035	0.20%	0.024%
79	10.709	3004	3007	3009	rBV2	242	180	0.01%	0.001%
80	10.792	3031	3033	3036	rVB2	313	171	0.01%	0.001%
81	10.825	3040	3043	3046	rBV	215	125	0.01%	0.001%
82	10.908	3061	3069	3076	rBV4	3056	3888	0.25%	0.031%
83	11.005	3097	3099	3102	rBV2	188	124	0.01%	0.001%
84	11.088	3123	3125	3128	rVV2	260	109	0.01%	0.001%
85	11.108	3128	3131	3137	rVV4	396	331	0.02%	0.003%
86	11.172	3143	3151	3160	rBV4	4791	7233	0.47%	0.058%
87	11.236	3160	3171	3200	rVV	879559	1361398	88.70%	10.849%
88	11.484	3246	3248	3249	rBV	244	82	0.01%	0.001%
89	11.612	3275	3288	3314	rBV	751005	1214029	79.10%	9.674%
90	11.863	3362	3366	3369	rBV2	291	263	0.02%	0.002%
91	11.966	3395	3398	3402	rBV	303	256	0.02%	0.002%
92	11.985	3402	3404	3406	rBV2	270	148	0.01%	0.001%
93	12.278	3492	3495	3498	rBV2	386	259	0.02%	0.002%
94	12.329	3508	3511	3514	rBV2	550	413	0.03%	0.003%
95	12.506	3560	3566	3568	rBV4	506	502	0.03%	0.004%
96	12.635	3597	3606	3616	rVB3	9377	13751	0.90%	0.110%
97	12.837	3662	3669	3681	rVB9	2326	3594	0.23%	0.029%
98	13.252	3789	3798	3809	rVB2	16323	24251	1.58%	0.193%
99	13.490	3865	3872	3896	rVB	74283	127615	8.31%	1.017%
100	13.731	3939	3947	3961	rVB	20676	32433	2.11%	0.258%




Sum of corrected areas: 12549083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029751.D
Acq On : 20 Dec 2022 15:14
Operator : SY/MD
Sample : N6130-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

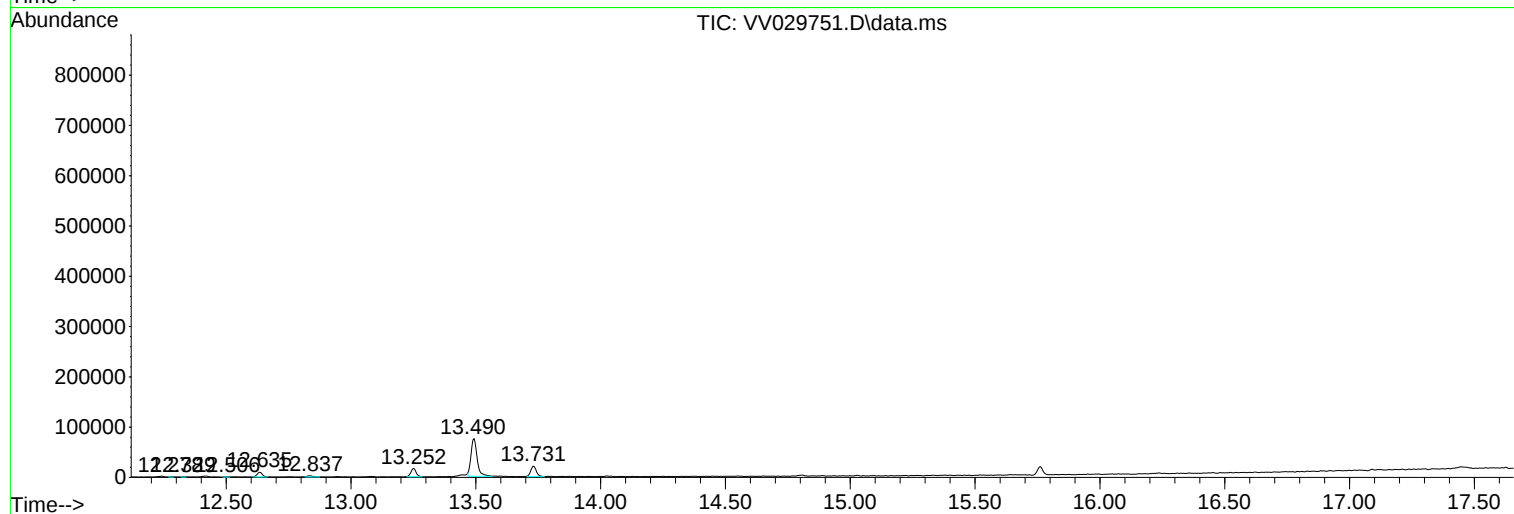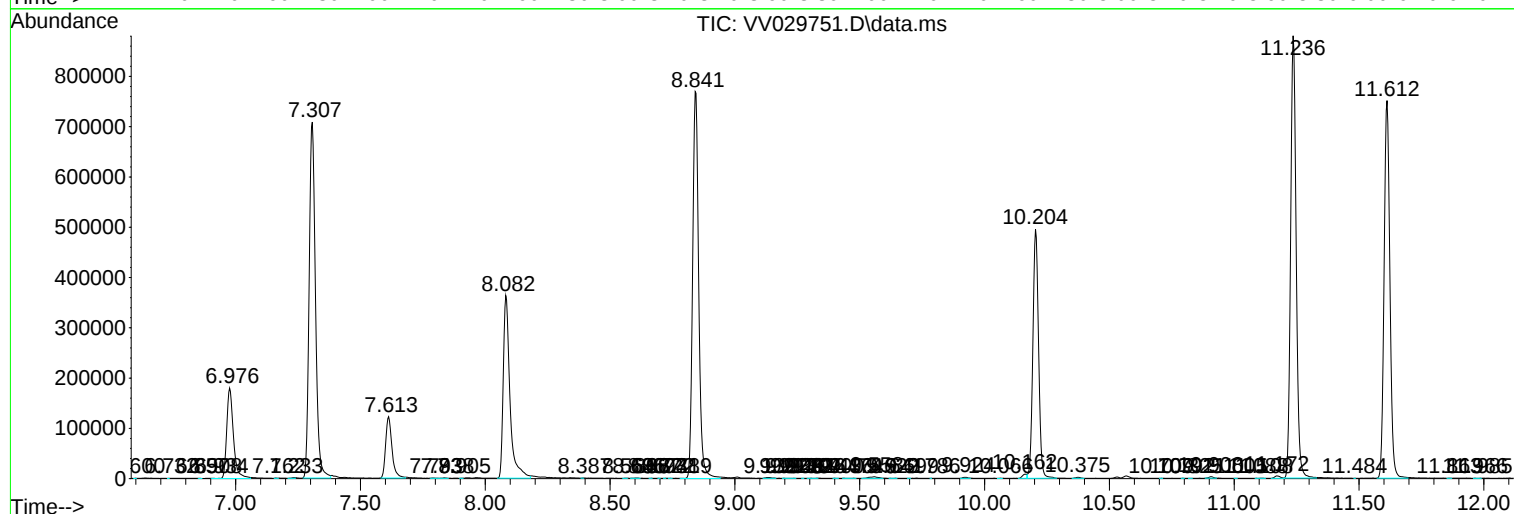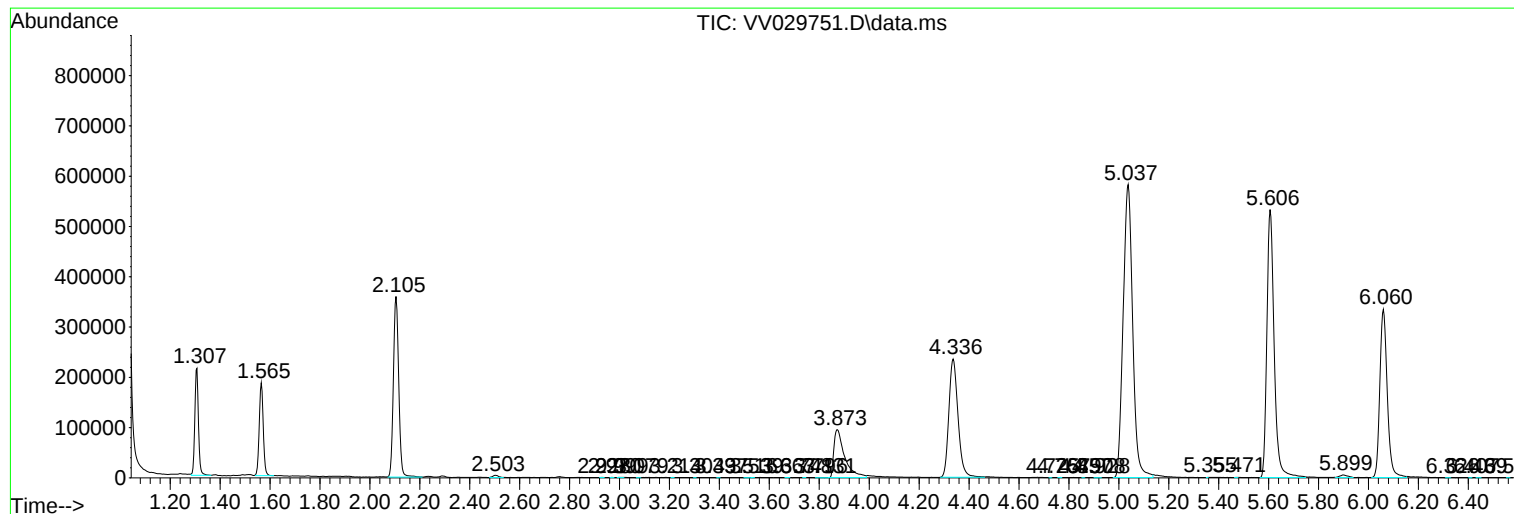

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029751.D
Acq On : 20 Dec 2022 15:14
Operator : SY/MD
Sample : N6130-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029751.D
Acq On : 20 Dec 2022 15:14
Operator : SY/MD
Sample : N6130-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc