
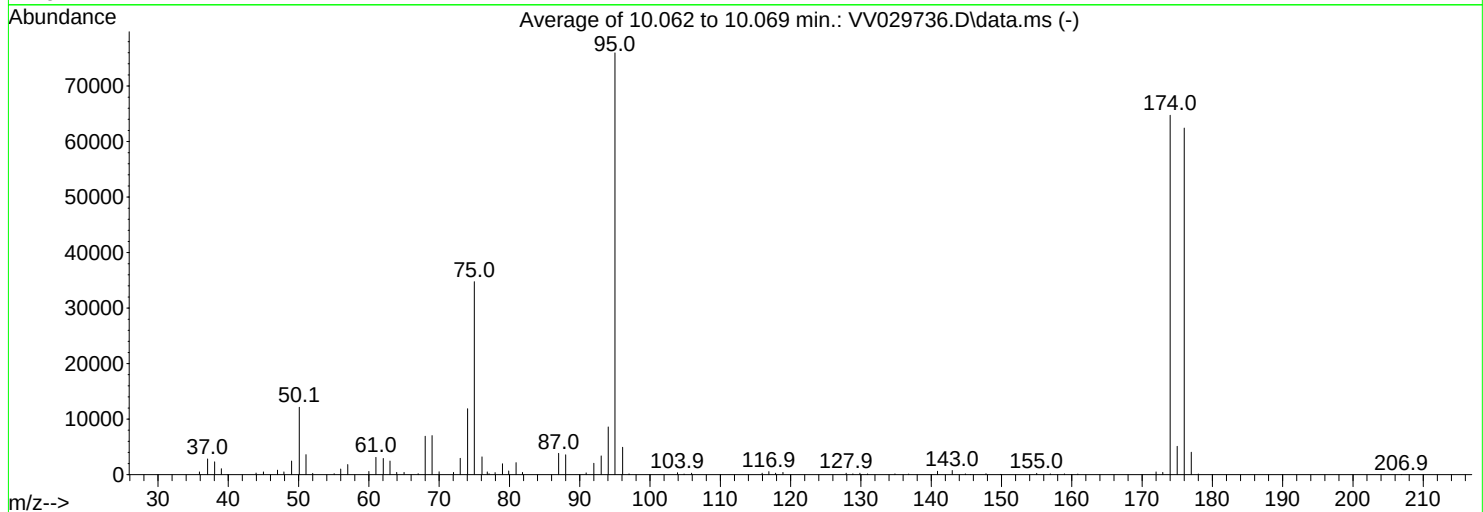


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122022\
Data File : VV029736.D
Acq On : 20 Dec 2022 08:56
Operator : SY/MD
Sample : BFB358
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB358

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Title : VOC Analysis
Last Update : Wed Dec 21 00:15:13 2022

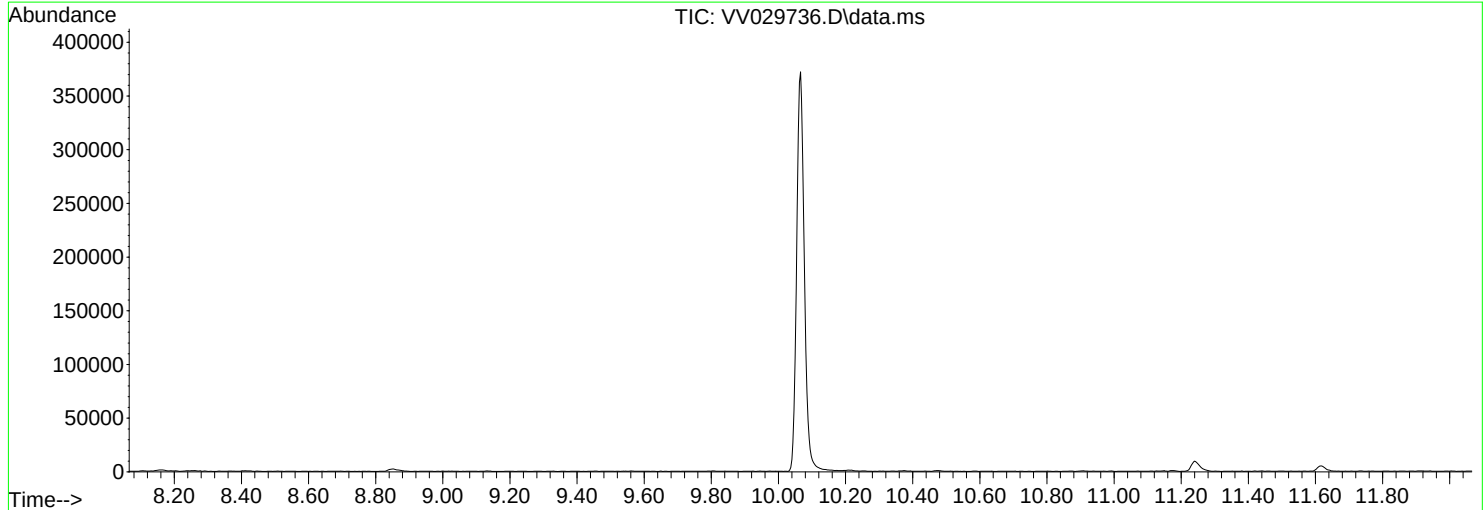

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	12124	PASS
75	95	30	80	45.8	34765	PASS
95	95	100	100	100.0	75979	PASS
96	95	5	9	6.5	4917	PASS
173	174	0.00	2	0.6	416	PASS
174	95	50	120	85.2	64720	PASS
175	174	5	9	7.9	5107	PASS
176	174	95	105	96.5	62429	PASS
177	176	5	10	6.5	4043	PASS

m/z	Abundance
40.00	237.0
43.90	331.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
35.90	472.0
37.10	2975.0
38.00	2352.0
39.00	1111.0
39.90	235.0
44.00	624.0
45.00	524.0
47.00	803.0
47.90	493.0
49.00	2578.0
50.10	12408.0
51.00	3781.0
52.00	238.0
55.00	200.0
56.00	1046.0
57.00	1837.0
60.00	544.0
61.00	3040.0
62.00	2974.0
63.00	2499.0
64.00	377.0
65.00	363.0
66.90	194.0
68.00	7094.0
69.00	7057.0
70.00	498.0
72.10	428.0
73.00	3002.0
74.10	12078.0
75.00	35456.0
76.10	3342.0
76.80	534.0
77.10	507.0
77.90	410.0
79.00	1977.0
79.90	634.0
80.90	2174.0
81.80	400.0
87.00	3945.0
88.00	3522.0
90.90	301.0
92.00	2219.0
93.10	3509.0
94.00	8490.0
95.00	76832.0
96.10	4880.0
97.00	145.0
103.90	360.0
104.80	104.0
105.90	282.0
115.90	261.0
116.90	463.0
117.80	236.0
118.90	391.0
127.90	253.0
128.90	115.0
129.80	270.0
131.00	157.0
134.90	101.0
136.80	103.0
140.90	614.0
143.00	784.0
144.90	170.0
145.60	104.0
147.70	156.0
154.90	248.0
156.90	132.0
159.00	113.0
160.90	121.0
172.00	459.0
172.90	602.0
174.00	63968.0
175.00	5016.0
176.00	61760.0
177.00	3994.0
178.00	115.0
206.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
35.90	520.0
37.10	2937.0
38.10	2350.0
39.00	1123.0
39.90	236.0
44.00	638.0
45.00	519.0
47.00	825.0
47.90	509.0
49.00	2550.0
50.10	12488.0
51.00	3672.0
52.00	259.0
55.10	184.0
56.00	1034.0
57.00	1886.0
60.00	599.0
61.00	3217.0
62.00	2959.0
63.00	2539.0
63.90	436.0
65.00	433.0
67.00	180.0
68.00	7126.0
69.00	7213.0
70.00	551.0
72.00	435.0
73.00	3016.0
74.00	12257.0
75.00	35912.0
76.10	3304.0
76.80	528.0
77.90	373.0
79.00	2047.0
79.90	712.0
81.00	2250.0
81.90	411.0
87.00	3974.0
88.00	3725.0
90.90	309.0
92.00	2098.0
93.00	3506.0
94.10	8842.0
95.00	78536.0
96.10	5083.0
97.00	157.0
103.90	347.0
104.90	116.0
105.80	280.0
115.90	254.0
116.90	569.0
117.90	271.0
118.90	417.0
127.90	263.0
128.80	133.0
129.90	270.0
130.90	135.0
134.90	135.0
136.80	116.0
140.90	621.0
143.00	783.0
144.90	149.0
147.80	158.0
149.90	109.0
155.00	238.0
156.90	156.0
158.90	146.0
160.80	115.0
172.00	507.0
173.00	645.0
174.00	66840.0
175.00	5311.0
176.00	64664.0
177.00	4215.0
178.00	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
35.90	506.0
37.00	2584.0
38.00	2245.0
39.00	990.0
39.90	260.0
44.00	626.0
45.00	421.0
47.00	794.0
47.90	454.0
49.00	2271.0
50.10	11475.0
51.10	3390.0
52.00	197.0
55.10	169.0
56.00	939.0
57.00	1742.0
60.00	590.0
61.00	3103.0
62.10	2772.0
63.00	2314.0
63.90	400.0
65.00	425.0
67.10	160.0
68.00	6569.0
69.00	6806.0
70.00	521.0
72.00	373.0
73.00	2817.0
74.00	11334.0
75.00	32928.0
76.10	2983.0
76.90	455.0
78.00	331.0
79.00	1857.0
79.90	672.0
81.00	2099.0
81.90	407.0
87.00	3546.0
88.00	3478.0
90.90	323.0
92.00	1853.0
93.00	3103.0
94.10	8451.0
95.00	72568.0
96.10	4789.0
97.00	155.0
103.90	306.0
104.90	135.0
106.00	253.0
116.00	234.0
116.90	614.0
117.90	284.0
118.90	426.0
127.90	258.0
128.80	155.0
129.90	217.0
130.90	121.0
134.80	168.0
136.80	111.0
140.90	586.0
143.00	724.0
144.80	126.0
147.90	187.0
149.80	103.0
155.10	217.0
157.00	135.0
158.90	147.0
160.80	102.0
172.00	512.0
174.00	63352.0
175.00	4993.0
176.00	60864.0
177.00	3921.0
178.00	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358