




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033504.D
 Acq On : 20 Dec 2023 12:14
 Operator : SY/MD
 Sample : 05850-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7

Manual IntegrationsAPPROVED

Quant Time: Dec 21 01:45:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 21 01:43:54 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

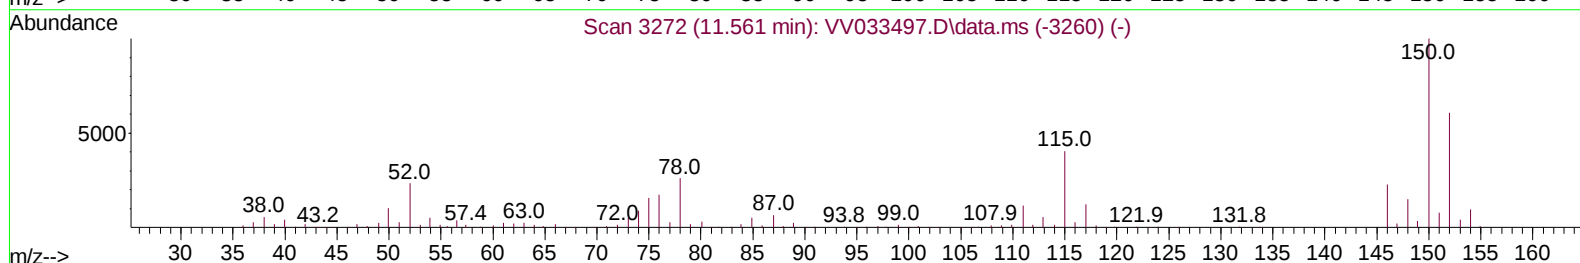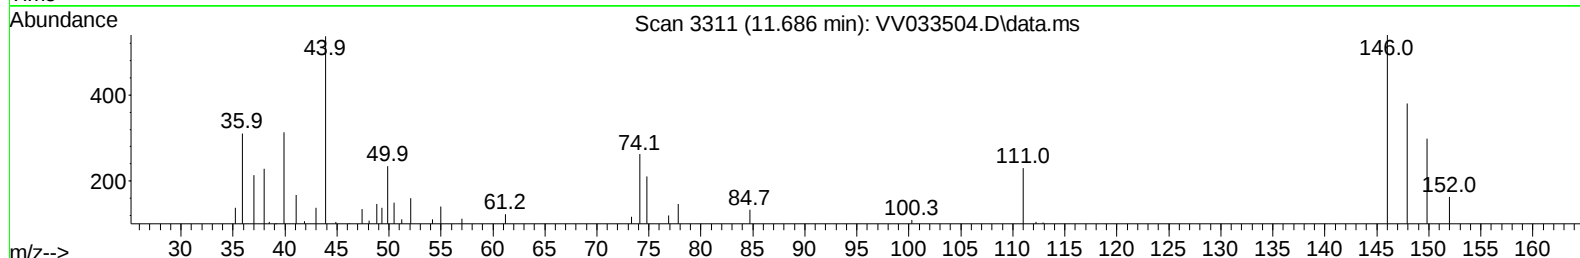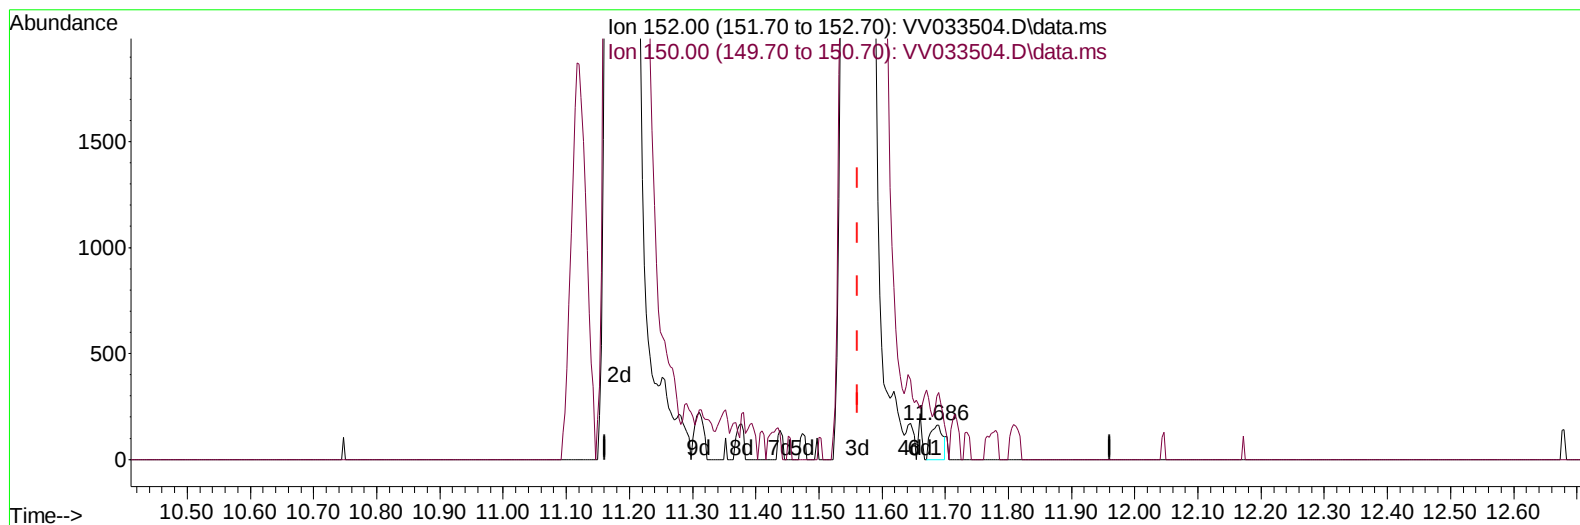

TIC: VV033504.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.686min (+ 0.125) 0.09 ug/L

response 229

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	171.50	134.93
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033504.D
 Acq On : 20 Dec 2023 12:14
 Operator : SY/MD
 Sample : 05850-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7

Manual IntegrationsAPPROVED

Quant Time: Dec 21 01:45:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 21 01:43:54 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

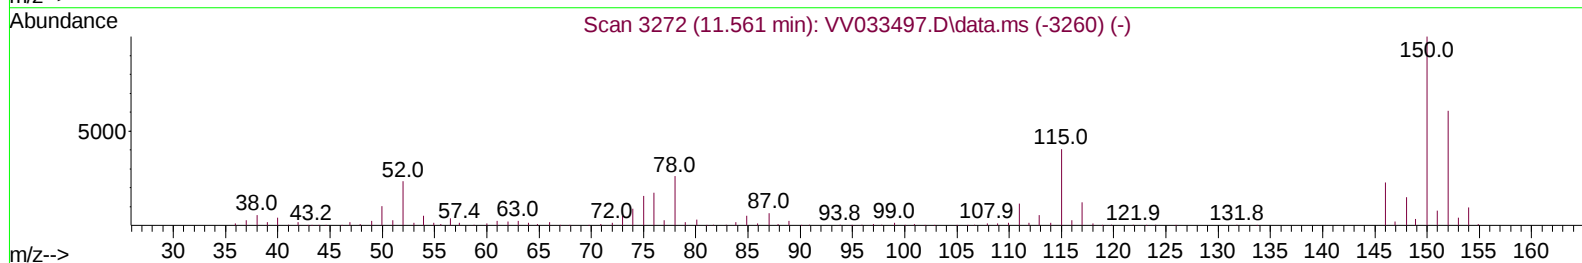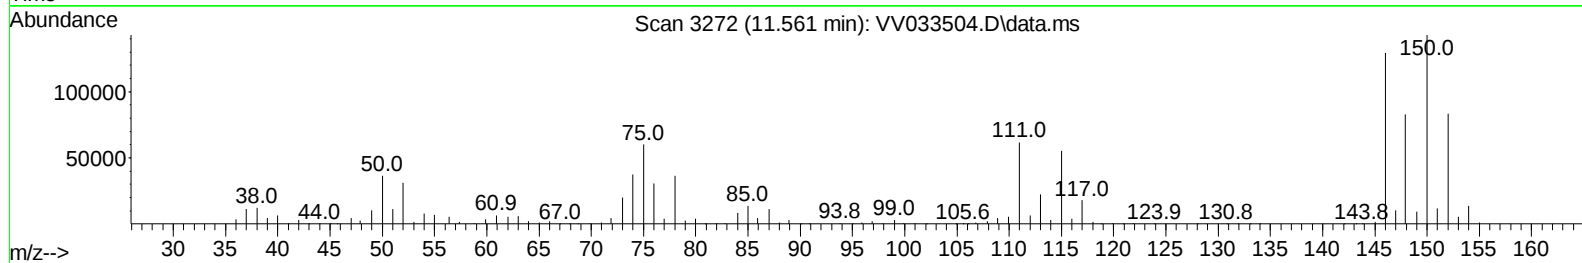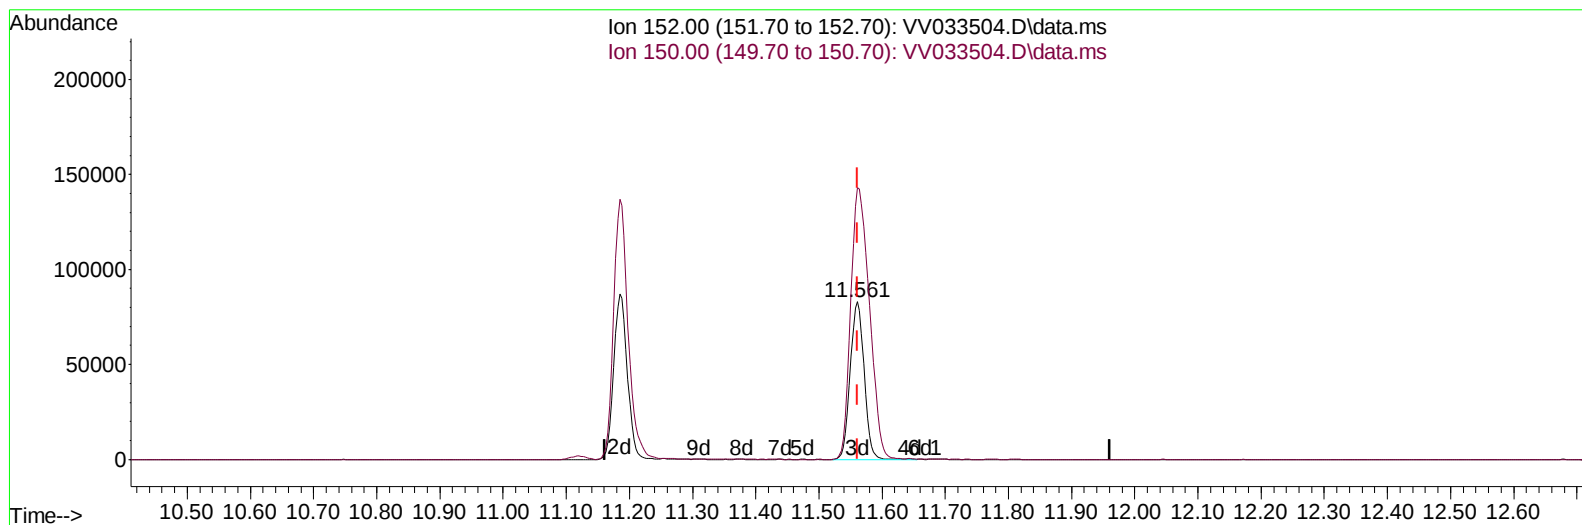

TIC: VV033504.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.561min (+ 0.000) 51.57 ug/L m

response 126737

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	171.50	0.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033504.D
 Acq On : 20 Dec 2023 12:14
 Operator : SY/MD
 Sample : 05850-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7

Manual IntegrationsAPPROVED

Quant Time: Dec 21 01:45:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 21 01:43:54 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	276049	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	292990	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	130773	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	102881	48.396	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	96.800%	
7) Chloroethane-d5	1.536	69	94636	49.606	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	99.220%	
11) 1,1-Dichloroethene-d2	2.063	65	47520	44.905	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.820%	
21) 2-Butanone-d5	3.786	46	94834	88.515	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	88.510%	
24) Chloroform-d	4.249	84	193082	45.916	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.840%	
26) 1,2-Dichloroethane-d4	4.941	65	124815	48.318	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.640%	
32) Benzene-d6	4.960	84	363962	46.123	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.240%	
36) 1,2-Dichloropropane-d6	5.989	67	118613	49.526	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	99.060%	
41) Toluene-d8	7.243	98	305036	42.246	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	84.500%	
43) trans-1,3-Dichloroprop...	7.551	79	49044	41.784	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	83.560%	
47) 2-Hexanone-d5	8.024	63	63635	78.997	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	79.000%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	147260	42.781	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.560%	
66) 1,2-Dichlorobenzene-d4	11.561	152	126737m	51.573	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	103.140%	
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	21840	17.561	ug/L	98
33) Benzene	5.011	78	13740	1.759	ug/L	100
51) Chlorobenzene	8.815	112	210384	35.269	ug/L	98
64) 1,3-Dichlorobenzene	11.120	146	34201	8.861	ug/L	98
65) 1,4-Dichlorobenzene	11.207	146	130945	31.523	ug/L	98
67) 1,2-Dichlorobenzene	11.577	146	957185	238.269	ug/L	98
70) 1,2,4-trichlorobenzene	13.198	180	181248	77.680	ug/L	99
72) 1,2,3-Trichlorobenzene	13.680	180	94485	41.400	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033504.D
Acq On : 20 Dec 2023 12:14
Operator : SY/MD
Sample : 05850-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/21/2023
Supervised By :Semsettin Yesilyurt 12/21/2023

Quant Time: Dec 21 01:45:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 21 01:43:54 2023
Response via : Initial Calibration

