

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033498.D
 Acq On : 20 Dec 2023 09:56
 Operator : SY/MD
 Sample : VV1220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK255

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	183088	192916	16.47%	2.181%
2	1.532	146	153	165	rVB	156386	180293	15.39%	2.038%
3	2.060	308	317	335	rBV	302313	436710	37.28%	4.936%
4	2.378	414	416	417	rBV2	1513	606	0.05%	0.007%
5	2.622	489	492	496	rBV6	991	814	0.07%	0.009%
6	2.651	500	501	505	rBV3	746	588	0.05%	0.007%
7	2.973	599	601	604	rBV3	936	568	0.05%	0.006%
8	3.011	611	613	618	rVB5	920	594	0.05%	0.007%
9	3.040	621	622	626	rBV4	827	534	0.05%	0.006%
10	3.098	637	640	641	rBV3	878	549	0.05%	0.006%
11	3.127	645	649	653	rVB3	1695	1185	0.10%	0.013%
12	3.147	653	655	657	rBV2	808	509	0.04%	0.006%
13	3.208	670	674	679	rBV6	1333	1508	0.13%	0.017%
14	3.320	706	709	710	rBV3	1533	978	0.08%	0.011%
15	3.394	729	732	734	rVB3	1252	828	0.07%	0.009%
16	3.433	739	744	745	rBV4	1200	940	0.08%	0.011%
17	3.555	778	782	784	rBV4	1077	852	0.07%	0.010%
18	3.658	809	814	815	rBV4	1144	676	0.06%	0.008%
19	3.716	830	832	834	rBV3	687	466	0.04%	0.005%
20	3.786	844	854	881	rBV	65005	188629	16.10%	2.132%
21	4.246	984	997	1019	rBV	180213	463493	39.57%	5.239%
22	4.500	1074	1076	1078	rBV3	1226	650	0.06%	0.007%
23	4.725	1144	1146	1149	rBV3	1207	580	0.05%	0.007%
24	4.741	1149	1151	1154	rBV4	1057	608	0.05%	0.007%
25	4.899	1196	1200	1202	rBV3	1534	1097	0.09%	0.012%
26	4.957	1202	1218	1247	rVV3	436636	1171325	100.00%	13.240%
27	5.465	1373	1376	1379	rBV5	1668	1229	0.10%	0.014%
28	5.532	1386	1397	1426	rBV	340946	709941	60.61%	8.025%
29	5.986	1527	1538	1564	rBV	253757	525349	44.85%	5.938%
30	6.497	1695	1697	1702	rBV6	1207	1074	0.09%	0.012%
31	6.593	1723	1727	1728	rBV3	1329	767	0.07%	0.009%
32	6.603	1728	1730	1733	rVB3	1270	606	0.05%	0.007%
33	6.822	1795	1798	1802	rBV5	803	684	0.06%	0.008%
34	6.912	1815	1826	1846	rBV2	121313	231349	19.75%	2.615%
35	7.243	1917	1929	1954	rBV	496106	886699	75.70%	10.022%
36	7.555	2017	2026	2047	rBV	85689	156788	13.39%	1.772%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033498.D
 Acq On : 20 Dec 2023 09:56
 Operator : SY/MD
 Sample : VV1220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK255

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.728	2078	2080	2082	rVB3	1898	890	0.08%	0.010%
38	7.879	2123	2127	2131	rBV7	1489	1332	0.11%	0.015%
39	7.915	2133	2138	2141	rBV7	1867	2088	0.18%	0.024%
40	8.024	2163	2172	2210	rBV2	215709	468786	40.02%	5.299%
41	8.368	2277	2279	2282	rBV4	1726	1072	0.09%	0.012%
42	8.503	2317	2321	2323	rBV5	1431	792	0.07%	0.009%
43	8.645	2362	2365	2366	rBV3	876	503	0.04%	0.006%
44	8.712	2383	2386	2392	rVB6	1604	1187	0.10%	0.013%
45	8.783	2394	2408	2434	rBV	549076	913902	78.02%	10.330%
46	9.330	2576	2578	2580	rBV2	1027	524	0.04%	0.006%
47	9.368	2588	2590	2592	rVB3	1390	595	0.05%	0.007%
48	9.481	2621	2625	2627	rBV4	2064	1518	0.13%	0.017%
49	9.574	2652	2654	2656	rVB3	1481	637	0.05%	0.007%
50	9.674	2682	2685	2687	rBV4	1266	717	0.06%	0.008%
51	9.722	2696	2700	2702	rBV3	928	708	0.06%	0.008%
52	9.834	2734	2735	2737	rBV	963	515	0.04%	0.006%
53	10.063	2803	2806	2807	rBV3	948	469	0.04%	0.005%
54	10.088	2812	2814	2818	rVB5	1000	587	0.05%	0.007%
55	10.153	2819	2834	2857	rBV	320407	524398	44.77%	5.927%
56	10.307	2880	2882	2884	rBV2	950	498	0.04%	0.006%
57	10.358	2895	2898	2899	rBV2	1063	574	0.05%	0.006%
58	10.397	2907	2910	2912	rBV3	1155	745	0.06%	0.008%
59	10.484	2928	2937	2942	rBV10	2413	3679	0.31%	0.042%
60	10.600	2971	2973	2977	rBV3	1268	1041	0.09%	0.012%
61	10.657	2986	2991	2994	rBV5	1316	1145	0.10%	0.013%
62	10.677	2994	2997	2999	rVV3	1263	859	0.07%	0.010%
63	10.776	3024	3028	3031	rBV6	963	778	0.07%	0.009%
64	10.802	3031	3036	3041	rVB8	1636	1896	0.16%	0.021%
65	10.825	3041	3043	3045	rBV3	1124	581	0.05%	0.007%
66	10.931	3075	3076	3080	rVB2	1018	500	0.04%	0.006%
67	10.985	3089	3093	3097	rVV6	787	641	0.05%	0.007%
68	11.014	3100	3102	3107	rBV5	1262	777	0.07%	0.009%
69	11.037	3107	3109	3112	rBV4	1185	742	0.06%	0.008%
70	11.127	3129	3137	3144	rBV10	4430	8202	0.70%	0.093%
71	11.185	3145	3155	3180	rVV	500772	799929	68.29%	9.042%
72	11.426	3226	3230	3231	rBV3	1113	605	0.05%	0.007%
73	11.436	3231	3233	3237	rVV4	768	544	0.05%	0.006%
74	11.561	3258	3272	3298	rBV	495371	796921	68.04%	9.008%
75	11.876	3367	3370	3373	rBV4	797	454	0.04%	0.005%
76	11.915	3380	3382	3384	rBV2	909	510	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033498.D
 Acq On : 20 Dec 2023 09:56
 Operator : SY/MD
 Sample : VV1220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK255

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.249	3482	3486	3490	rBV6	1697	974	0.08%	0.011%
78	12.374	3519	3525	3530	rVB7	2290	3143	0.27%	0.036%
79	12.403	3530	3534	3535	rBV4	1122	760	0.06%	0.009%
80	12.448	3545	3548	3552	rBV6	1065	793	0.07%	0.009%
81	12.506	3563	3566	3568	rVB3	1466	643	0.05%	0.007%
82	12.522	3568	3571	3573	rBV3	1102	656	0.06%	0.007%
83	12.590	3583	3592	3601	rBV7	7342	12097	1.03%	0.137%
84	12.744	3637	3640	3644	rBV6	1486	1617	0.14%	0.018%
85	12.850	3671	3673	3675	rBV2	1008	623	0.05%	0.007%
86	12.863	3675	3677	3686	rVB7	892	736	0.06%	0.008%
87	12.985	3709	3715	3717	rBV4	1667	1548	0.13%	0.017%
88	13.021	3724	3726	3729	rBV4	958	577	0.05%	0.007%
89	13.204	3774	3783	3794	rBV4	12421	21966	1.88%	0.248%
90	13.281	3802	3807	3811	rBV7	1055	1055	0.09%	0.012%
91	13.442	3848	3857	3867	rBV	34673	59390	5.07%	0.671%
92	13.683	3922	3932	3946	rBV6	16232	28843	2.46%	0.326%
93	13.853	3983	3985	3988	rBV3	1129	521	0.04%	0.006%
94	13.927	4006	4008	4010	rBV2	1215	671	0.06%	0.008%
95	14.316	4127	4129	4132	rVB3	1292	697	0.06%	0.008%
96	14.767	4267	4269	4272	rVB4	1209	635	0.05%	0.007%
97	14.927	4317	4319	4321	rBV2	1127	599	0.05%	0.007%
98	15.242	4415	4417	4420	rBV3	997	504	0.04%	0.006%
99	15.262	4421	4423	4427	rVB3	1120	738	0.06%	0.008%
100	15.329	4441	4444	4449	rBV7	1350	1503	0.13%	0.017%


Sum of corrected areas: 8847112

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033498.D
Acq On : 20 Dec 2023 09:56
Operator : SY/MD
Sample : VV1220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK255

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

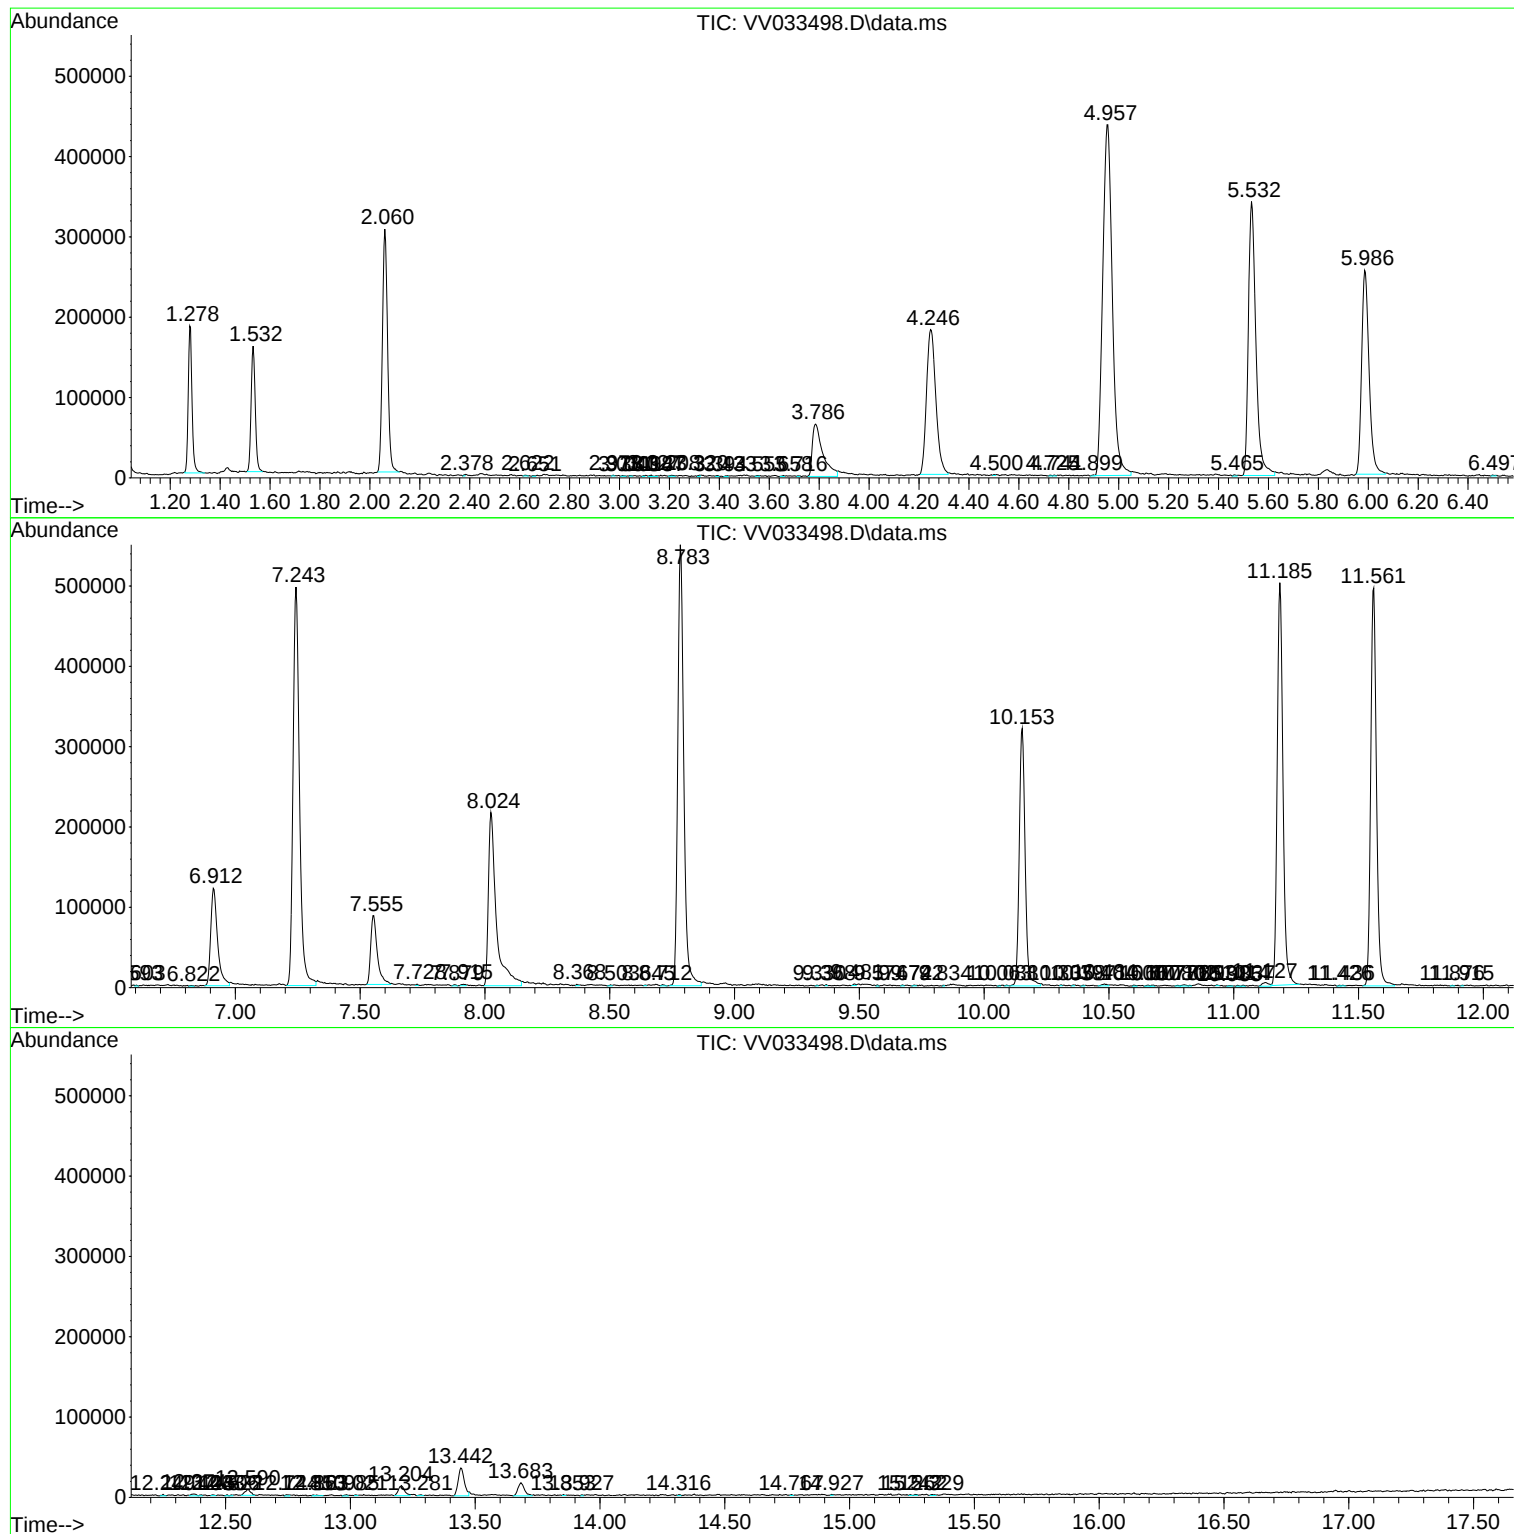

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033498.D
Acq On : 20 Dec 2023 09:56
Operator : SY/MD
Sample : VV1220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK255

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033498.D
Acq On : 20 Dec 2023 09:56
Operator : SY/MD
Sample : VV1220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK255

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc