

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033499.D
 Acq On : 20 Dec 2023 10:19
 Operator : SY/MD
 Sample : VV1220WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	176080	187393	16.37%	2.224%
2	1.532	146	153	167	rVB	150778	178598	15.60%	2.120%
3	2.060	308	317	337	rVB	285642	419673	36.67%	4.981%
4	2.478	445	447	451	rVB5	1379	600	0.05%	0.007%
5	2.513	456	458	461	rBV4	699	420	0.04%	0.005%
6	2.545	466	468	472	rBV3	1747	1430	0.12%	0.017%
7	2.944	590	592	596	rVB3	1304	844	0.07%	0.010%
8	2.999	605	609	610	rBV2	678	541	0.05%	0.006%
9	3.028	614	618	619	rBV4	1452	1024	0.09%	0.012%
10	3.076	630	633	636	rBV4	1939	1797	0.16%	0.021%
11	3.169	655	662	663	rBV6	1028	1088	0.10%	0.013%
12	3.285	695	698	703	rBV6	1583	1268	0.11%	0.015%
13	3.314	703	707	709	rBV4	1327	780	0.07%	0.009%
14	3.372	721	725	727	rBV4	1523	1135	0.10%	0.013%
15	3.404	733	735	738	rBV2	1124	671	0.06%	0.008%
16	3.529	768	774	776	rBV5	1241	1044	0.09%	0.012%
17	3.564	783	785	790	rVB6	925	669	0.06%	0.008%
18	3.632	803	806	809	rVV4	1013	655	0.06%	0.008%
19	3.648	809	811	814	rVB2	1743	829	0.07%	0.010%
20	3.783	845	853	877	rBV2	64395	178428	15.59%	2.118%
21	4.246	985	997	1024	rVB	178264	451388	39.44%	5.357%
22	4.802	1167	1170	1172	rVB3	879	476	0.04%	0.006%
23	4.822	1172	1176	1179	rBV6	809	719	0.06%	0.009%
24	4.957	1198	1218	1244	rBV2	426450	1144604	100.00%	13.584%
25	5.535	1386	1398	1422	rBV	323120	675549	59.02%	8.018%
26	5.989	1525	1539	1562	rBV	248502	525070	45.87%	6.232%
27	6.433	1674	1677	1679	rVB3	1187	715	0.06%	0.008%
28	6.471	1684	1689	1691	rVV5	1437	990	0.09%	0.012%
29	6.529	1705	1707	1710	rVB3	1566	712	0.06%	0.008%
30	6.551	1710	1714	1715	rBV3	1809	1247	0.11%	0.015%
31	6.593	1724	1727	1730	rBV4	1281	1055	0.09%	0.013%
32	6.741	1771	1773	1779	rVB6	1187	754	0.07%	0.009%
33	6.844	1801	1805	1808	rBV4	1207	896	0.08%	0.011%
34	6.912	1817	1826	1847	rBV2	115119	220598	19.27%	2.618%
35	7.156	1900	1902	1904	rBV3	1448	724	0.06%	0.009%
36	7.243	1918	1929	1951	rBV	473837	845587	73.88%	10.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033499.D
 Acq On : 20 Dec 2023 10:19
 Operator : SY/MD
 Sample : VV1220WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.481	2001	2003	2006	rBV4	1462	926	0.08%	0.011%
38	7.555	2017	2026	2047	rBV2	84775	156737	13.69%	1.860%
39	7.828	2108	2111	2113	rVB4	896	482	0.04%	0.006%
40	7.908	2132	2136	2141	rBV7	2125	1913	0.17%	0.023%
41	7.969	2152	2155	2157	rBV4	1482	1023	0.09%	0.012%
42	8.024	2163	2172	2212	rBV	207825	455571	39.80%	5.407%
43	8.712	2383	2386	2389	rBV3	766	548	0.05%	0.007%
44	8.731	2389	2392	2394	rBV3	1172	814	0.07%	0.010%
45	8.783	2398	2408	2431	rBV	532653	872308	76.21%	10.353%
46	9.124	2510	2514	2515	rBV4	1008	712	0.06%	0.008%
47	9.281	2562	2563	2566	rBV2	858	442	0.04%	0.005%
48	9.355	2582	2586	2587	rBV4	793	528	0.05%	0.006%
49	9.416	2603	2605	2607	rVV2	756	462	0.04%	0.005%
50	9.465	2617	2620	2622	rBV4	933	604	0.05%	0.007%
51	9.564	2647	2651	2652	rBV5	1461	885	0.08%	0.011%
52	9.625	2666	2670	2672	rBV4	1362	960	0.08%	0.011%
53	9.767	2710	2714	2716	rBV4	905	820	0.07%	0.010%
54	9.834	2733	2735	2737	rBV2	819	438	0.04%	0.005%
55	9.928	2762	2764	2767	rBV2	976	424	0.04%	0.005%
56	10.018	2788	2792	2796	rBV7	1142	984	0.09%	0.012%
57	10.153	2819	2834	2860	rVV	316323	513938	44.90%	6.100%
58	10.452	2925	2927	2932	rVB6	1248	965	0.08%	0.011%
59	10.513	2943	2946	2948	rBV3	737	437	0.04%	0.005%
60	10.558	2958	2960	2964	rBV5	1036	637	0.06%	0.008%
61	10.651	2987	2989	2990	rBV2	1005	534	0.05%	0.006%
62	10.690	2997	3001	3004	rBV6	1141	910	0.08%	0.011%
63	10.831	3042	3045	3049	rBV4	1206	856	0.07%	0.010%
64	10.857	3049	3053	3055	rBV6	1279	1058	0.09%	0.013%
65	11.053	3111	3114	3116	rBV3	707	492	0.04%	0.006%
66	11.092	3122	3126	3129	rBV4	694	648	0.06%	0.008%
67	11.185	3145	3155	3177	rBV	483286	751071	65.62%	8.914%
68	11.513	3253	3257	3258	rBV4	1124	894	0.08%	0.011%
69	11.561	3260	3272	3289	rVV	480199	761576	66.54%	9.039%
70	11.850	3360	3362	3365	rVB3	949	528	0.05%	0.006%
71	11.870	3365	3368	3370	rBV4	1011	620	0.05%	0.007%
72	12.345	3511	3516	3518	rBV3	825	804	0.07%	0.010%
73	12.445	3544	3547	3548	rBV3	826	503	0.04%	0.006%
74	12.477	3554	3557	3564	rVB5	885	906	0.08%	0.011%
75	12.673	3615	3618	3619	rBV	998	574	0.05%	0.007%
76	12.760	3641	3645	3647	rBV5	805	793	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033499.D
 Acq On : 20 Dec 2023 10:19
 Operator : SY/MD
 Sample : VV1220WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.805	3656	3659	3665	rBV5	972	906	0.08%	0.011%
78	12.863	3672	3677	3679	rBV5	1206	999	0.09%	0.012%
79	12.911	3689	3692	3694	rVB4	731	435	0.04%	0.005%
80	12.924	3694	3696	3697	rBV2	1066	483	0.04%	0.006%
81	12.944	3701	3702	3704	rBV2	1122	489	0.04%	0.006%
82	12.985	3712	3715	3719	rBV5	1091	737	0.06%	0.009%
83	13.162	3767	3770	3774	rBV5	1026	993	0.09%	0.012%
84	13.204	3777	3783	3791	rVB10	4721	7063	0.62%	0.084%
85	13.291	3807	3810	3812	rVV4	870	485	0.04%	0.006%
86	13.336	3823	3824	3828	rVB4	907	505	0.04%	0.006%
87	13.448	3850	3859	3871	rVB3	10141	17405	1.52%	0.207%
88	13.567	3893	3896	3898	rBV4	1064	651	0.06%	0.008%
89	13.879	3991	3993	3996	rBV3	786	530	0.05%	0.006%
90	13.895	3996	3998	4001	rVV4	1064	653	0.06%	0.008%
91	14.017	4033	4036	4038	rBV4	1045	807	0.07%	0.010%
92	14.079	4052	4055	4057	rBV5	1315	973	0.09%	0.012%
93	14.262	4110	4112	4114	rBV3	833	508	0.04%	0.006%
94	14.381	4146	4149	4150	rBV3	1176	599	0.05%	0.007%
95	14.406	4155	4157	4161	rBV5	930	824	0.07%	0.010%
96	14.564	4204	4206	4208	rBV3	1283	501	0.04%	0.006%
97	14.812	4279	4283	4284	rBV3	945	618	0.05%	0.007%
98	14.950	4324	4326	4332	rVB5	1499	757	0.07%	0.009%
99	14.979	4332	4335	4336	rBV3	1273	670	0.06%	0.008%
100	15.085	4365	4368	4370	rBV3	1838	1002	0.09%	0.012%


Sum of corrected areas: 8425889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033499.D
Acq On : 20 Dec 2023 10:19
Operator : SY/MD
Sample : VV1220WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

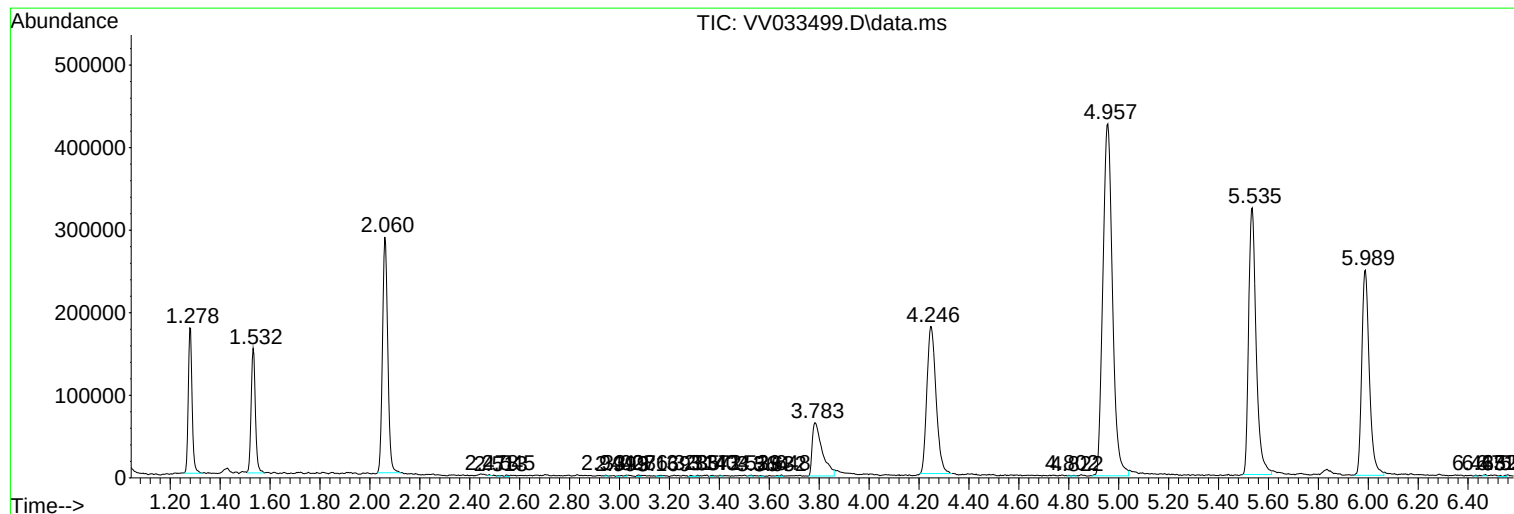

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033499.D
Acq On : 20 Dec 2023 10:19
Operator : SY/MD
Sample : VV1220WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033499.D
Acq On : 20 Dec 2023 10:19
Operator : SY/MD
Sample : VV1220WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------