

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033501.D
 Acq On : 20 Dec 2023 11:06
 Operator : SY/MD
 Sample : 05927-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rBV	160579	165814	15.27%	2.059%
2	1.532	146	153	165	rVB	137607	161582	14.88%	2.007%
3	2.059	309	317	329	rBV	260388	373959	34.43%	4.645%
4	2.423	428	430	432	rBV3	1069	613	0.06%	0.008%
5	2.526	459	462	463	rBV2	1005	555	0.05%	0.007%
6	2.535	463	465	467	rVV3	1095	501	0.05%	0.006%
7	2.693	510	514	515	rBV3	872	580	0.05%	0.007%
8	2.905	577	580	582	rBV4	1264	512	0.05%	0.006%
9	3.011	611	613	619	rVB6	930	730	0.07%	0.009%
10	3.053	619	626	629	rBV5	1493	1492	0.14%	0.019%
11	3.133	647	651	654	rBV5	1163	796	0.07%	0.010%
12	3.230	678	681	683	rBV4	889	451	0.04%	0.006%
13	3.243	683	685	688	rVB4	1006	518	0.05%	0.006%
14	3.262	688	691	693	rBV3	1562	829	0.08%	0.010%
15	3.339	712	715	717	rBV3	1016	658	0.06%	0.008%
16	3.378	725	727	731	rBV5	1044	938	0.09%	0.012%
17	3.426	740	742	744	rBV2	1030	691	0.06%	0.009%
18	3.487	759	761	766	rVB5	1216	565	0.05%	0.007%
19	3.545	776	779	780	rBV	1141	513	0.05%	0.006%
20	3.600	792	796	797	rBV4	696	496	0.05%	0.006%
21	3.645	806	810	813	rVB5	1813	1412	0.13%	0.018%
22	3.667	813	817	818	rBV3	785	447	0.04%	0.006%
23	3.783	845	853	883	rBV	59516	171213	15.76%	2.127%
24	4.249	985	998	1024	rVB	166705	428428	39.44%	5.321%
25	4.735	1147	1149	1151	rBV3	803	501	0.05%	0.006%
26	4.957	1203	1218	1252	rVV2	402950	1086226	100.00%	13.491%
27	5.194	1290	1292	1295	rBV4	1395	871	0.08%	0.011%
28	5.490	1381	1384	1386	rBV2	1410	956	0.09%	0.012%
29	5.532	1386	1397	1428	rVV	308583	658906	60.66%	8.184%
30	5.989	1527	1539	1563	rBV	237112	496352	45.70%	6.165%
31	6.413	1667	1671	1672	rBV4	1375	886	0.08%	0.011%
32	6.596	1725	1728	1729	rBV3	1651	899	0.08%	0.011%
33	6.764	1778	1780	1785	rBV4	978	851	0.08%	0.011%
34	6.911	1816	1826	1848	rBV	114827	222484	20.48%	2.763%
35	7.130	1890	1894	1896	rBV4	929	793	0.07%	0.010%
36	7.243	1918	1929	1950	rBV	453611	810908	74.65%	10.072%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033501.D
 Acq On : 20 Dec 2023 11:06
 Operator : SY/MD
 Sample : 05927-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.445	1990	1992	1994	rBV3	1543	647	0.06%	0.008%
38	7.551	2016	2025	2046	rBV	82540	157467	14.50%	1.956%
39	7.834	2111	2113	2115	rBV3	945	474	0.04%	0.006%
40	7.876	2120	2126	2129	rVV8	2321	2955	0.27%	0.037%
41	8.024	2163	2172	2206	rBV	198716	431493	39.72%	5.359%
42	8.689	2375	2379	2381	rVB4	1408	874	0.08%	0.011%
43	8.783	2396	2408	2440	rBV	501354	854282	78.65%	10.610%
44	9.185	2531	2533	2537	rVB4	1027	663	0.06%	0.008%
45	9.259	2551	2556	2559	rBV5	1530	1506	0.14%	0.019%
46	9.342	2580	2582	2585	rVB3	1381	869	0.08%	0.011%
47	9.484	2622	2626	2627	rBV3	2319	1279	0.12%	0.016%
48	9.657	2673	2680	2699	rBV10	6351	15756	1.45%	0.196%
49	10.046	2798	2801	2805	rBV4	1466	1080	0.10%	0.013%
50	10.152	2823	2834	2852	rBV	300331	479931	44.18%	5.961%
51	10.287	2874	2876	2877	rBV3	900	438	0.04%	0.005%
52	10.397	2906	2910	2913	rBV6	1220	1141	0.11%	0.014%
53	10.525	2947	2950	2952	rBV3	1377	956	0.09%	0.012%
54	10.561	2960	2961	2965	rBV5	1141	656	0.06%	0.008%
55	10.664	2990	2993	2995	rVB3	1435	617	0.06%	0.008%
56	10.696	3001	3003	3008	rBV5	937	454	0.04%	0.006%
57	10.857	3049	3053	3054	rBV4	1151	698	0.06%	0.009%
58	10.902	3065	3067	3069	rBV3	898	448	0.04%	0.006%
59	11.056	3112	3115	3121	rVB6	1882	1630	0.15%	0.020%
60	11.120	3132	3135	3140	rBV7	1649	1939	0.18%	0.024%
61	11.185	3144	3155	3177	rBV	468258	733215	67.50%	9.107%
62	11.461	3236	3241	3242	rBV5	1048	891	0.08%	0.011%
63	11.561	3261	3272	3291	rBV	461327	731135	67.31%	9.081%
64	11.767	3333	3336	3339	rBV5	1300	1201	0.11%	0.015%
65	11.902	3375	3378	3382	rBV4	1258	741	0.07%	0.009%
66	12.024	3414	3416	3418	rVB3	1236	438	0.04%	0.005%
67	12.082	3431	3434	3435	rBV2	998	524	0.05%	0.007%
68	12.127	3445	3448	3450	rBV4	1341	736	0.07%	0.009%
69	12.201	3466	3471	3472	rBV4	1233	949	0.09%	0.012%
70	12.242	3482	3484	3488	rVB4	1516	662	0.06%	0.008%
71	12.348	3514	3517	3519	rVB2	1383	786	0.07%	0.010%
72	12.361	3519	3521	3523	rBV3	1059	504	0.05%	0.006%
73	12.374	3523	3525	3528	rBV4	1370	1005	0.09%	0.012%
74	12.471	3554	3555	3561	rVB4	1304	1119	0.10%	0.014%
75	12.545	3576	3578	3580	rBV3	1018	555	0.05%	0.007%
76	12.622	3598	3602	3605	rBV6	1344	857	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033501.D
 Acq On : 20 Dec 2023 11:06
 Operator : SY/MD
 Sample : 05927-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.648	3608	3610	3615	rBV4	764	658	0.06%	0.008%
78	12.924	3693	3696	3700	rVB3	1259	760	0.07%	0.009%
79	12.975	3709	3712	3717	rBV6	1083	1102	0.10%	0.014%
80	12.998	3717	3719	3722	rVB4	960	440	0.04%	0.005%
81	13.062	3737	3739	3741	rVB2	974	447	0.04%	0.006%
82	13.207	3777	3784	3788	rBV8	2704	3353	0.31%	0.042%
83	13.326	3819	3821	3824	rBV2	1038	668	0.06%	0.008%
84	13.355	3828	3830	3832	rBV3	993	522	0.05%	0.006%
85	13.442	3855	3857	3860	rBV4	2427	1749	0.16%	0.022%
86	13.535	3881	3886	3889	rBV7	1047	843	0.08%	0.010%
87	13.644	3914	3920	3924	rBV9	995	1187	0.11%	0.015%
88	13.664	3924	3926	3928	rBV3	1241	630	0.06%	0.008%
89	13.676	3928	3930	3931	rBV2	1667	808	0.07%	0.010%
90	13.747	3950	3952	3955	rVB4	1530	737	0.07%	0.009%
91	13.763	3955	3957	3959	rBV2	1123	726	0.07%	0.009%
92	13.966	4015	4020	4021	rBV5	1500	918	0.08%	0.011%
93	14.046	4042	4045	4048	rBV5	1141	911	0.08%	0.011%
94	14.390	4150	4152	4155	rBV3	1529	862	0.08%	0.011%
95	14.435	4162	4166	4167	rBV3	1345	899	0.08%	0.011%
96	14.612	4218	4221	4223	rBV3	1439	772	0.07%	0.010%
97	14.827	4284	4288	4290	rBV5	787	704	0.06%	0.009%
98	15.361	4450	4454	4455	rBV3	1715	982	0.09%	0.012%
99	15.512	4497	4501	4504	rBV5	1582	1535	0.14%	0.019%
100	15.818	4594	4596	4599	rBV3	1303	656	0.06%	0.008%


Sum of corrected areas: 8051366

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033501.D
Acq On : 20 Dec 2023 11:06
Operator : SY/MD
Sample : 05927-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

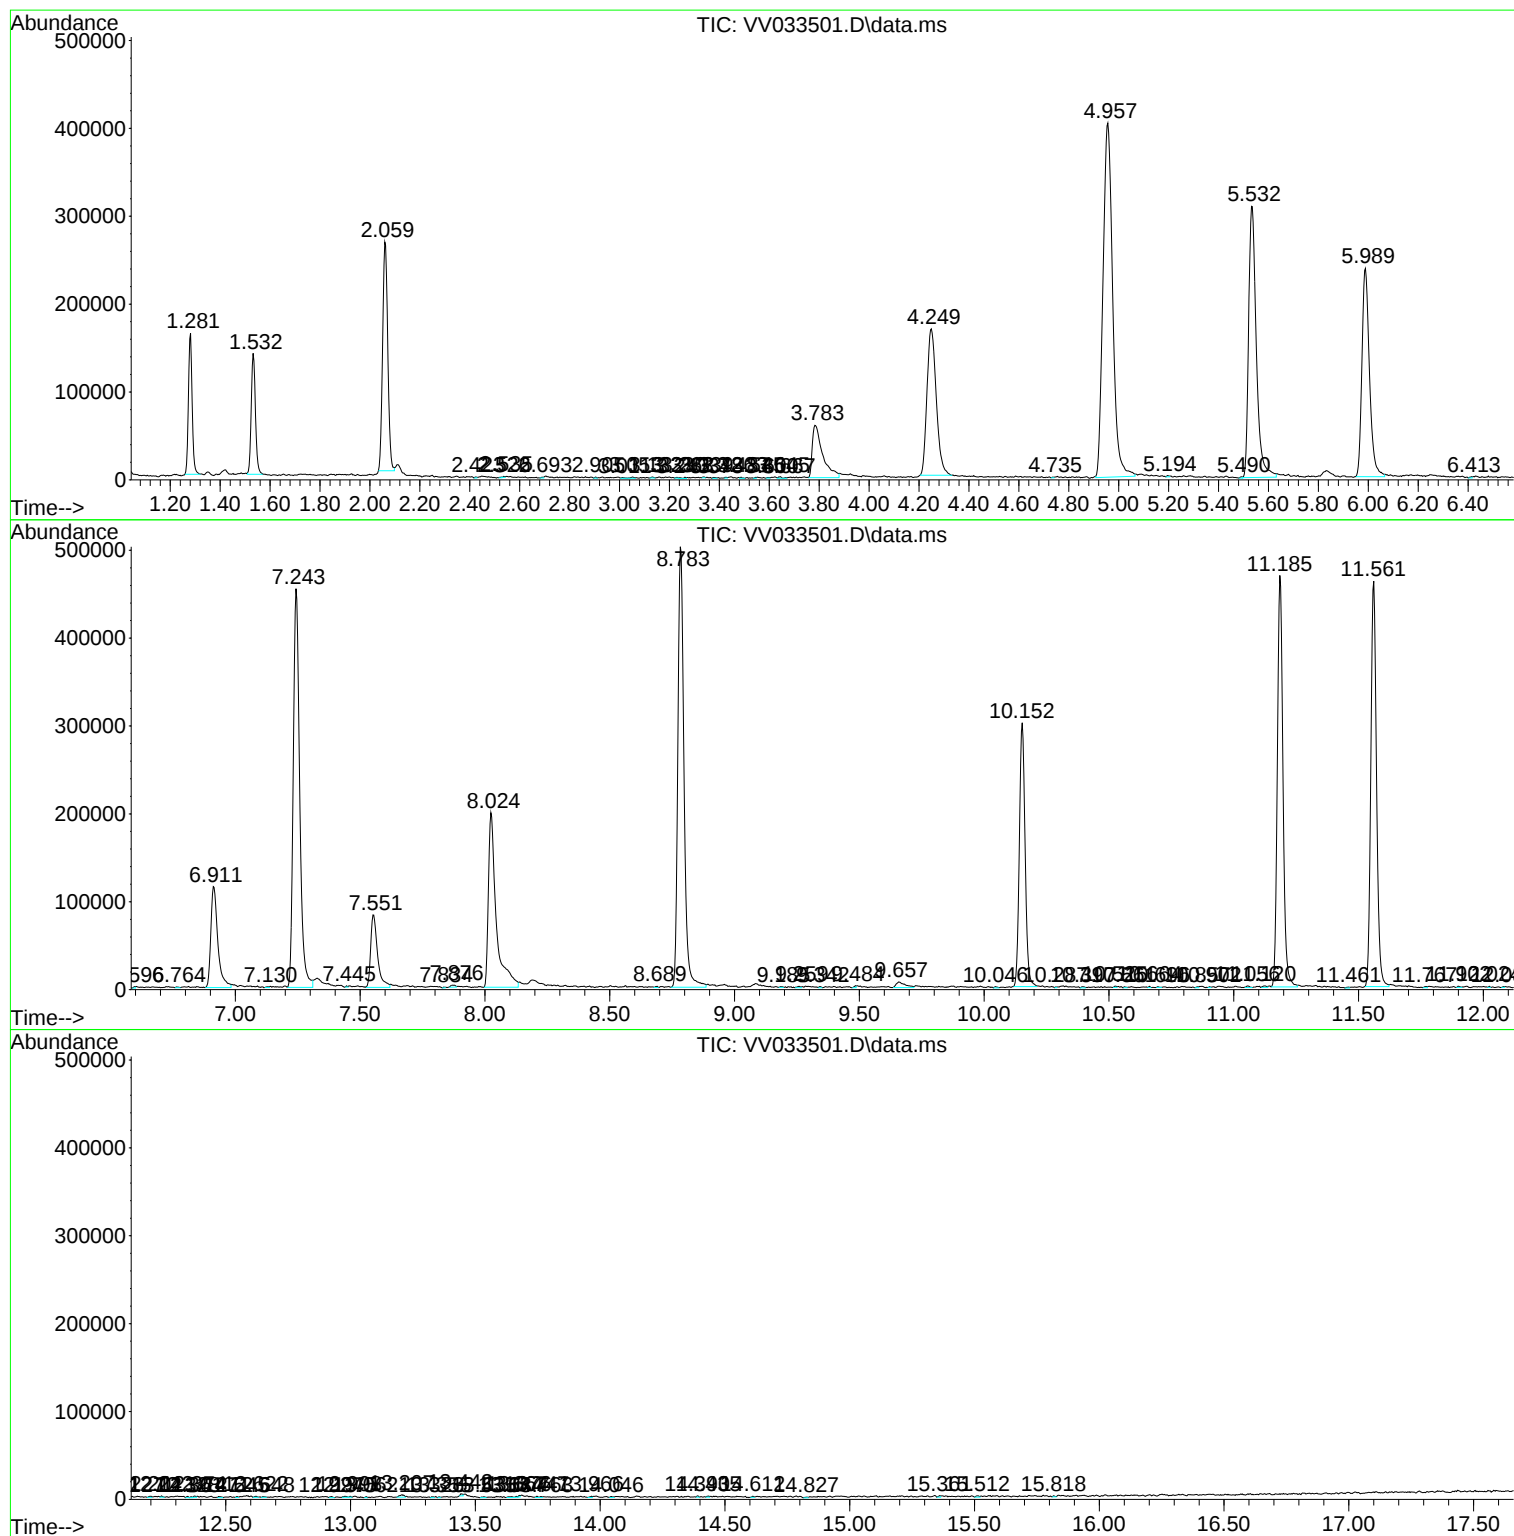

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033501.D
Acq On : 20 Dec 2023 11:06
Operator : SY/MD
Sample : 05927-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033501.D
Acq On : 20 Dec 2023 11:06
Operator : SY/MD
Sample : 05927-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc