

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033502.D
 Acq On : 20 Dec 2023 11:28
 Operator : SY/MD
 Sample : 05927-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	159216	166603	15.06%	2.025%
2	1.532	146	153	164	rVB	139037	162696	14.70%	1.978%
3	2.063	309	318	332	rBV	263410	386959	34.97%	4.704%
4	2.314	392	396	398	rBV4	1505	939	0.08%	0.011%
5	2.413	422	427	430	rBV6	1385	1282	0.12%	0.016%
6	2.892	573	576	581	rBV5	1049	989	0.09%	0.012%
7	3.011	609	613	617	rBV7	937	726	0.07%	0.009%
8	3.156	656	658	660	rBV2	983	555	0.05%	0.007%
9	3.294	698	701	703	rVB3	1014	506	0.05%	0.006%
10	3.336	711	714	720	rVB6	1586	1523	0.14%	0.019%
11	3.372	720	725	726	rBV4	1208	1025	0.09%	0.012%
12	3.413	737	738	742	rVB4	1058	571	0.05%	0.007%
13	3.433	742	744	747	rVB3	1067	512	0.05%	0.006%
14	3.535	774	776	779	rBV4	1417	743	0.07%	0.009%
15	3.635	805	807	810	rVB4	1323	557	0.05%	0.007%
16	3.751	838	843	844	rBV5	1102	746	0.07%	0.009%
17	3.786	846	854	881	rVV	57354	162622	14.70%	1.977%
18	4.191	977	980	981	rBV3	860	495	0.04%	0.006%
19	4.249	984	998	1030	rVB2	175891	460648	41.63%	5.600%
20	4.635	1116	1118	1121	rBV4	1378	768	0.07%	0.009%
21	4.876	1190	1193	1194	rBV3	1000	494	0.04%	0.006%
22	4.957	1202	1218	1241	rBV2	419919	1106514	100.00%	13.452%
23	5.429	1363	1365	1368	rVB3	1802	757	0.07%	0.009%
24	5.487	1379	1383	1385	rBV5	934	857	0.08%	0.010%
25	5.535	1387	1398	1424	rVV	315201	666215	60.21%	8.099%
26	5.789	1474	1477	1481	rBV5	1558	1023	0.09%	0.012%
27	5.989	1523	1539	1567	rBV	247713	523995	47.36%	6.370%
28	6.375	1656	1659	1660	rBV3	1298	715	0.06%	0.009%
29	6.452	1678	1683	1686	rBV7	1165	1180	0.11%	0.014%
30	6.497	1693	1697	1699	rBV4	994	820	0.07%	0.010%
31	6.584	1721	1724	1725	rBV3	1627	728	0.07%	0.009%
32	6.654	1744	1746	1752	rVB5	1569	1514	0.14%	0.018%
33	6.680	1752	1754	1756	rVB2	1043	568	0.05%	0.007%
34	6.751	1774	1776	1780	rBV5	1327	1144	0.10%	0.014%
35	6.809	1791	1794	1796	rBV3	826	498	0.05%	0.006%
36	6.915	1817	1827	1847	rBV2	115341	223933	20.24%	2.722%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033502.D
 Acq On : 20 Dec 2023 11:28
 Operator : SY/MD
 Sample : 05927-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.182	1905	1910	1914	rBV8	1564	1616	0.15%	0.020%
38	7.243	1918	1929	1950	rBV	462959	825927	74.64%	10.041%
39	7.555	2017	2026	2049	rBV	84019	159134	14.38%	1.935%
40	7.838	2110	2114	2117	rBV5	1200	979	0.09%	0.012%
41	7.876	2117	2126	2135	rBV2	16562	28537	2.58%	0.347%
42	7.960	2147	2152	2157	rBV9	1343	1258	0.11%	0.015%
43	8.024	2161	2172	2190	rBV	184671	370679	33.50%	4.506%
44	8.654	2366	2368	2371	rVB3	1208	632	0.06%	0.008%
45	8.731	2388	2392	2394	rBV4	1012	774	0.07%	0.009%
46	8.786	2398	2409	2433	rBV	524870	873107	78.91%	10.614%
47	9.047	2487	2490	2494	rBV5	1916	1332	0.12%	0.016%
48	9.217	2539	2543	2545	rBV4	1196	967	0.09%	0.012%
49	9.262	2554	2557	2559	rBV4	941	666	0.06%	0.008%
50	9.403	2598	2601	2604	rVB3	1287	704	0.06%	0.009%
51	9.423	2604	2607	2609	rBV4	1284	685	0.06%	0.008%
52	9.461	2617	2619	2621	rBV3	1327	807	0.07%	0.010%
53	9.587	2656	2658	2662	rBV4	801	642	0.06%	0.008%
54	9.670	2679	2684	2687	rBV4	2382	2395	0.22%	0.029%
55	9.818	2728	2730	2734	rBV3	1316	962	0.09%	0.012%
56	9.934	2763	2766	2768	rBV4	1142	750	0.07%	0.009%
57	10.014	2784	2791	2793	rBV5	1539	1325	0.12%	0.016%
58	10.153	2819	2834	2858	rBV	309248	492175	44.48%	5.983%
59	10.329	2882	2889	2899	rVB3	19310	32244	2.91%	0.392%
60	10.448	2923	2926	2928	rBV3	1041	633	0.06%	0.008%
61	10.587	2967	2969	2972	rBV4	1077	613	0.06%	0.007%
62	10.715	3006	3009	3010	rBV3	1022	532	0.05%	0.006%
63	10.735	3010	3015	3016	rVV4	1087	829	0.07%	0.010%
64	10.837	3045	3047	3051	rBV4	999	703	0.06%	0.009%
65	10.902	3066	3067	3071	rVB3	1179	663	0.06%	0.008%
66	10.953	3081	3083	3085	rBV3	986	530	0.05%	0.006%
67	11.108	3129	3131	3134	rVB3	1114	532	0.05%	0.006%
68	11.185	3143	3155	3177	rBV	492045	762781	68.94%	9.273%
69	11.387	3216	3218	3223	rBV5	984	740	0.07%	0.009%
70	11.561	3261	3272	3290	rVV	475954	750024	67.78%	9.118%
71	11.696	3312	3314	3319	rVB5	1909	1333	0.12%	0.016%
72	11.718	3319	3321	3324	rBV4	1121	751	0.07%	0.009%
73	12.133	3445	3450	3452	rBV6	1375	1194	0.11%	0.015%
74	12.374	3522	3525	3528	rBV4	1168	915	0.08%	0.011%
75	12.403	3531	3534	3535	rBV3	878	514	0.05%	0.006%
76	12.439	3540	3545	3548	rBV4	746	797	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033502.D
 Acq On : 20 Dec 2023 11:28
 Operator : SY/MD
 Sample : 05927-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.455	3548	3550	3553	rVB4	1159	543	0.05%	0.007%
78	12.580	3584	3589	3590	rBV5	1115	908	0.08%	0.011%
79	12.667	3614	3616	3618	rBV4	881	533	0.05%	0.006%
80	12.773	3646	3649	3652	rBV4	960	597	0.05%	0.007%
81	12.927	3692	3697	3698	rBV5	1093	890	0.08%	0.011%
82	12.969	3708	3710	3714	rVB3	1182	635	0.06%	0.008%
83	12.992	3714	3717	3719	rBV3	877	477	0.04%	0.006%
84	13.111	3751	3754	3756	rBV3	1329	931	0.08%	0.011%
85	13.201	3778	3782	3783	rBV4	1405	944	0.09%	0.011%
86	13.239	3790	3794	3796	rBV4	949	728	0.07%	0.009%
87	13.352	3826	3829	3831	rBV4	1009	584	0.05%	0.007%
88	13.445	3855	3858	3859	rBV3	2414	1345	0.12%	0.016%
89	13.715	3941	3942	3945	rVB3	1262	576	0.05%	0.007%
90	13.734	3945	3948	3955	rBV6	1272	1389	0.13%	0.017%
91	13.837	3978	3980	3983	rBV4	1171	776	0.07%	0.009%
92	13.988	4023	4027	4029	rBV4	1617	1338	0.12%	0.016%
93	14.156	4076	4079	4084	rBV5	1307	1162	0.11%	0.014%
94	14.252	4105	4109	4113	rBV6	1557	1757	0.16%	0.021%
95	14.416	4155	4160	4164	rBV7	1211	1425	0.13%	0.017%
96	14.876	4300	4303	4304	rBV3	1081	596	0.05%	0.007%
97	14.927	4317	4319	4322	rBV2	1119	703	0.06%	0.009%
98	15.104	4371	4374	4375	rBV4	1223	627	0.06%	0.008%
99	15.377	4457	4459	4462	rBV4	1448	896	0.08%	0.011%
100	15.628	4536	4537	4539	rBV2	1324	515	0.05%	0.006%




Sum of corrected areas: 8225676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033502.D
Acq On : 20 Dec 2023 11:28
Operator : SY/MD
Sample : 05927-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

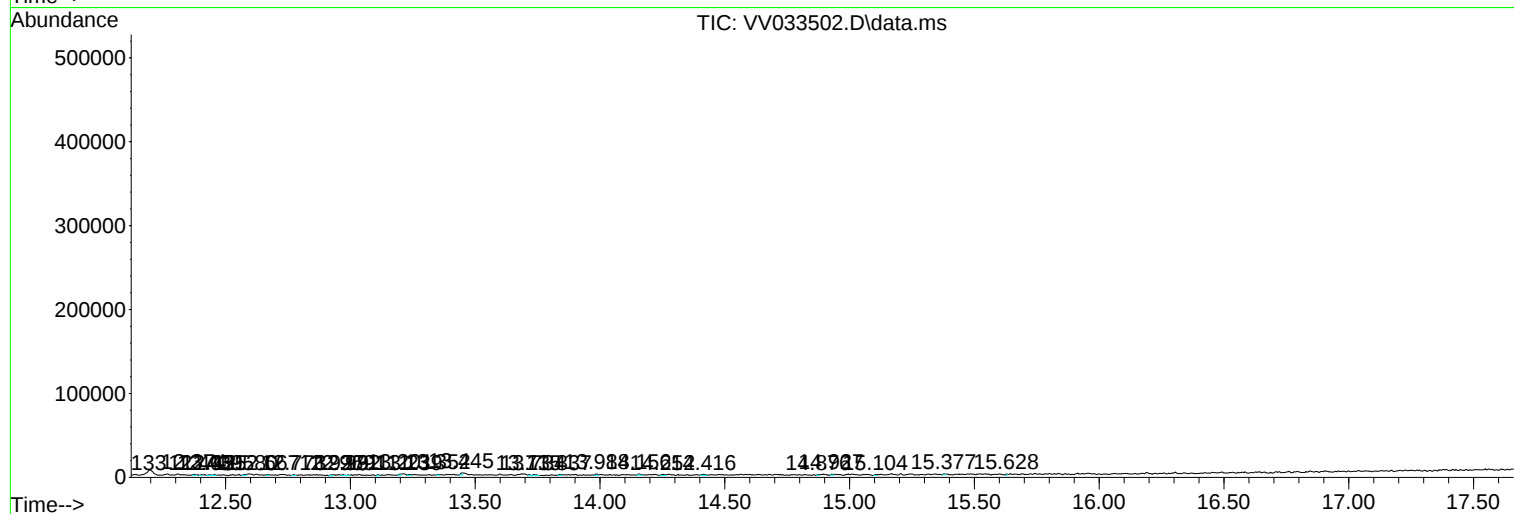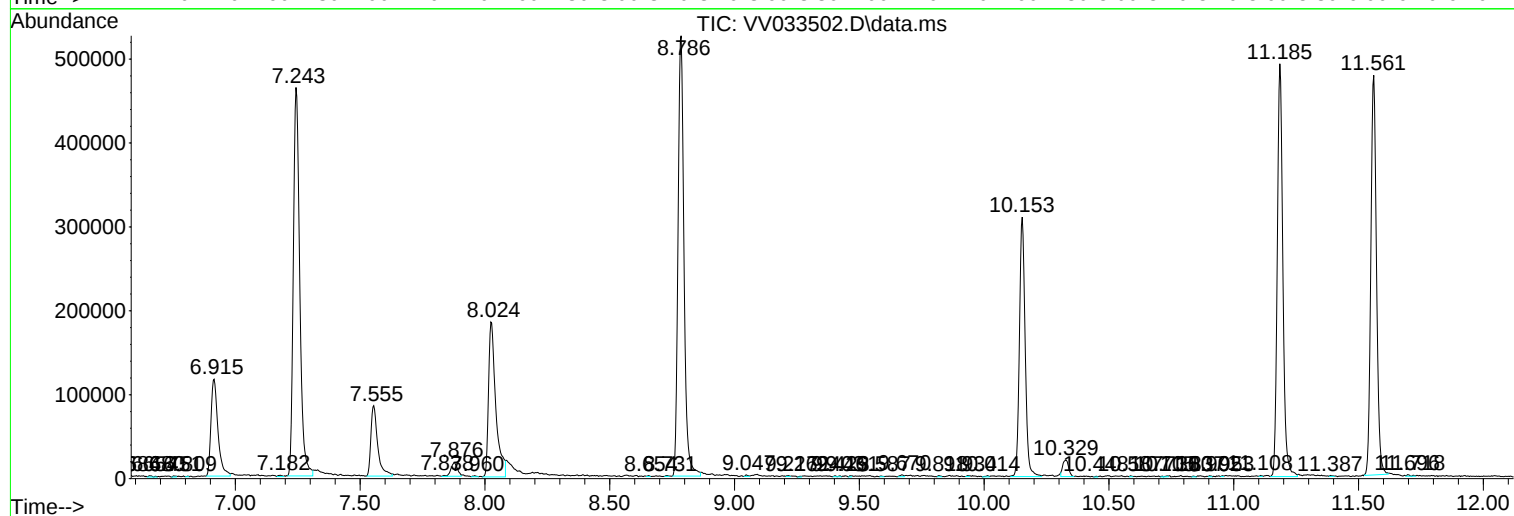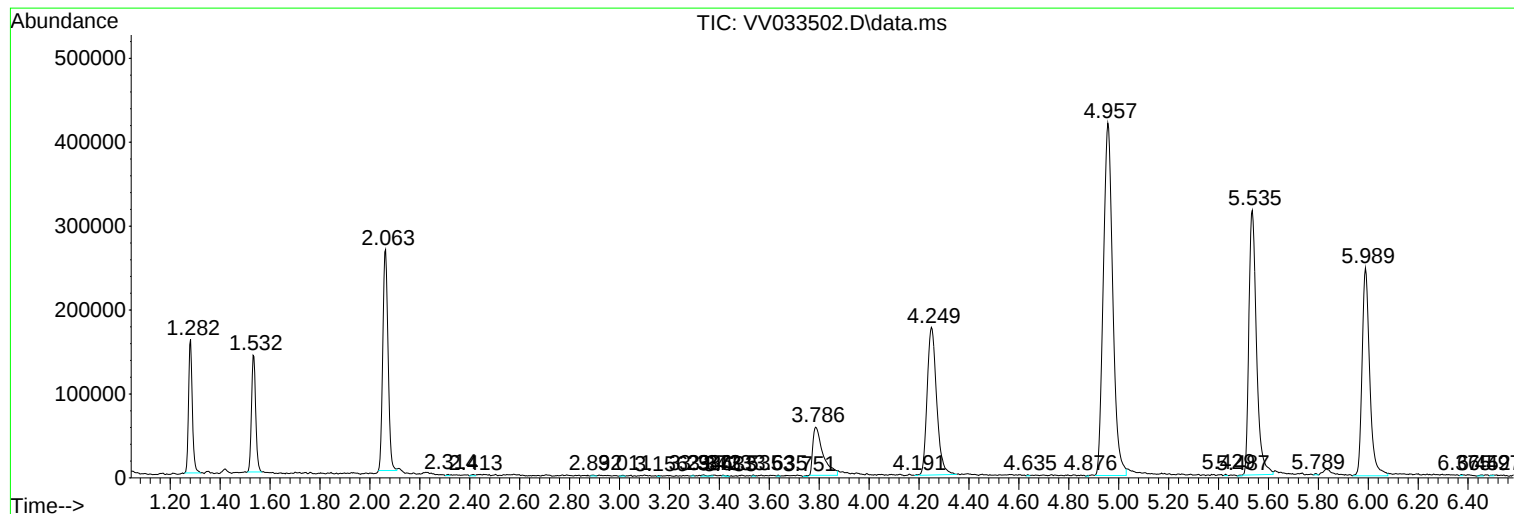

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033502.D
Acq On : 20 Dec 2023 11:28
Operator : SY/MD
Sample : 05927-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033502.D
Acq On : 20 Dec 2023 11:28
Operator : SY/MD
Sample : 05927-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc