

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033503.D
 Acq On : 20 Dec 2023 11:51
 Operator : SY/MD
 Sample : 05850-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	62	rBV5	3363	4050	0.35%	0.048%
2	1.282	68	75	86	rBV	172454	173992	15.11%	2.056%
3	1.536	147	154	165	rVB	141756	166702	14.48%	1.970%
4	2.063	308	318	330	rBV	278245	408258	35.46%	4.824%
5	2.407	421	425	426	rBV4	1289	731	0.06%	0.009%
6	2.452	432	439	440	rBV3	2244	2498	0.22%	0.030%
7	2.642	495	498	499	rVB	1463	639	0.06%	0.008%
8	2.671	504	507	508	rBV4	1406	581	0.05%	0.007%
9	2.825	551	555	557	rVV4	1153	996	0.09%	0.012%
10	2.847	560	562	566	rVV3	852	568	0.05%	0.007%
11	2.963	593	598	601	rBV4	1540	1301	0.11%	0.015%
12	3.034	618	620	622	rBV3	1172	648	0.06%	0.008%
13	3.117	644	646	652	rVB5	1582	1114	0.10%	0.013%
14	3.146	652	655	659	rBV5	1216	964	0.08%	0.011%
15	3.326	708	711	716	rBV6	1216	877	0.08%	0.010%
16	3.349	716	718	721	rVV4	798	535	0.05%	0.006%
17	3.400	729	734	737	rVB5	1386	1107	0.10%	0.013%
18	3.455	750	751	754	rBV3	834	545	0.05%	0.006%
19	3.510	764	768	771	rBV5	1529	816	0.07%	0.010%
20	3.558	780	783	785	rBV3	897	546	0.05%	0.006%
21	3.584	788	791	795	rBV4	981	784	0.07%	0.009%
22	3.670	814	818	822	rVB7	1406	1356	0.12%	0.016%
23	3.741	835	840	841	rBV6	960	853	0.07%	0.010%
24	3.786	844	854	876	rBV	55944	155992	13.55%	1.843%
25	4.249	979	998	1026	rBV	182814	485588	42.18%	5.738%
26	4.867	1188	1190	1192	rBV3	961	521	0.05%	0.006%
27	4.957	1202	1218	1249	rBV2	427129	1151316	100.00%	13.605%
28	5.452	1370	1372	1375	rVB3	983	572	0.05%	0.007%
29	5.535	1386	1398	1423	rBV	326449	685916	59.58%	8.105%
30	5.834	1484	1491	1499	rBV9	6158	11182	0.97%	0.132%
31	5.989	1527	1539	1566	rBV	254771	524650	45.57%	6.200%
32	6.346	1646	1650	1656	rBV8	1968	2106	0.18%	0.025%
33	6.503	1695	1699	1700	rBV4	1071	721	0.06%	0.009%
34	6.696	1756	1759	1762	rBV4	1195	905	0.08%	0.011%
35	6.857	1807	1809	1811	rBV3	1047	618	0.05%	0.007%
36	6.912	1817	1826	1849	rBV	121970	232233	20.17%	2.744%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033503.D
 Acq On : 20 Dec 2023 11:51
 Operator : SY/MD
 Sample : 05850-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.075	1875	1877	1880	rBV3	905	533	0.05%	0.006%
38	7.243	1918	1929	1955	rBV	489921	863354	74.99%	10.202%
39	7.555	2016	2026	2045	rBV	87195	161549	14.03%	1.909%
40	7.876	2118	2126	2133	rBV4	7261	10885	0.95%	0.129%
41	7.944	2144	2147	2149	rBV3	1062	703	0.06%	0.008%
42	7.985	2158	2160	2162	rBV3	980	552	0.05%	0.007%
43	8.024	2162	2172	2207	rBV	193522	413504	35.92%	4.886%
44	8.783	2397	2408	2431	rBV	537816	890175	77.32%	10.519%
45	9.162	2523	2526	2527	rBV4	1489	907	0.08%	0.011%
46	9.233	2545	2548	2551	rVB5	1285	814	0.07%	0.010%
47	9.542	2640	2644	2645	rBV4	1129	855	0.07%	0.010%
48	9.616	2665	2667	2672	rBV4	1467	880	0.08%	0.010%
49	9.648	2674	2677	2680	rVV4	1007	770	0.07%	0.009%
50	9.847	2735	2739	2743	rBV6	1451	1720	0.15%	0.020%
51	9.866	2743	2745	2747	rVV2	1163	685	0.06%	0.008%
52	9.876	2747	2748	2752	rVV5	1857	942	0.08%	0.011%
53	9.892	2752	2753	2757	rVB5	1322	679	0.06%	0.008%
54	9.979	2778	2780	2784	rVB4	863	599	0.05%	0.007%
55	10.037	2796	2798	2800	rVB3	1231	602	0.05%	0.007%
56	10.046	2800	2801	2804	rBV3	1233	701	0.06%	0.008%
57	10.111	2818	2821	2822	rBV	1886	850	0.07%	0.010%
58	10.153	2823	2834	2858	rVB	312507	500908	43.51%	5.919%
59	10.326	2881	2888	2899	rVB2	9692	15622	1.36%	0.185%
60	10.390	2904	2908	2909	rBV3	1672	913	0.08%	0.011%
61	10.435	2920	2922	2926	rVB4	1011	569	0.05%	0.007%
62	10.506	2942	2944	2947	rBV3	754	551	0.05%	0.007%
63	10.545	2954	2956	2960	rVB4	1116	663	0.06%	0.008%
64	10.664	2989	2993	2994	rBV3	1122	845	0.07%	0.010%
65	10.751	3018	3020	3023	rBV4	1070	564	0.05%	0.007%
66	10.911	3068	3070	3073	rVB4	1520	702	0.06%	0.008%
67	11.027	3103	3106	3109	rVB4	1007	556	0.05%	0.007%
68	11.120	3130	3135	3136	rBV3	1927	1363	0.12%	0.016%
69	11.185	3144	3155	3172	rBV	498312	767552	66.67%	9.070%
70	11.468	3241	3243	3249	rBV5	1618	1204	0.10%	0.014%
71	11.561	3261	3272	3293	rBV	491742	770071	66.89%	9.100%
72	11.908	3378	3380	3382	rBV3	998	629	0.05%	0.007%
73	11.924	3382	3385	3386	rBV3	981	570	0.05%	0.007%
74	12.448	3545	3548	3549	rBV2	1025	545	0.05%	0.006%
75	12.522	3568	3571	3574	rBV4	1242	666	0.06%	0.008%
76	12.567	3583	3585	3588	rBV4	845	558	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033503.D
 Acq On : 20 Dec 2023 11:51
 Operator : SY/MD
 Sample : 05850-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.693	3621	3624	3628	rVB4	1498	1001	0.09%	0.012%
78	12.725	3631	3634	3635	rBV2	1550	809	0.07%	0.010%
79	12.763	3643	3646	3651	rBV6	1174	1219	0.11%	0.014%
80	12.908	3688	3691	3694	rVB4	1479	821	0.07%	0.010%
81	13.021	3724	3726	3728	rBV3	1001	556	0.05%	0.007%
82	13.056	3732	3737	3741	rBV7	1236	1588	0.14%	0.019%
83	13.345	3824	3827	3831	rBV6	994	671	0.06%	0.008%
84	13.368	3831	3834	3836	rBV4	1127	791	0.07%	0.009%
85	13.406	3841	3846	3850	rBV6	1281	1148	0.10%	0.014%
86	13.750	3951	3953	3957	rBV5	1013	581	0.05%	0.007%
87	13.786	3962	3964	3968	rBV4	1312	1027	0.09%	0.012%
88	13.812	3970	3972	3974	rVB3	1632	523	0.05%	0.006%
89	13.982	4023	4025	4028	rBV3	1168	916	0.08%	0.011%
90	14.120	4064	4068	4071	rVB5	1182	776	0.07%	0.009%
91	14.265	4108	4113	4115	rBV5	966	748	0.06%	0.009%
92	14.532	4194	4196	4201	rBV5	1099	828	0.07%	0.010%
93	14.660	4232	4236	4238	rBV4	1699	1258	0.11%	0.015%
94	14.767	4265	4269	4272	rBV4	935	852	0.07%	0.010%
95	14.821	4282	4286	4287	rBV3	1256	861	0.07%	0.010%
96	15.017	4345	4347	4351	rBV6	992	789	0.07%	0.009%
97	15.046	4351	4356	4359	rVB6	1490	1329	0.12%	0.016%
98	15.069	4359	4363	4365	rBV4	1509	1164	0.10%	0.014%
99	15.316	4436	4440	4443	rBV6	1519	1295	0.11%	0.015%
100	15.503	4496	4498	4503	rBV5	1382	878	0.08%	0.010%




Sum of corrected areas: 8462520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033503.D
Acq On : 20 Dec 2023 11:51
Operator : SY/MD
Sample : 05850-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

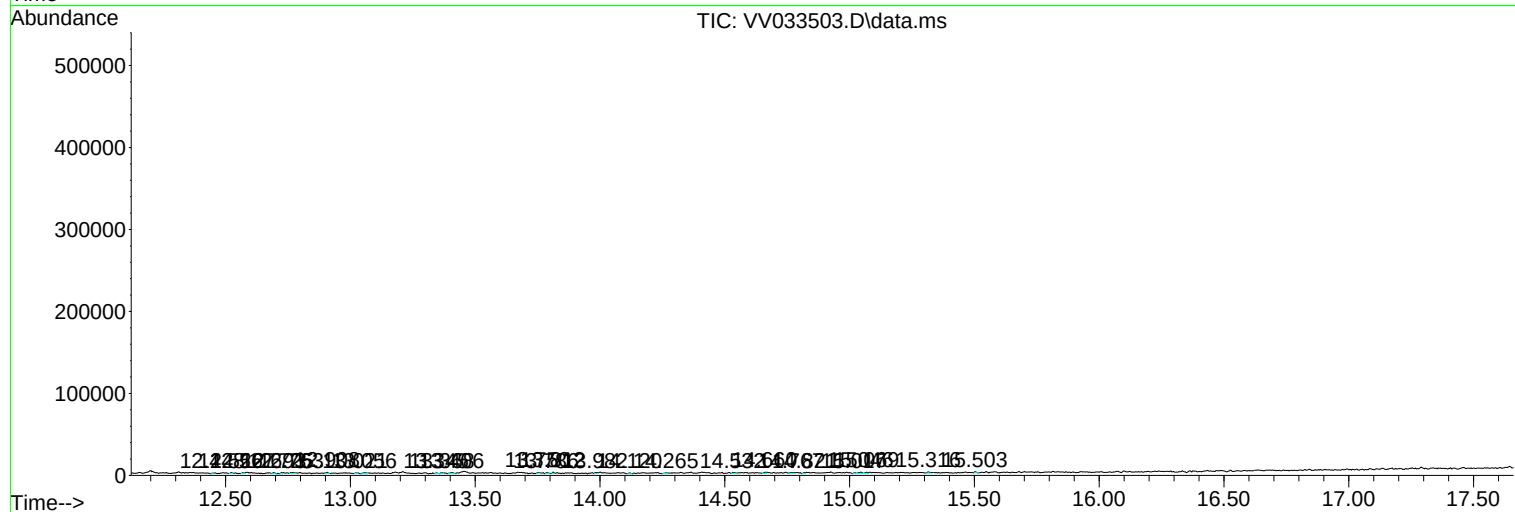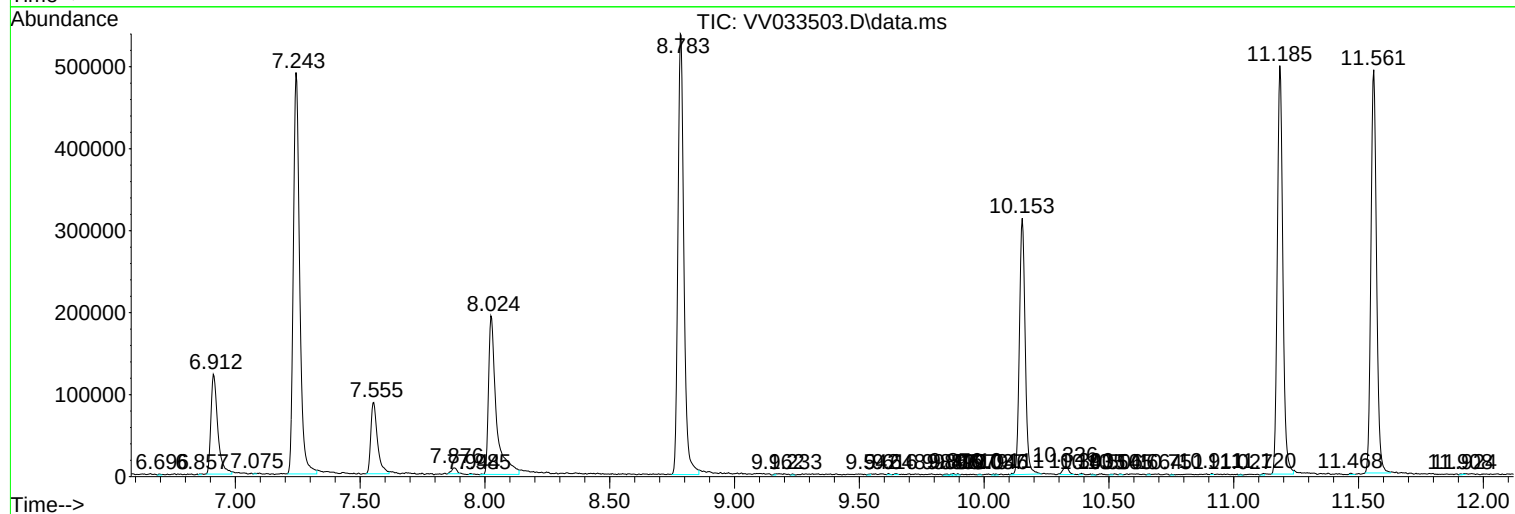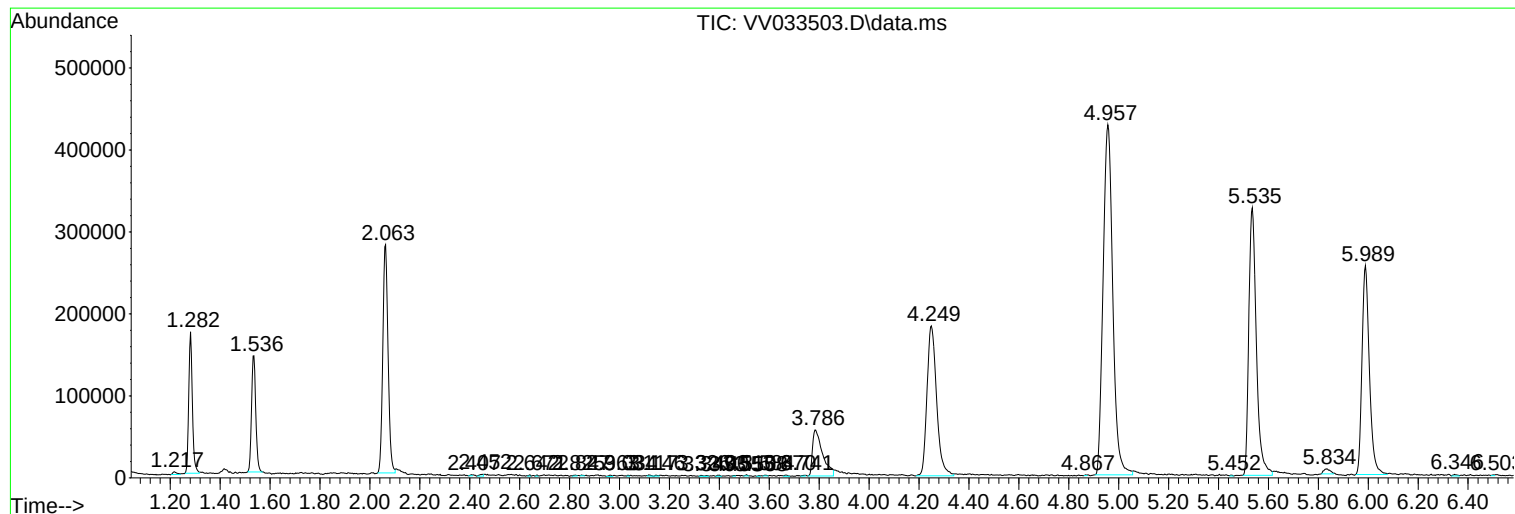

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033503.D
Acq On : 20 Dec 2023 11:51
Operator : SY/MD
Sample : 05850-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033503.D
Acq On : 20 Dec 2023 11:51
Operator : SY/MD
Sample : 05850-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc